

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091520\
 Data File : P0071346.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Sep 2020 12:40
 Operator : DD\AJ
 Sample : PB131614BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB131614BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 13:47:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.343	3.527	1913272	976465	26.998	25.011
2)	SA Decachlor...	9.954	8.705	2062739	1102248	22.119	20.010
Target Compounds							
16)	L4 AR-1242-1	5.616f	0.000	5424	0	2.318	N.D. #
20)	L4 AR-1242-5	6.631f	0.000	12627	0	5.691	N.D. #
25)	L5 AR-1248-5	6.631f	0.000	12627	0	3.795	N.D. #
27)	L6 AR-1254-2	6.773	0.000	3663	0	0.637	N.D. #
30)	L6 AR-1254-5	7.839f	0.000	124625	0	22.341	N.D. #
35)	L7 AR-1260-5	8.454f	0.000	18471	0	1.457	N.D. #
37)	L8 AR-1262-2	8.454f	0.000	18471	0	1.280	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091520\
Data File : PO071346.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Sep 2020 12:40
Operator : DD\AJ
Sample : PB131614BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB131614BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 13:47:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

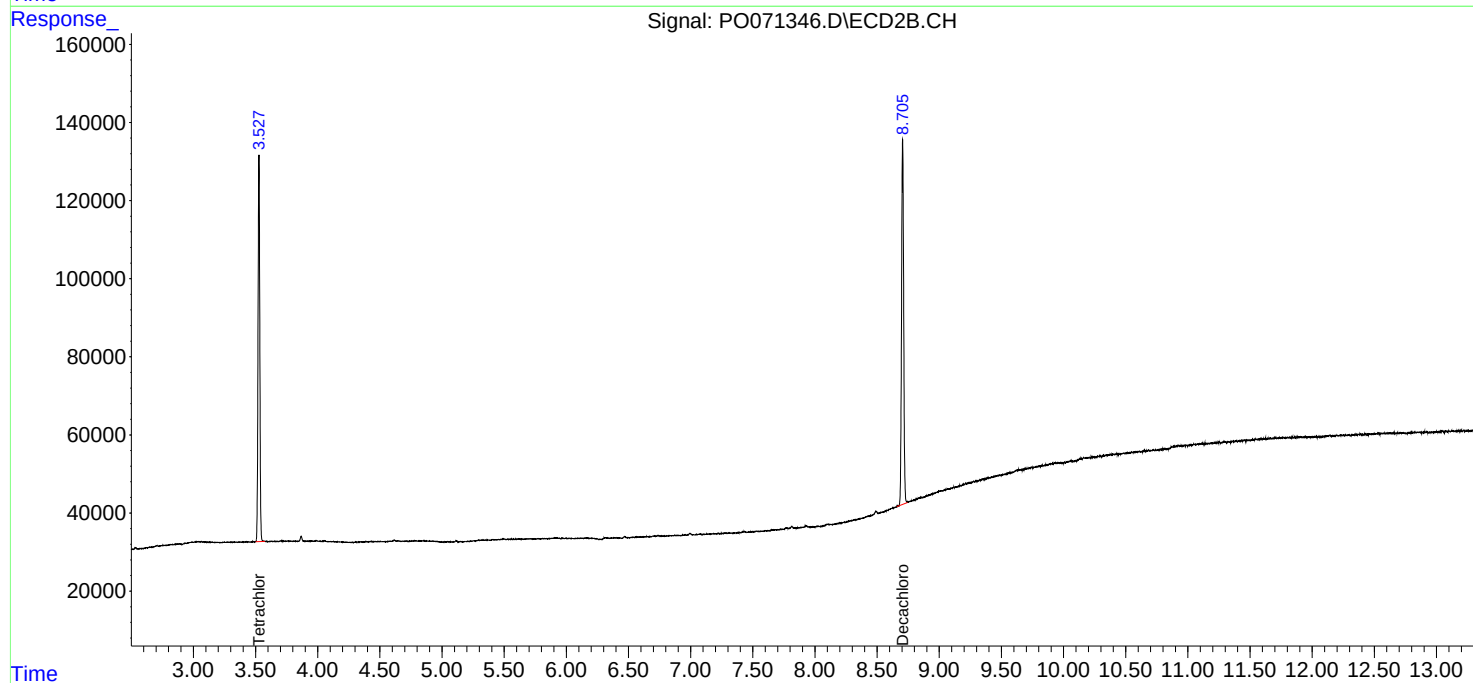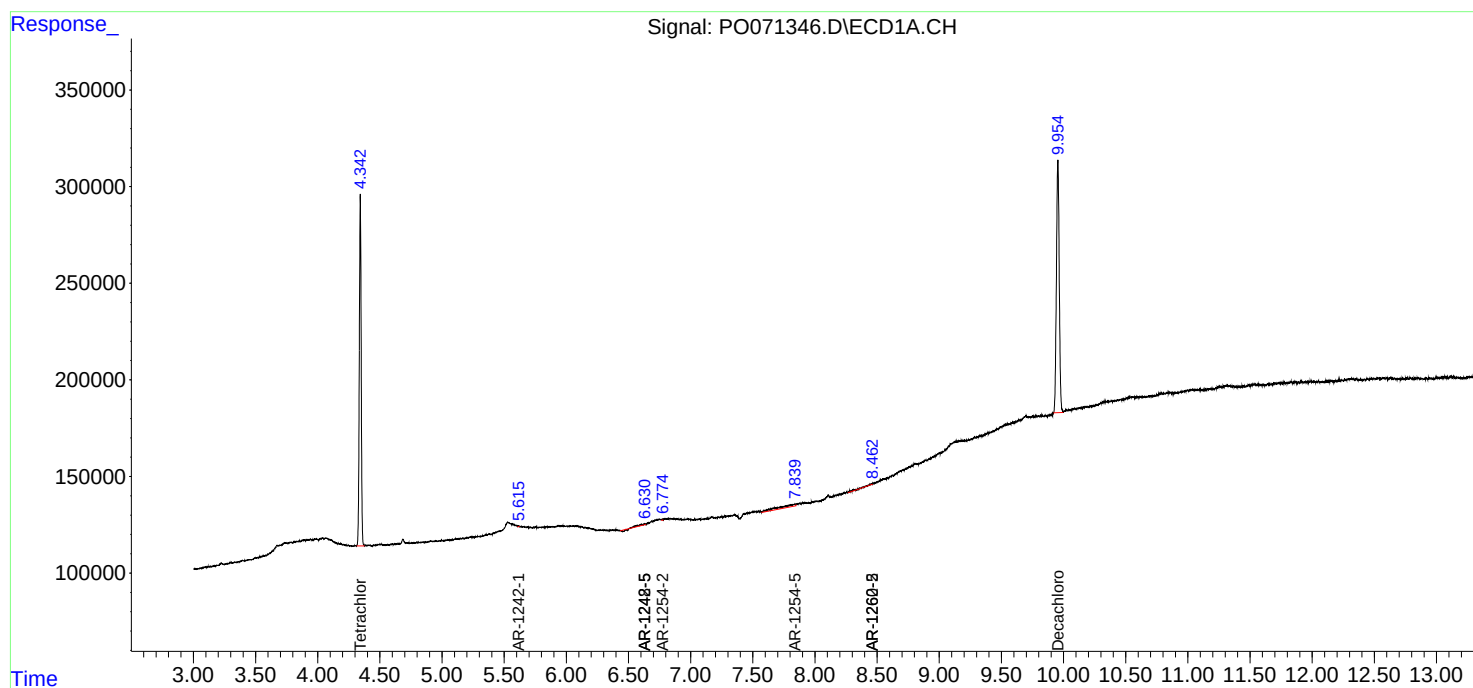


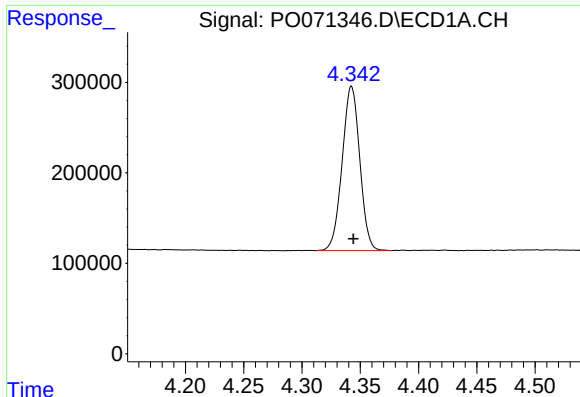

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: -0.001 min
Response: 1913272
Conc: 27.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB131614BL

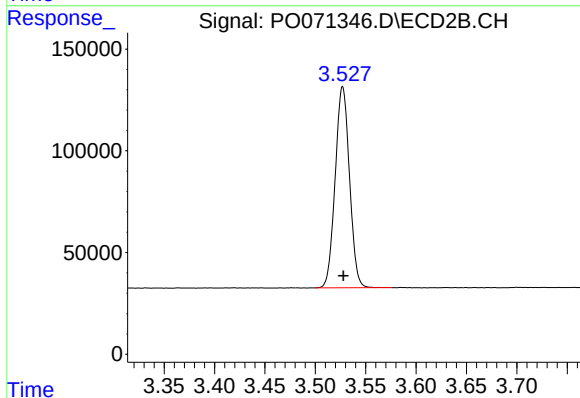


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 976465
Conc: 25.01 ng/ml

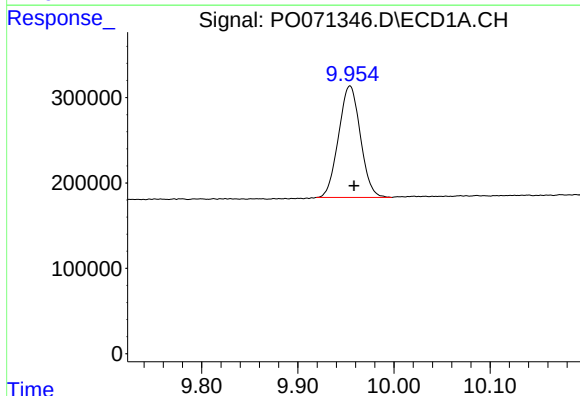


#2 Decachlorobiphenyl

R.T.: 9.954 min
Delta R.T.: -0.004 min
Response: 2062739
Conc: 22.12 ng/ml

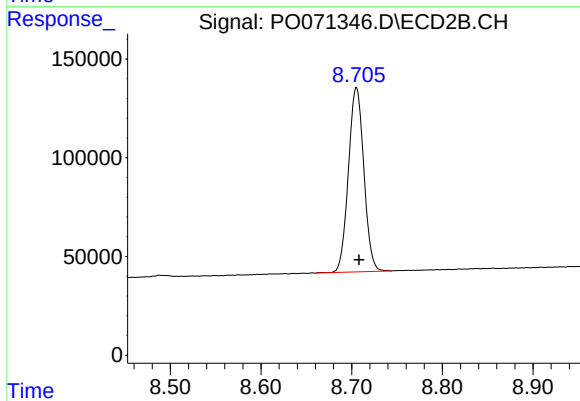

#2 Decachlorobiphenyl


R.T.: 8.705 min
Delta R.T.: -0.003 min
Response: 1102248
Conc: 20.01 ng/ml

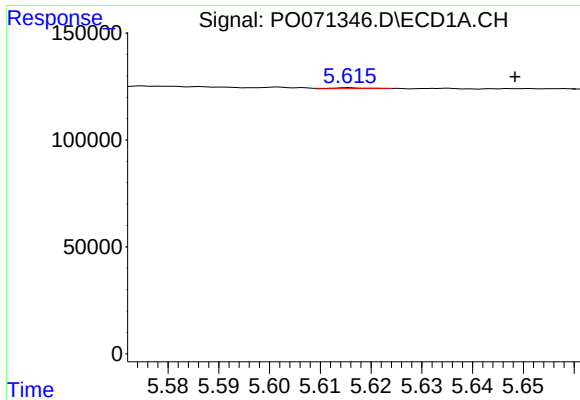

#16 AR-1242-1


R.T.: 5.616 min
Delta R.T.: -0.033 min
Response: 5424
Conc: 2.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB131614BL

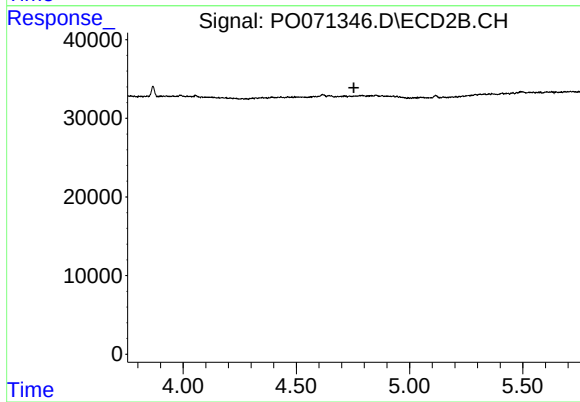


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.754 min
Response: 0
Conc: N.D.

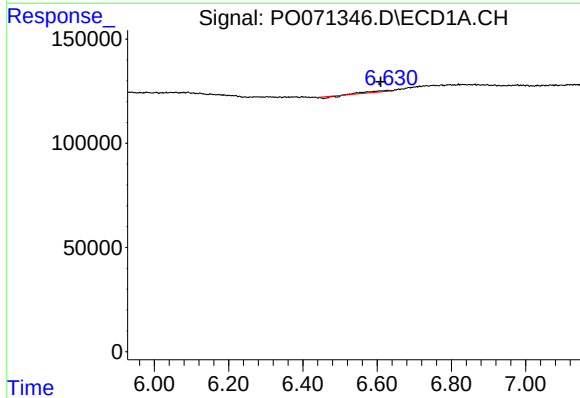


#20 AR-1242-5

R.T.: 6.631 min
Delta R.T.: 0.021 min
Response: 12627
Conc: 5.69 ng/ml

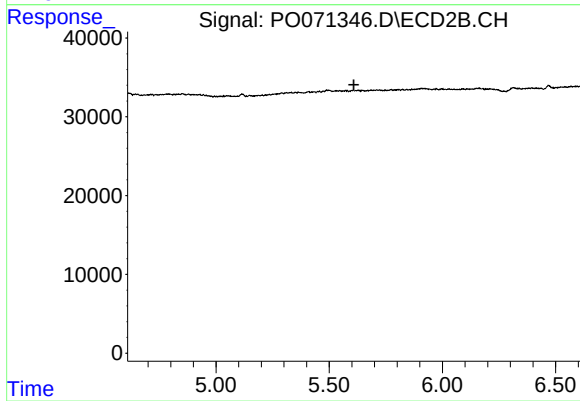

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.609 min
Response: 0
Conc: N.D.

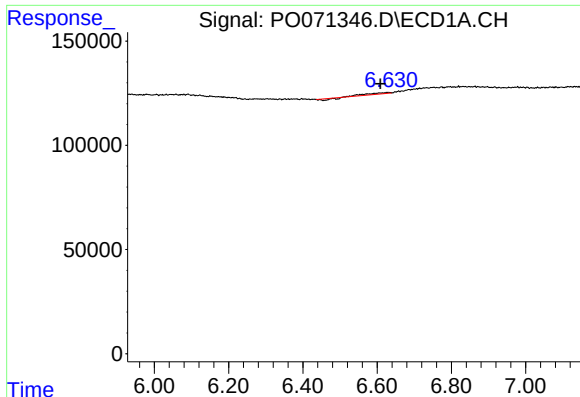

#25 AR-1248-5


R.T.: 6.631 min
Delta R.T.: 0.022 min
Response: 12627
Conc: 3.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB131614BL

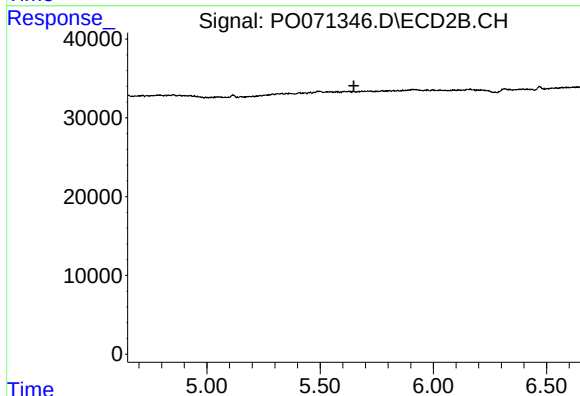


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.649 min
Response: 0
Conc: N.D.

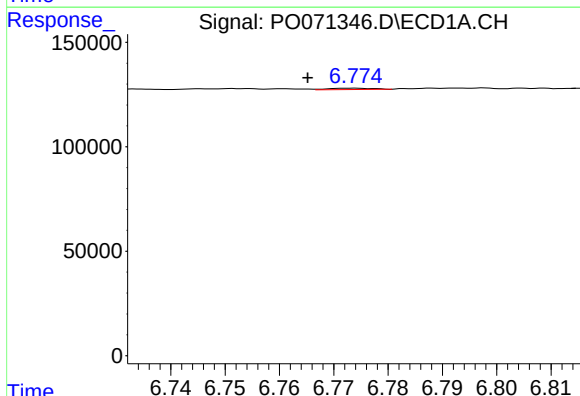


#27 AR-1254-2

R.T.: 6.773 min
Delta R.T.: 0.008 min
Response: 3663
Conc: 0.64 ng/ml

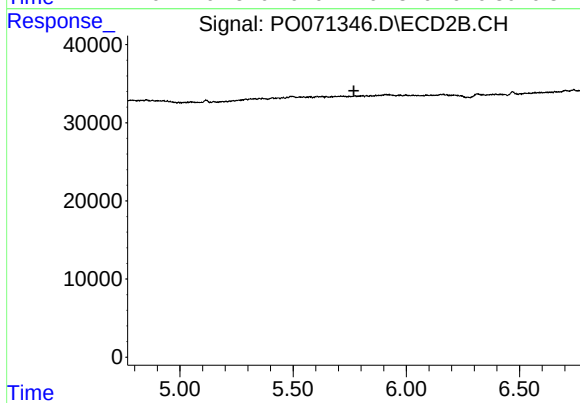

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 5.768 min
Response: 0
Conc: N.D.

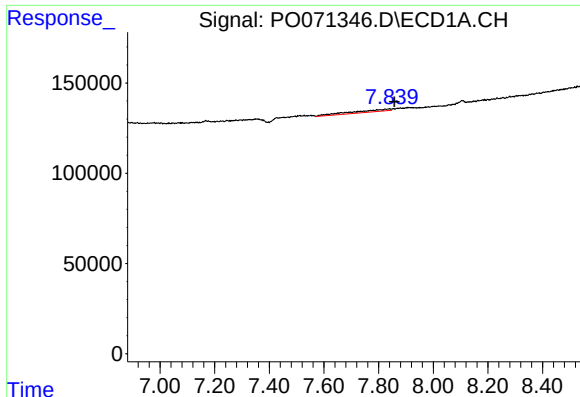

#30 AR-1254-5


R.T.: 7.839 min
Delta R.T.: -0.018 min
Response: 124625
Conc: 22.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB131614BL

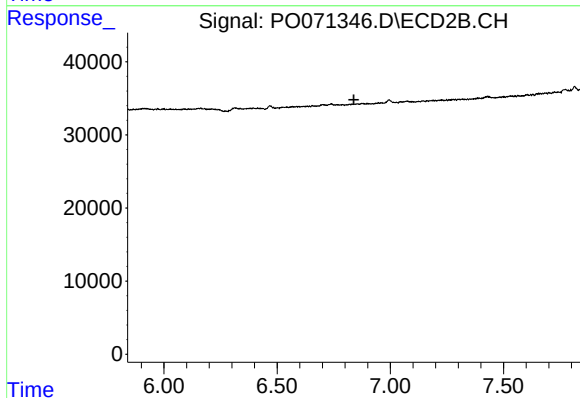


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.839 min
Response: 0
Conc: N.D.

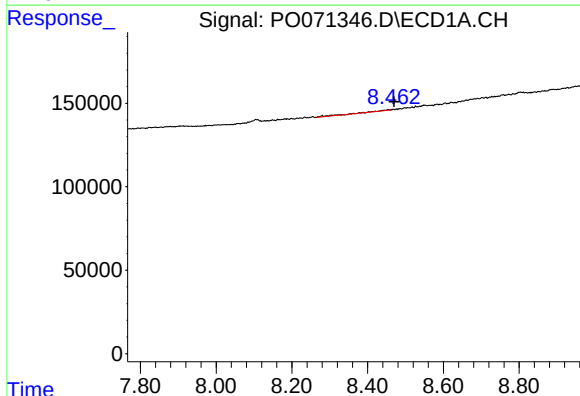


#35 AR-1260-5

R.T.: 8.454 min
Delta R.T.: -0.016 min
Response: 18471
Conc: 1.46 ng/ml

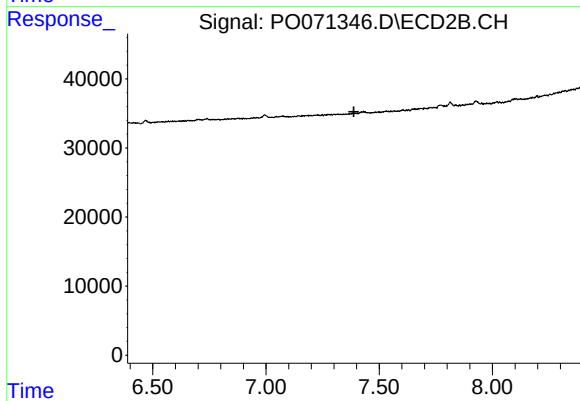

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

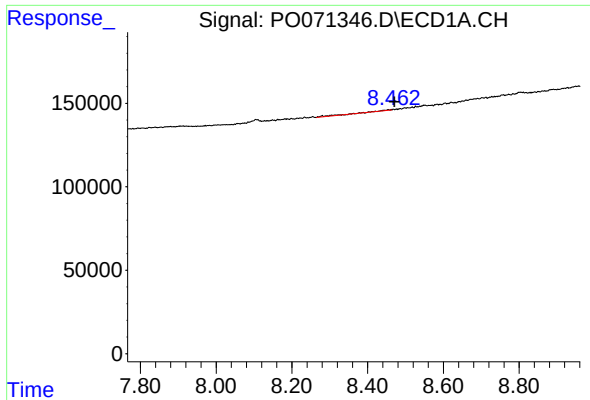

#37 AR-1262-2

R.T.: 8.454 min
Delta R.T.: -0.017 min
Response: 18471
Conc: 1.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB131614BL

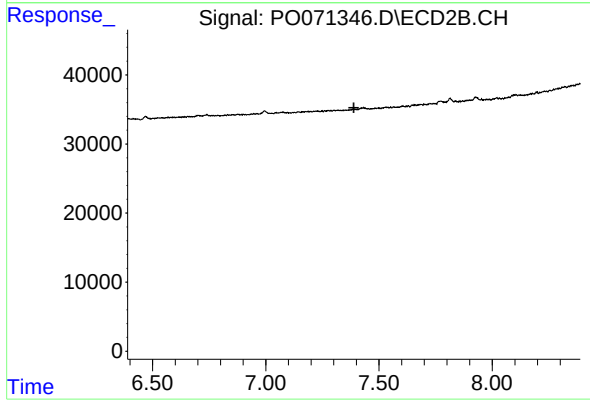

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.