

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091520\
 Data File : P0071355.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Sep 2020 15:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 16:49:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.346	3.530	1625699	994884	22.940	25.483
2)	SA Decachlor...	9.958	8.709	1625940	871276	17.436	15.817
Target Compounds							
20)	L4 AR-1242-5	0.000	5.628f	0	57382	N.D.	41.464 #
24)	L5 AR-1248-4	6.552f	0.000	128484	0	35.357	N.D. #
25)	L5 AR-1248-5	0.000	5.628f	0	57382	N.D.	33.479 #
26)	L6 AR-1254-1	6.552	5.628f	128484	57382	36.622	21.572 #
35)	L7 AR-1260-5	8.477	0.000	70471	0	5.557	N.D. #
37)	L8 AR-1262-2	8.477	0.000	70471	0	4.882	N.D. #
39)	L8 AR-1262-4	8.810	0.000	89854	0	14.132	N.D. #
42)	L9 AR-1268-2	8.810	0.000	89854	0	6.427	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091520\
Data File : P0071355.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Sep 2020 15:13
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 16:49:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

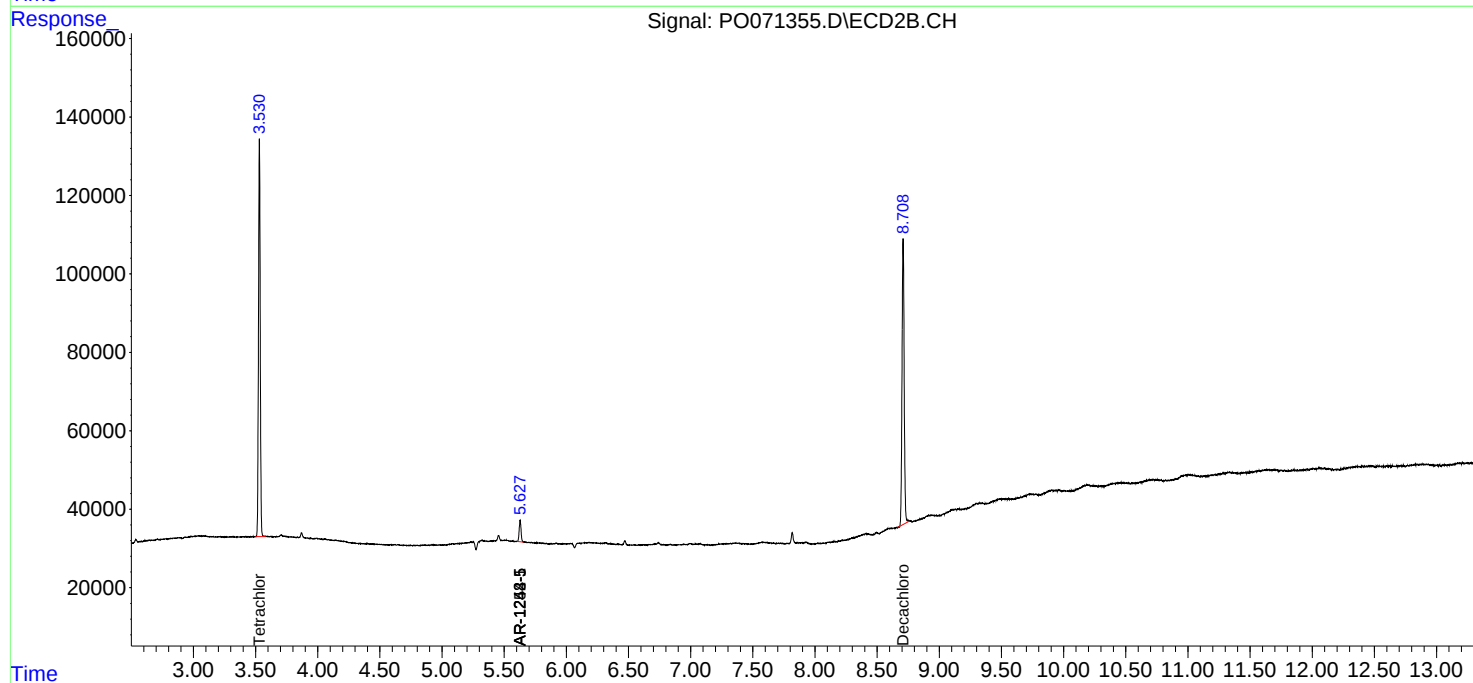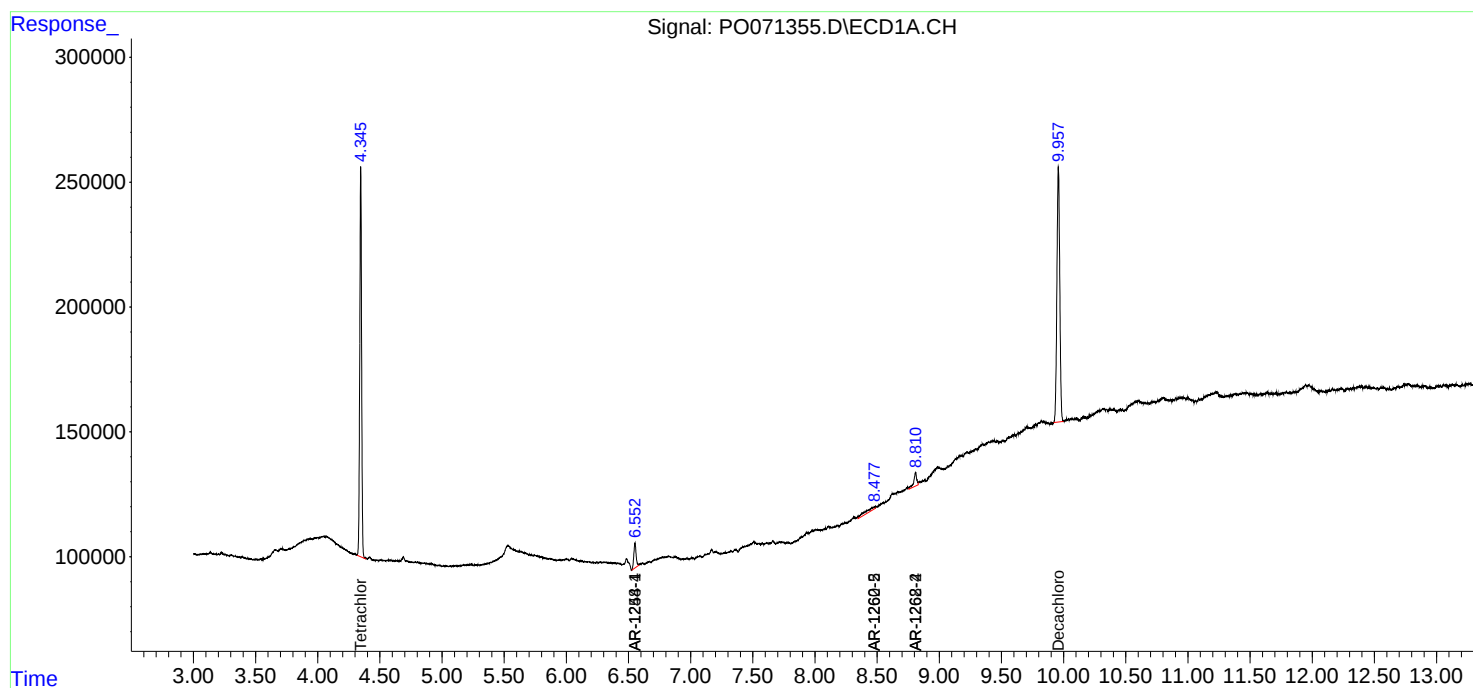


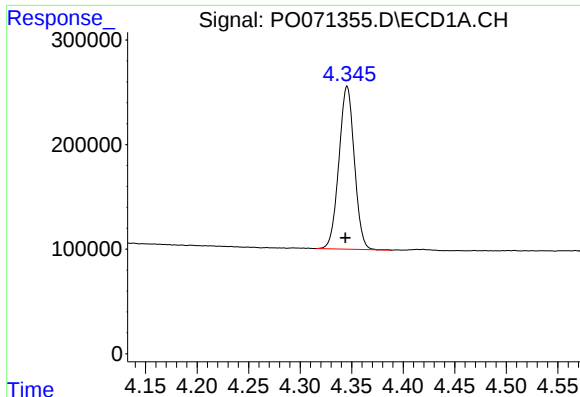

#1 Tetrachloro-m-xylene


R.T.: 4.346 min
Delta R.T.: 0.002 min
Response: 1625699
Conc: 22.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

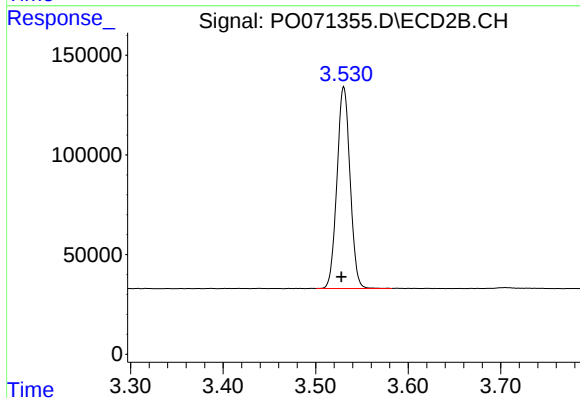


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: 0.002 min
Response: 994884
Conc: 25.48 ng/ml

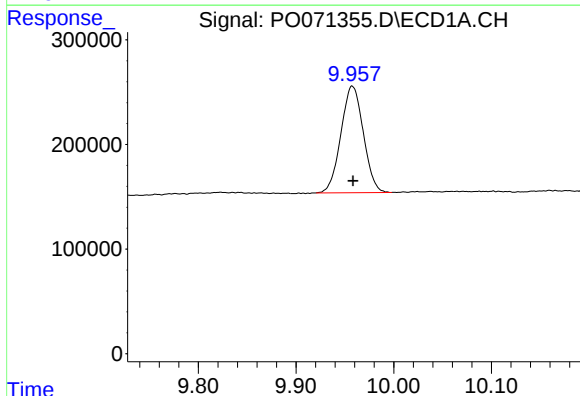


#2 Decachlorobiphenyl

R.T.: 9.958 min
Delta R.T.: 0.000 min
Response: 1625940
Conc: 17.44 ng/ml

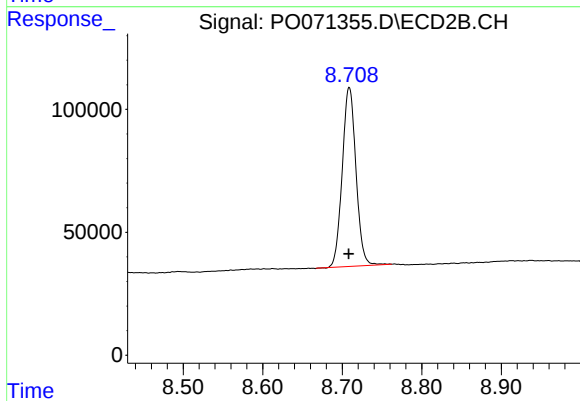

#2 Decachlorobiphenyl


R.T.: 8.709 min
Delta R.T.: 0.000 min
Response: 871276
Conc: 15.82 ng/ml

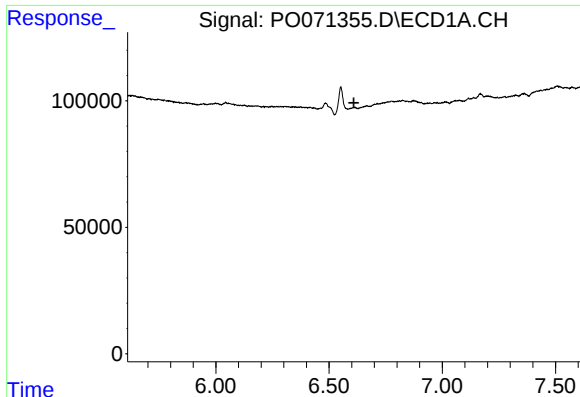

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.609 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

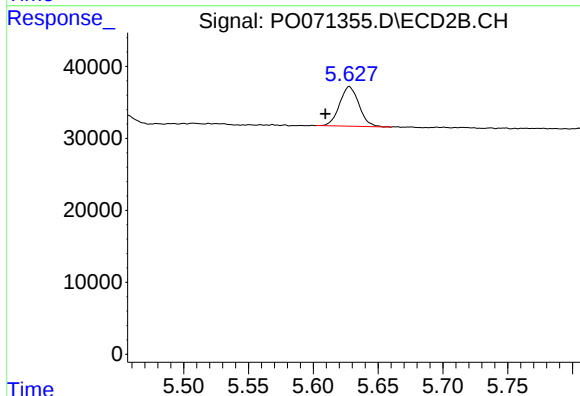


#20 AR-1242-5

R.T.: 5.628 min
Delta R.T.: 0.018 min
Response: 57382
Conc: 41.46 ng/ml

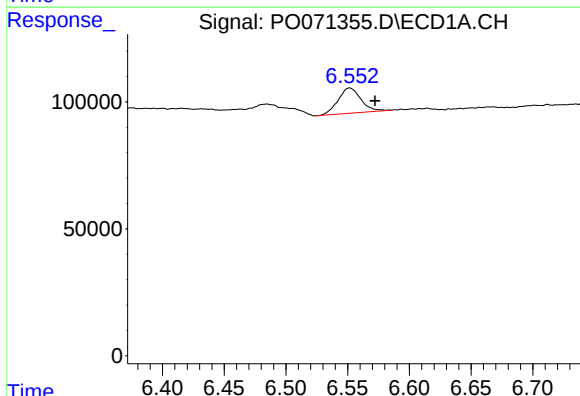


#24 AR-1248-4

R.T.: 6.552 min
Delta R.T.: -0.020 min
Response: 128484
Conc: 35.36 ng/ml

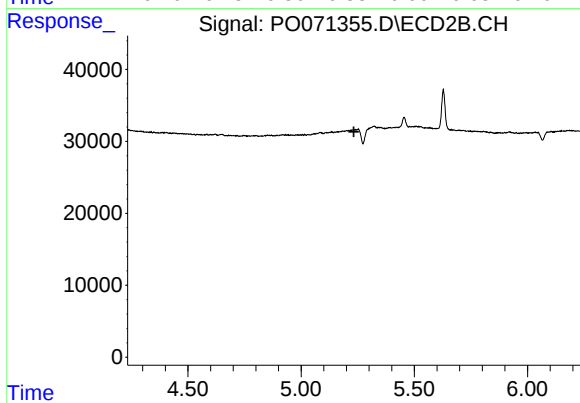

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.233 min
Response: 0
Conc: N.D.

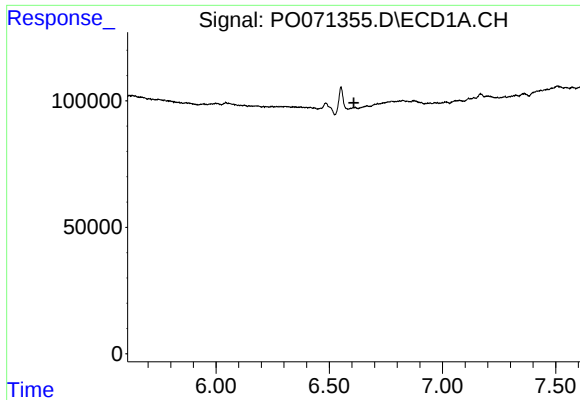

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.609 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

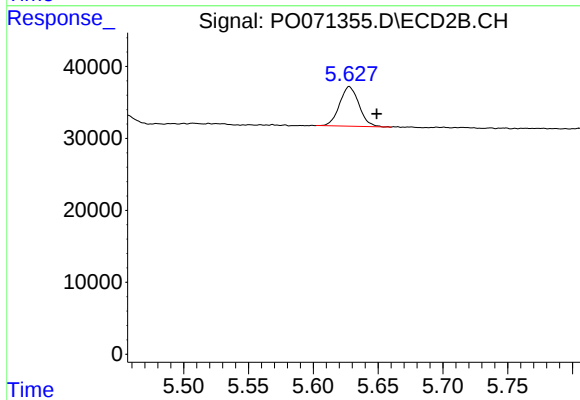


#25 AR-1248-5

R.T.: 5.628 min
Delta R.T.: -0.021 min
Response: 57382
Conc: 33.48 ng/ml

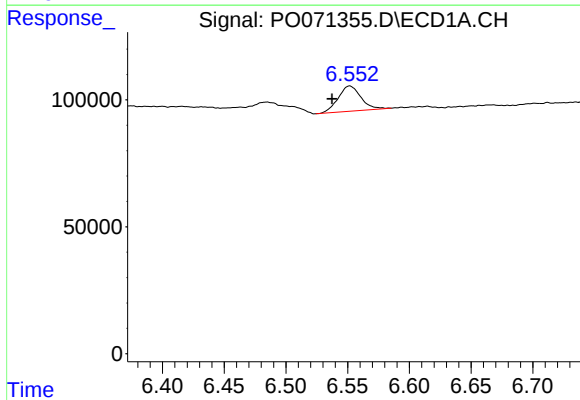


#26 AR-1254-1

R.T.: 6.552 min
Delta R.T.: 0.014 min
Response: 128484
Conc: 36.62 ng/ml

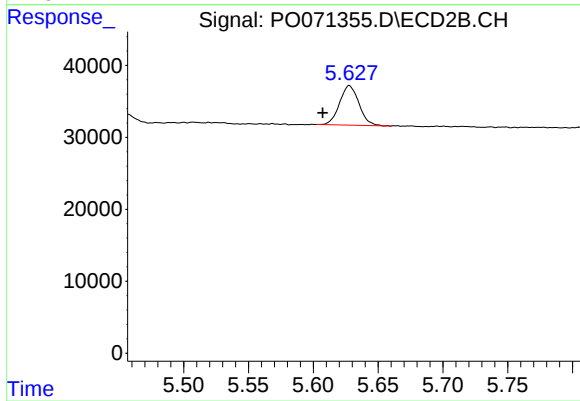

#26 AR-1254-1


R.T.: 5.628 min
Delta R.T.: 0.021 min
Response: 57382
Conc: 21.57 ng/ml

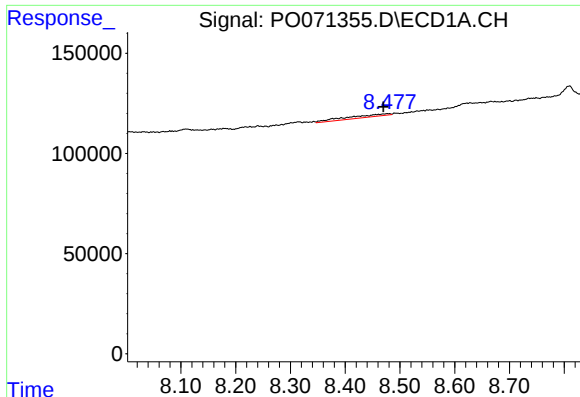

#35 AR-1260-5


R.T.: 8.477 min
Delta R.T.: 0.007 min
Response: 70471
Conc: 5.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

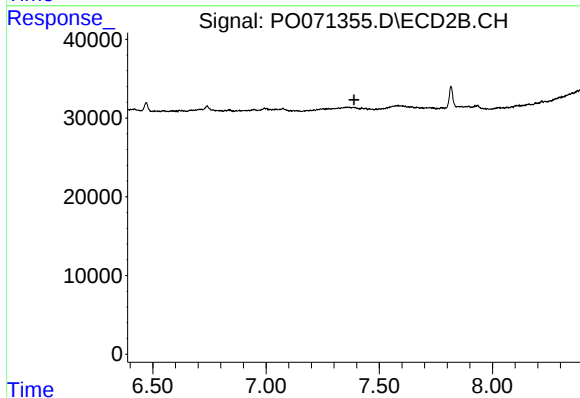


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

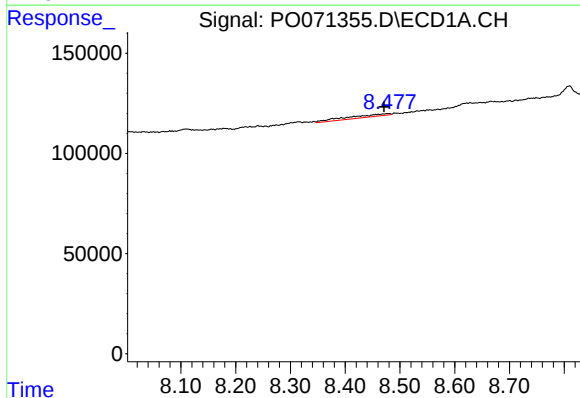


#37 AR-1262-2

R.T.: 8.477 min
Delta R.T.: 0.006 min
Response: 70471
Conc: 4.88 ng/ml

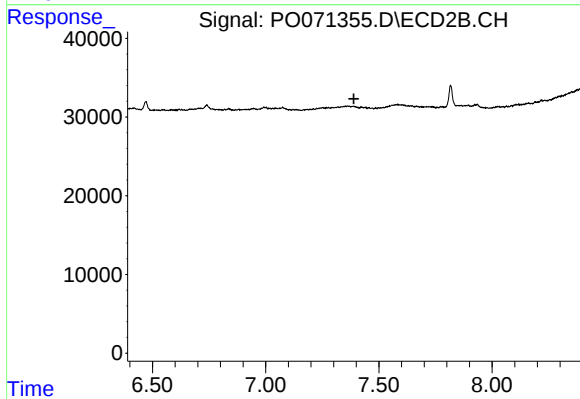

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

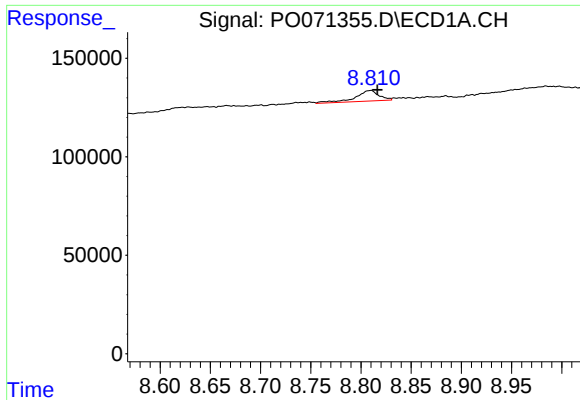

#39 AR-1262-4


R.T.: 8.810 min
Delta R.T.: -0.007 min
Response: 89854
Conc: 14.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

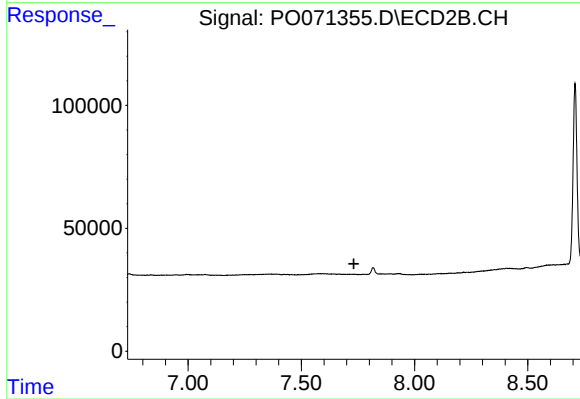


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.732 min
Response: 0
Conc: N.D.

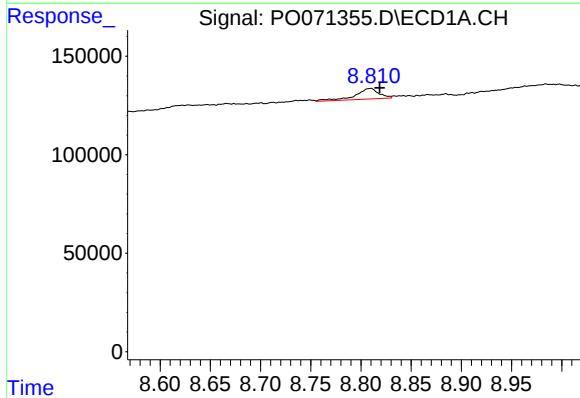

#42 AR-1268-2

R.T.: 8.810 min
Delta R.T.: -0.009 min
Response: 89854
Conc: 6.43 ng/ml

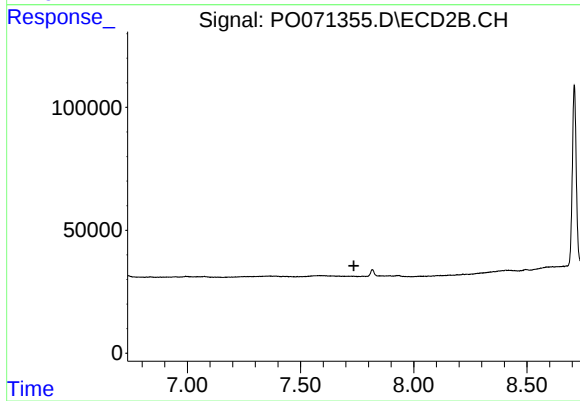

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.735 min
Response: 0
Conc: N.D.