

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091520\
 Data File : P0071364.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Sep 2020 18:23
 Operator : DD\AJ
 Sample : L4013-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAV-B40-091420-10-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 05:15:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.528	1746475	935939	24.644	23.973
2) SA Decachlor...	9.958	8.707	1551757	848538	16.640	15.404
Target Compounds						
19) L4 AR-1242-4	5.883f	0.000	69131	0	40.802	N.D. #
34) L7 AR-1260-4	8.156	0.000	17192	0	3.003	N.D. #
35) L7 AR-1260-5	8.491f	0.000	6324	0	0.499	N.D. #
37) L8 AR-1262-2	8.491f	0.000	6324	0	0.438	N.D. #
39) L8 AR-1262-4	8.808	0.000	36895	0	5.803	N.D. #
42) L9 AR-1268-2	8.808	0.000	36895	0	2.639	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091520\
Data File : P0071364.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Sep 2020 18:23
Operator : DD\AJ
Sample : L4013-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PAV-B40-091420-10-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 05:15:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

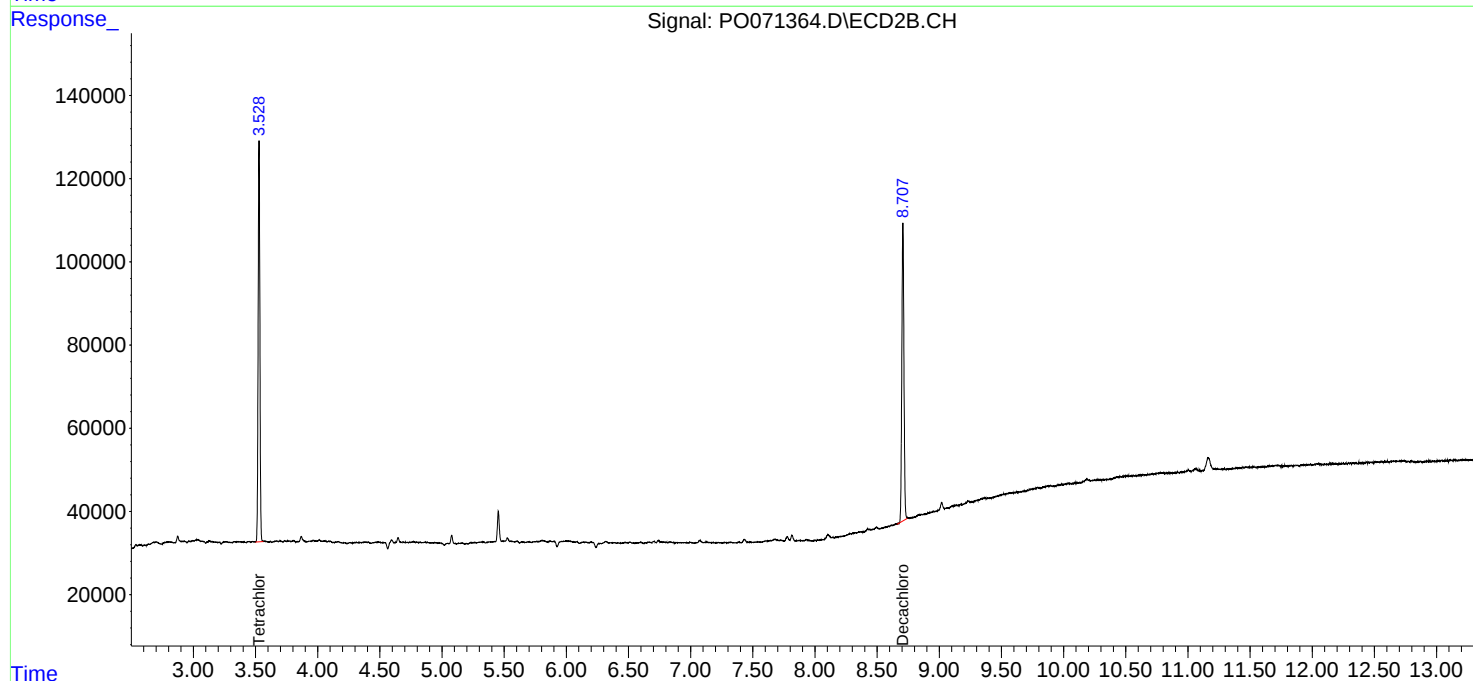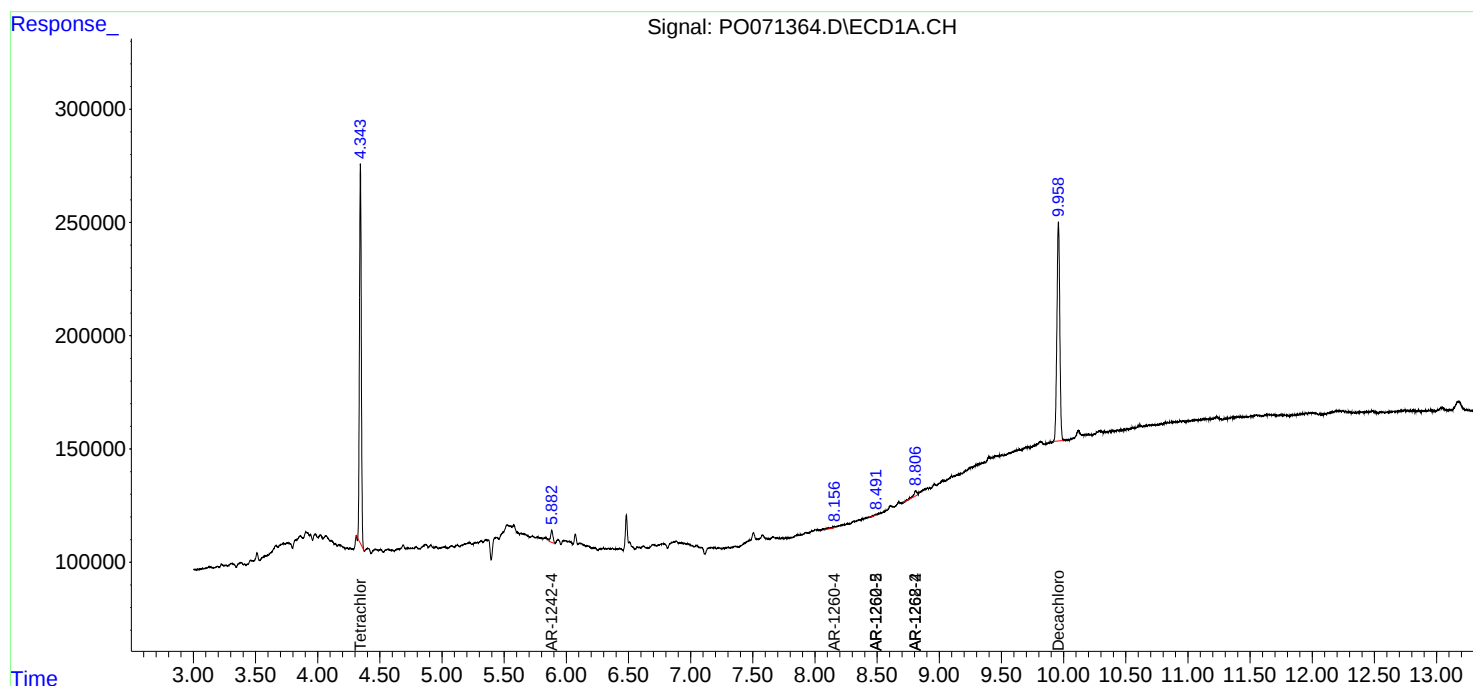


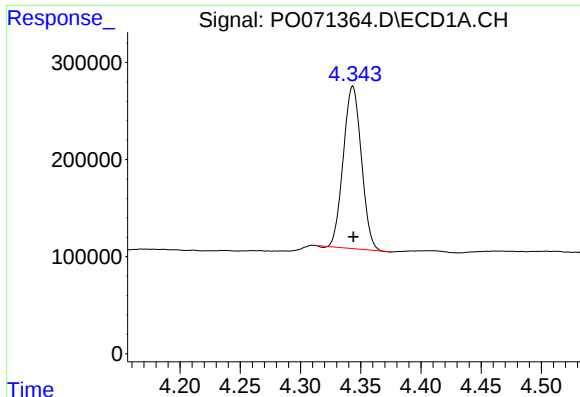

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 1746475
Conc: 24.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAV-B40-091420-10-15

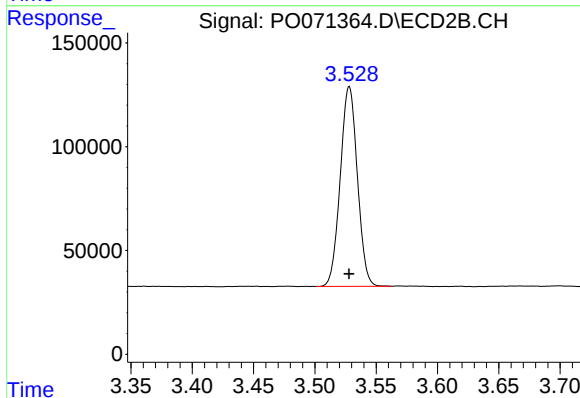


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 935939
Conc: 23.97 ng/ml

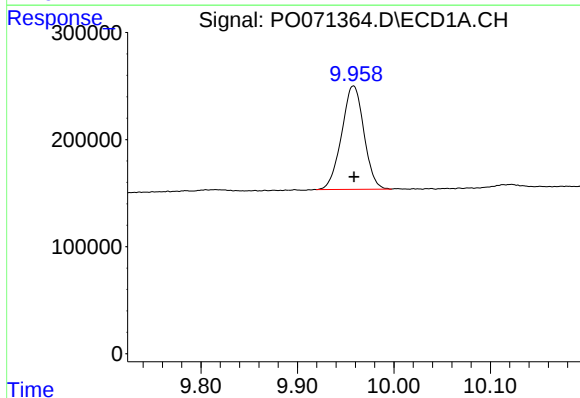


#2 Decachlorobiphenyl

R.T.: 9.958 min
Delta R.T.: 0.000 min
Response: 1551757
Conc: 16.64 ng/ml

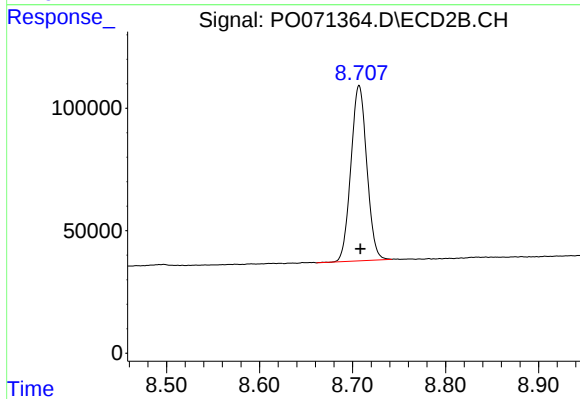

#2 Decachlorobiphenyl


R.T.: 8.707 min
Delta R.T.: -0.001 min
Response: 848538
Conc: 15.40 ng/ml

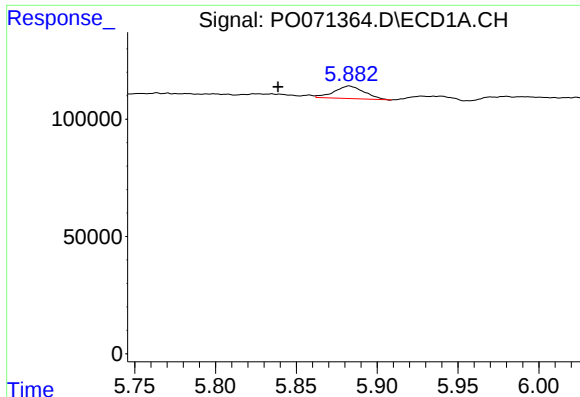

#19 AR-1242-4


R.T.: 5.883 min
Delta R.T.: 0.044 min
Response: 69131
Conc: 40.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAV-B40-091420-10-15

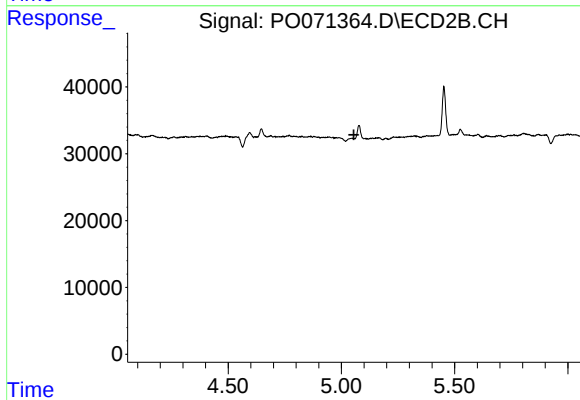


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.055 min
Response: 0
Conc: N.D.

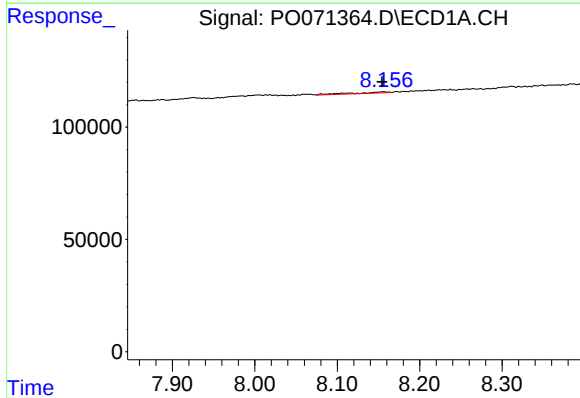


#34 AR-1260-4

R.T.: 8.156 min
Delta R.T.: 0.001 min
Response: 17192
Conc: 3.00 ng/ml

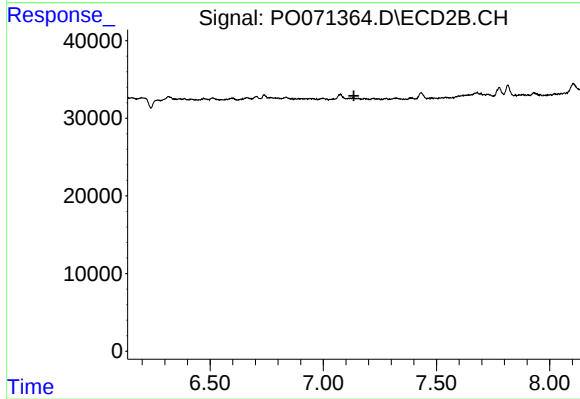

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.135 min
Response: 0
Conc: N.D.

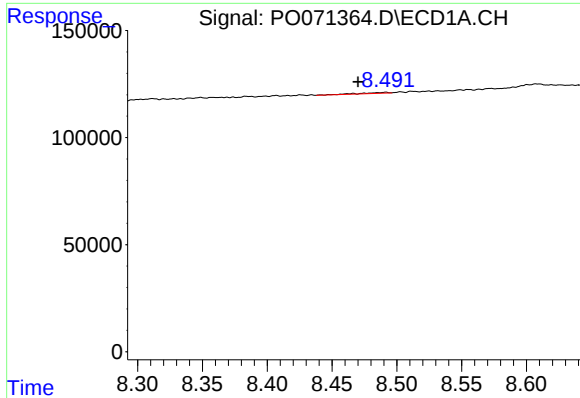

#35 AR-1260-5


R.T.: 8.491 min
Delta R.T.: 0.021 min
Response: 6324
Conc: 0.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAV-B40-091420-10-15

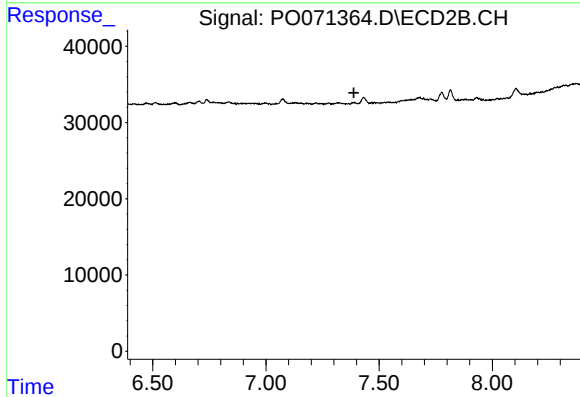


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

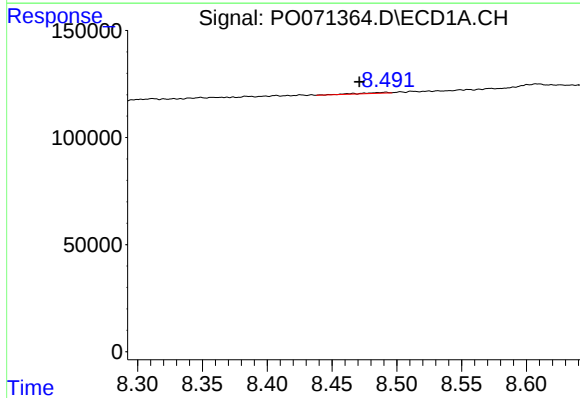


#37 AR-1262-2

R.T.: 8.491 min
Delta R.T.: 0.020 min
Response: 6324
Conc: 0.44 ng/ml

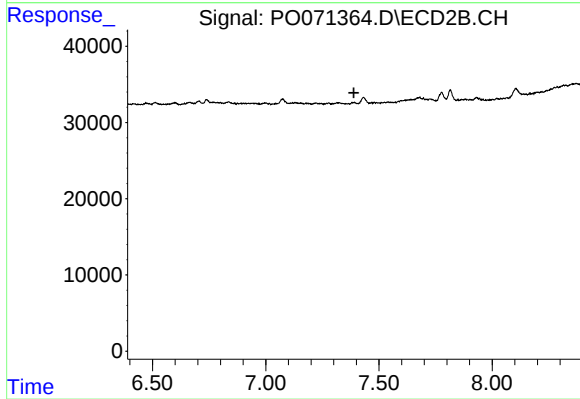

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

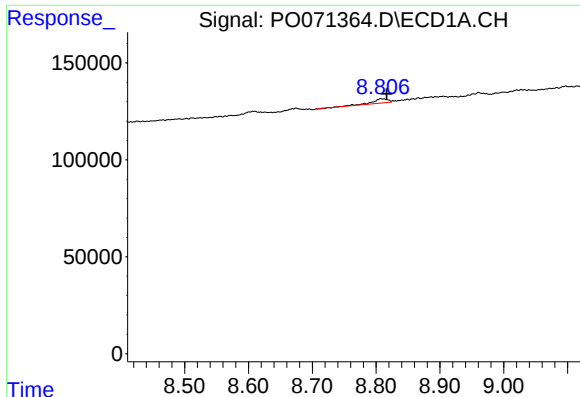

#39 AR-1262-4


R.T.: 8.808 min
Delta R.T.: -0.009 min
Response: 36895
Conc: 5.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAV-B40-091420-10-15

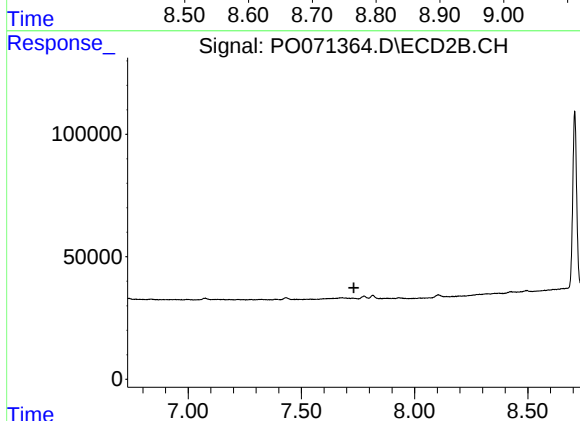


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.732 min
Response: 0
Conc: N.D.

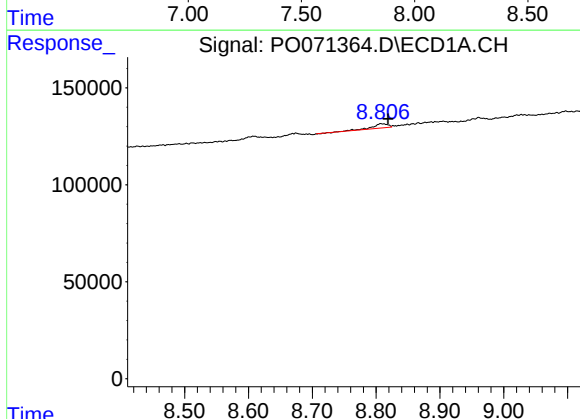

#42 AR-1268-2

R.T.: 8.808 min
Delta R.T.: -0.011 min
Response: 36895
Conc: 2.64 ng/ml

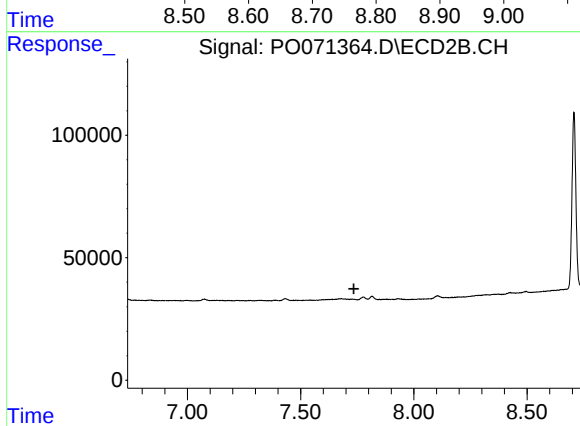

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.735 min
Response: 0
Conc: N.D.