

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091520\
 Data File : P0071342.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Sep 2020 10:37
 Operator : DD\AJ
 Sample : L3981-09RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B19-7-9RE

Manual Integrations
 APPROVED

Ankita
 9/16/2020 1:55:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 13:46:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.529	2000381	945657	28.227m	24.222m
2) SA Decachlor...	9.956	8.706	4746573	2397222	50.899	43.519

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091520\
Data File : P0071342.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Sep 2020 10:37
Operator : DD\AJ
Sample : L3981-09RE
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
B19-7-9RE


Manual Integrations
APPROVED

Ankita
9/16/2020 1:55:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 13:46:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

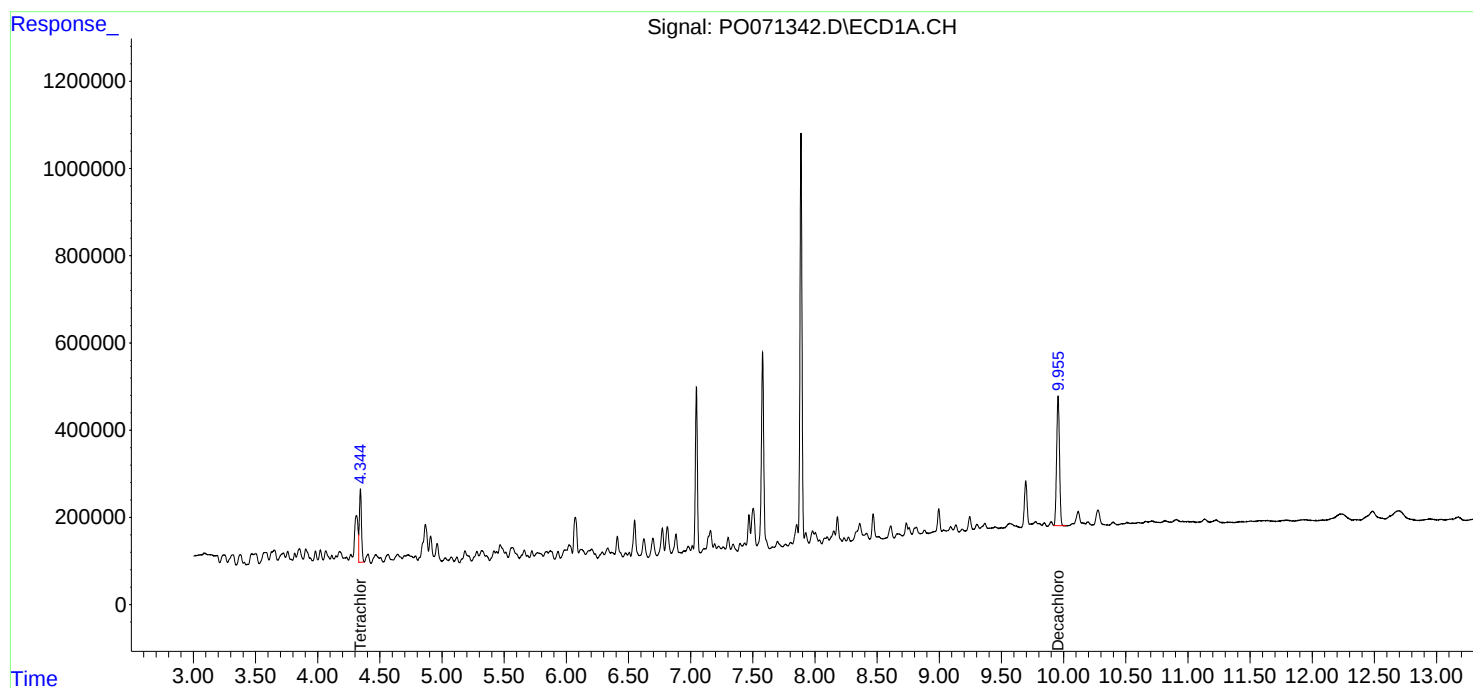

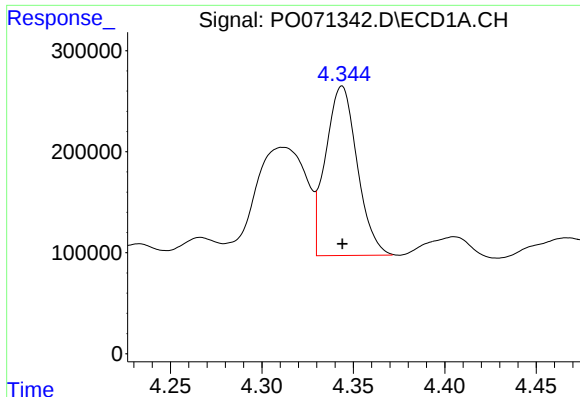


#1 Tetrachloro-m-xylene

R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 2000381
Conc: 28.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
B19-7-9RE


Manual Integrations
APPROVED

Ankita
9/16/2020 1:55:00 PM

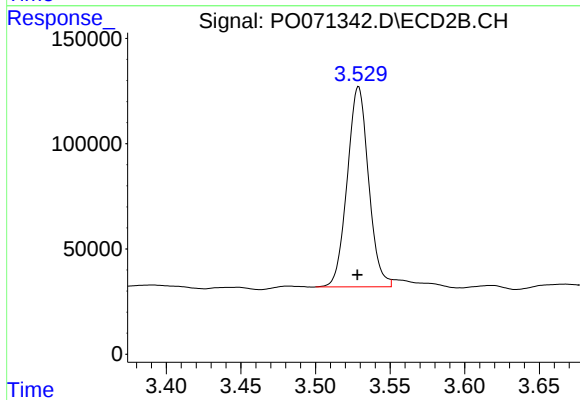


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 945657
Conc: 24.22 ng/ml m

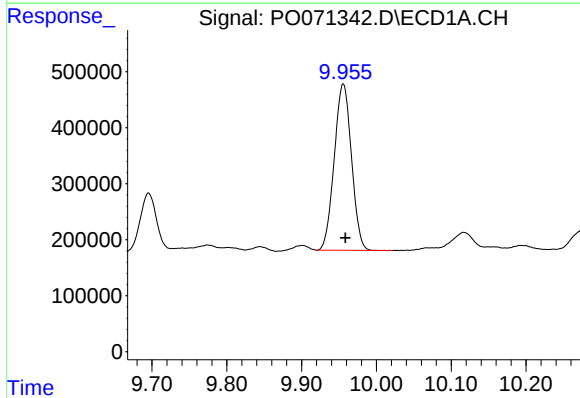

#2 Decachlorobiphenyl

R.T.: 9.956 min
Delta R.T.: -0.003 min
Response: 4746573
Conc: 50.90 ng/ml

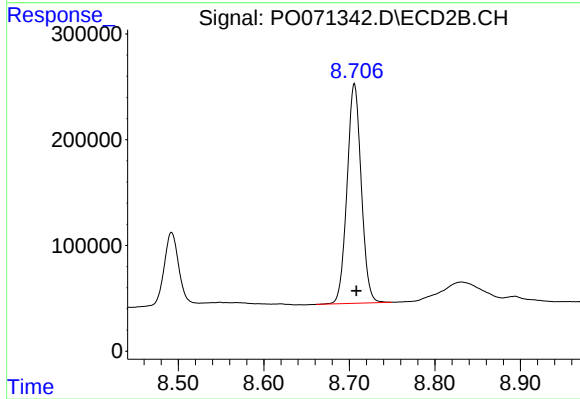

#2 Decachlorobiphenyl

R.T.: 8.706 min
Delta R.T.: -0.002 min
Response: 2397222
Conc: 43.52 ng/ml