

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091521\
 Data File : P0081229.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Sep 2021 12:16
 Operator : AJ\MA
 Sample : M3700-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SIMW-02-20210909

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 05:38:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.926	4.055	1844490	594360	23.365	24.051
2) SA Decachlor...	10.988	9.413	1587431	606803	26.735	25.994

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091521\
Data File : P0081229.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Sep 2021 12:16
Operator : AJ\MA
Sample : M3700-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SIMW-02-20210909

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 05:38:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

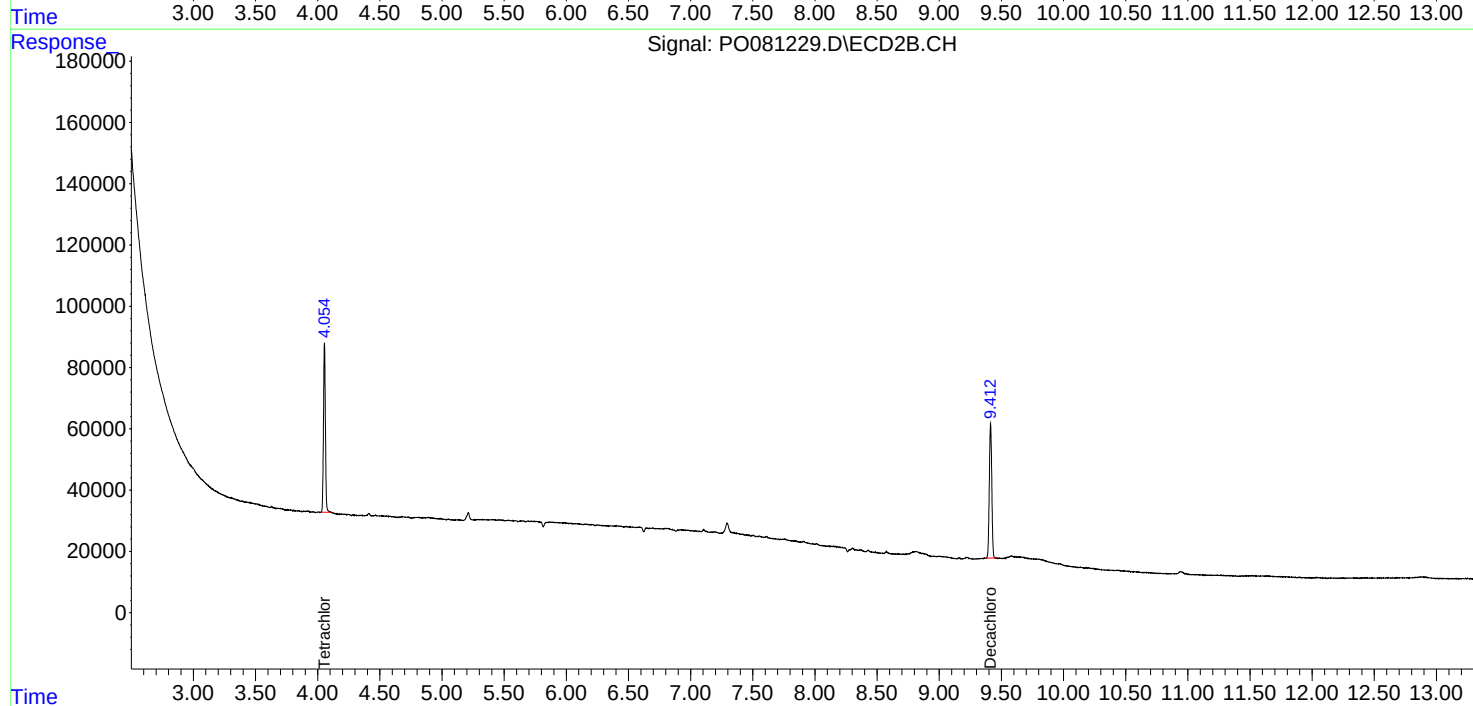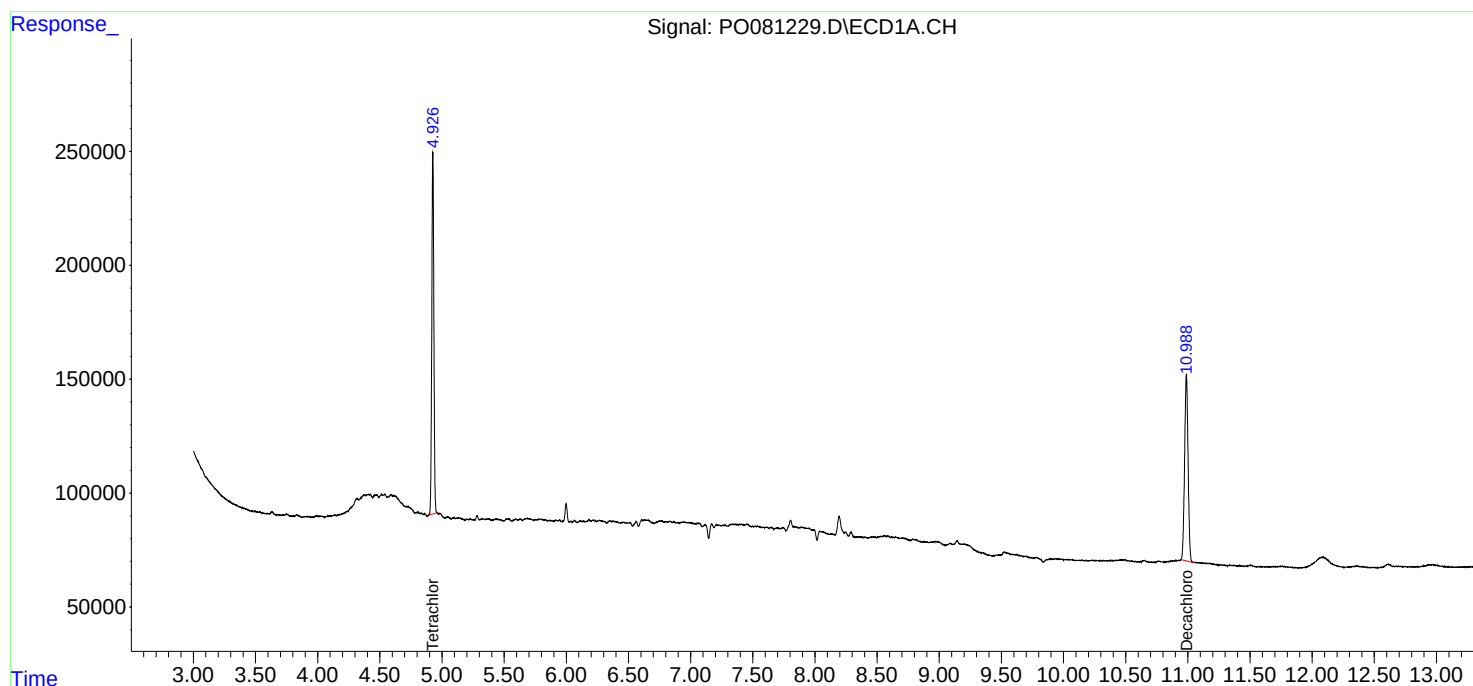


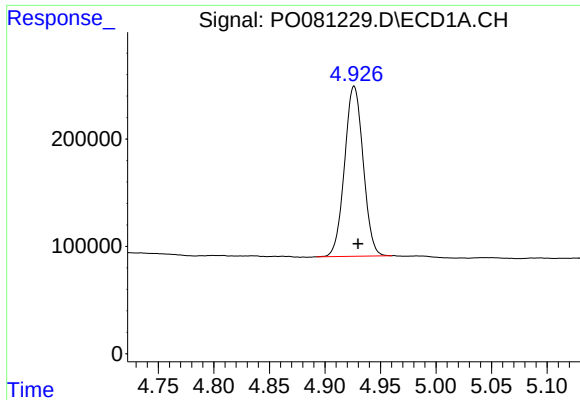

#1 Tetrachloro-m-xylene


R.T.: 4.926 min
Delta R.T.: -0.004 min
Response: 1844490
Conc: 23.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
SIMW-02-20210909

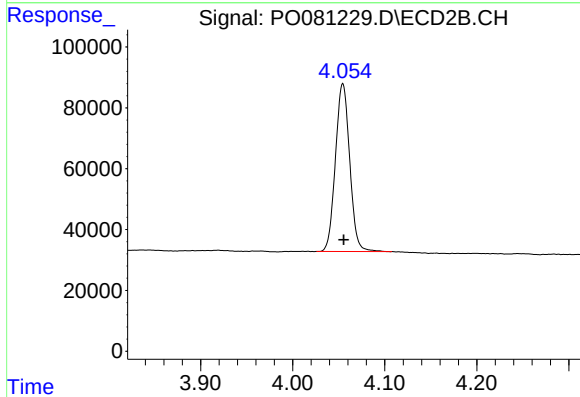


#1 Tetrachloro-m-xylene

R.T.: 4.055 min
Delta R.T.: 0.000 min
Response: 594360
Conc: 24.05 ng/ml

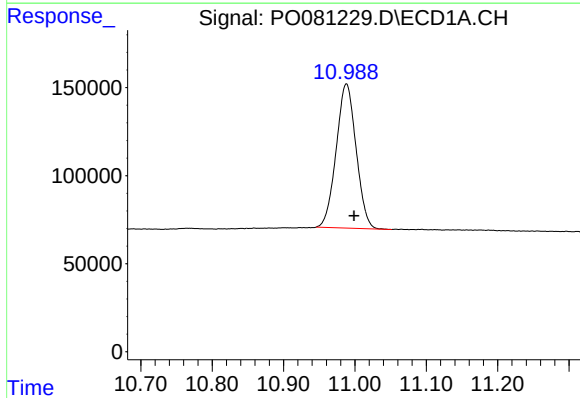

#2 Decachlorobiphenyl

R.T.: 10.988 min
Delta R.T.: -0.011 min
Response: 1587431
Conc: 26.74 ng/ml

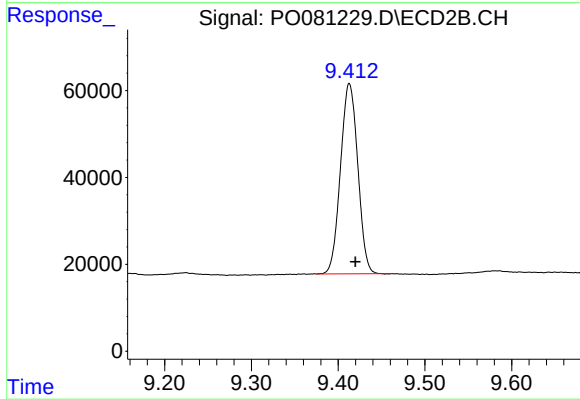

#2 Decachlorobiphenyl

R.T.: 9.413 min
Delta R.T.: -0.007 min
Response: 606803
Conc: 25.99 ng/ml