

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091521\
 Data File : P0081246.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Sep 2021 17:49
 Operator : AJ\MA
 Sample : M3730-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BRICKS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 05:44:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	4.055	1919235	605138	24.312	24.488
2) SA Decachlor...	10.991	9.415	1531452	587730	25.793	25.177

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091521\
Data File : P0081246.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Sep 2021 17:49
Operator : AJ\MA
Sample : M3730-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BRICKS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 05:44:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

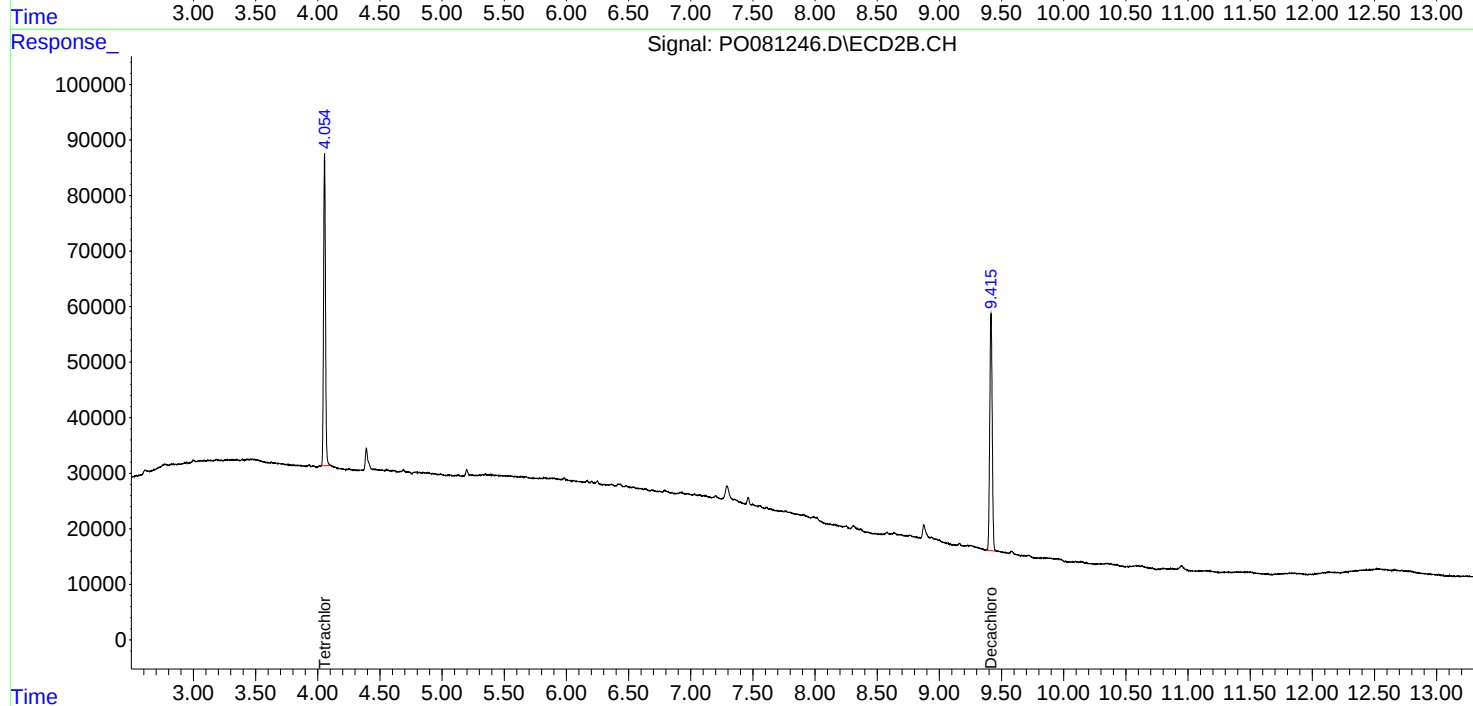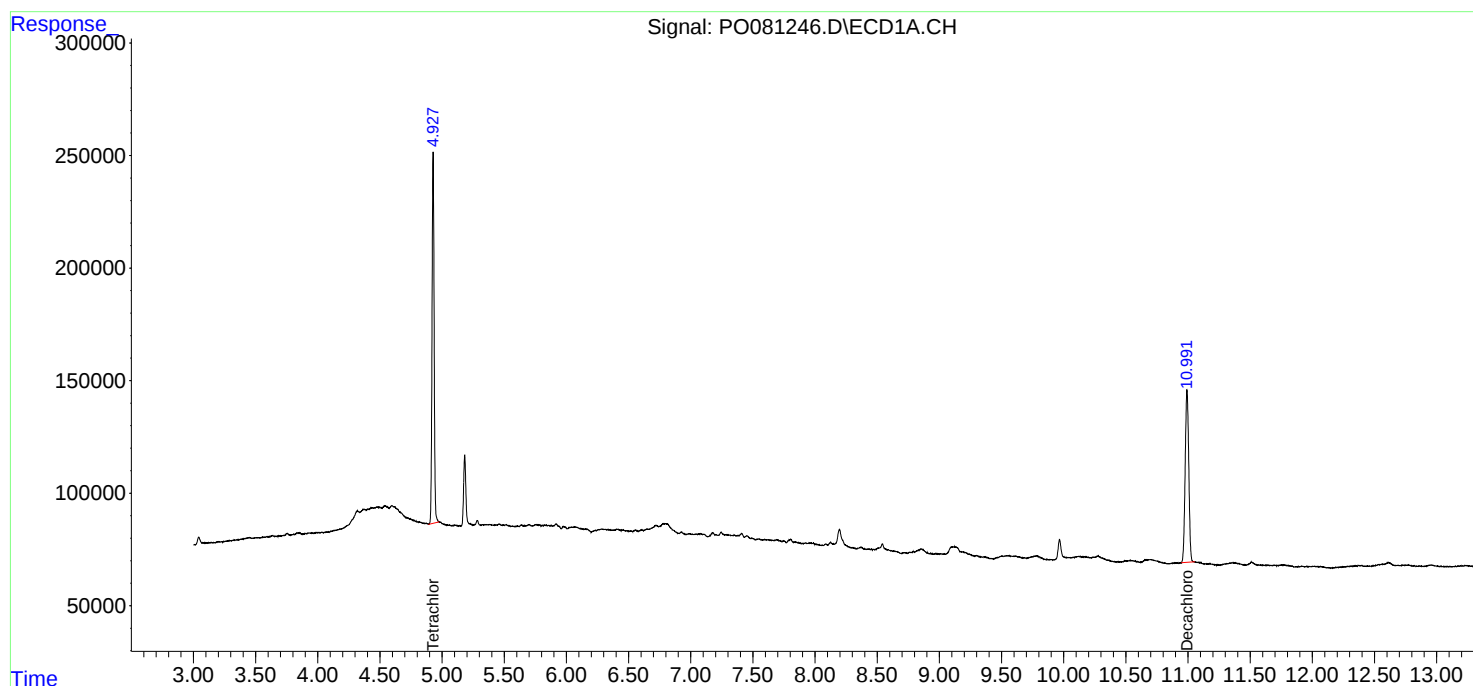


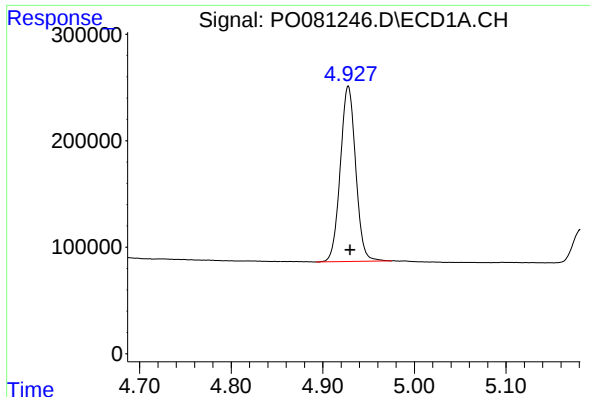

#1 Tetrachloro-m-xylene


R.T.: 4.928 min
Delta R.T.: -0.002 min
Response: 1919235
Conc: 24.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
BRICKS

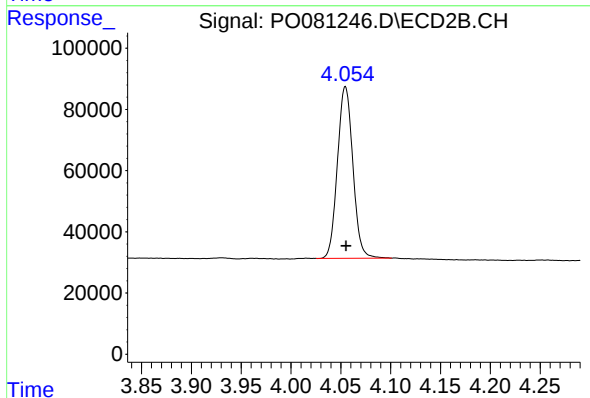


#1 Tetrachloro-m-xylene

R.T.: 4.055 min
Delta R.T.: 0.000 min
Response: 605138
Conc: 24.49 ng/ml

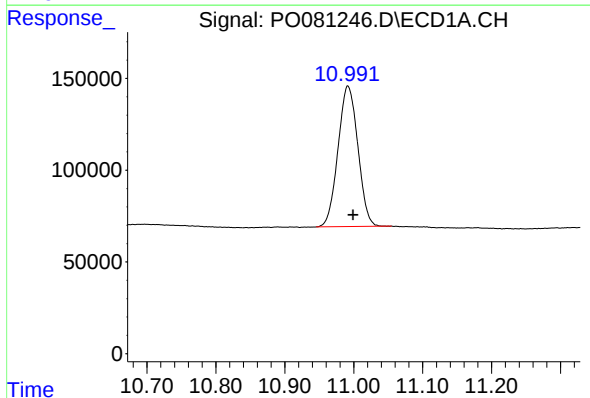

#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: -0.008 min
Response: 1531452
Conc: 25.79 ng/ml

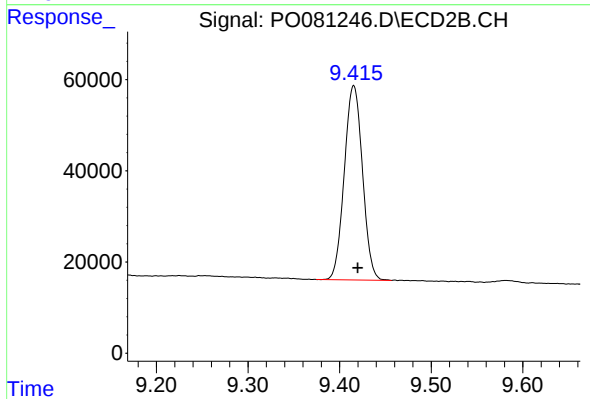

#2 Decachlorobiphenyl

R.T.: 9.415 min
Delta R.T.: -0.004 min
Response: 587730
Conc: 25.18 ng/ml