

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091521\
 Data File : P0081264.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Sep 2021 23:35
 Operator : AJ\MA
 Sample : M3696-08 20X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 869141B-3B-END-1-2

Manual Integrations
 APPROVED

mohammad
 9/16/2021 1:27:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 05:49:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	4.052	73728	27766	0.934m	1.124
2) SA Decachlor...	10.988	9.411	50046	20348	0.843	0.872

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091521\
Data File : P0081264.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Sep 2021 23:35
Operator : AJ\MA
Sample : M3696-08 20X
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
869141B-3B-END-1-2


Manual Integrations
APPROVED

mohammad
9/16/2021 1:27:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 05:49:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

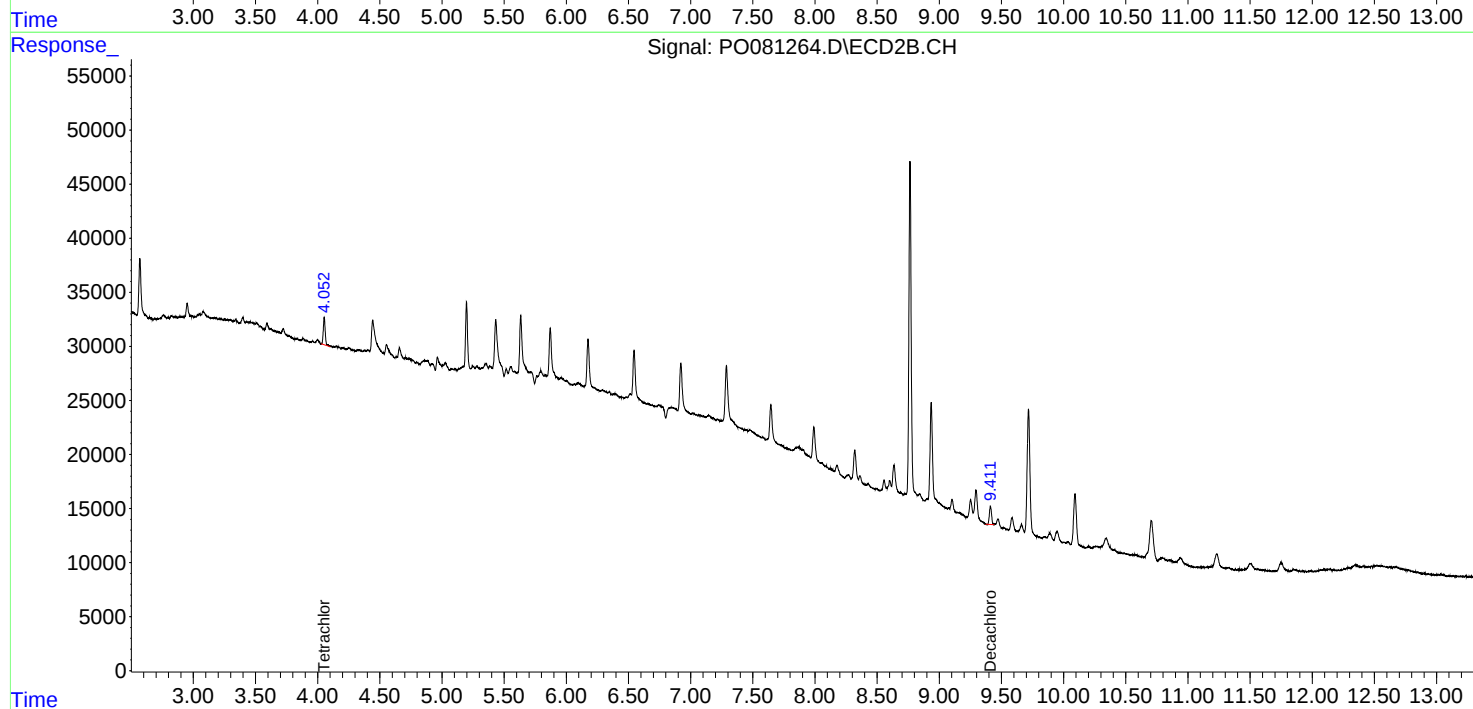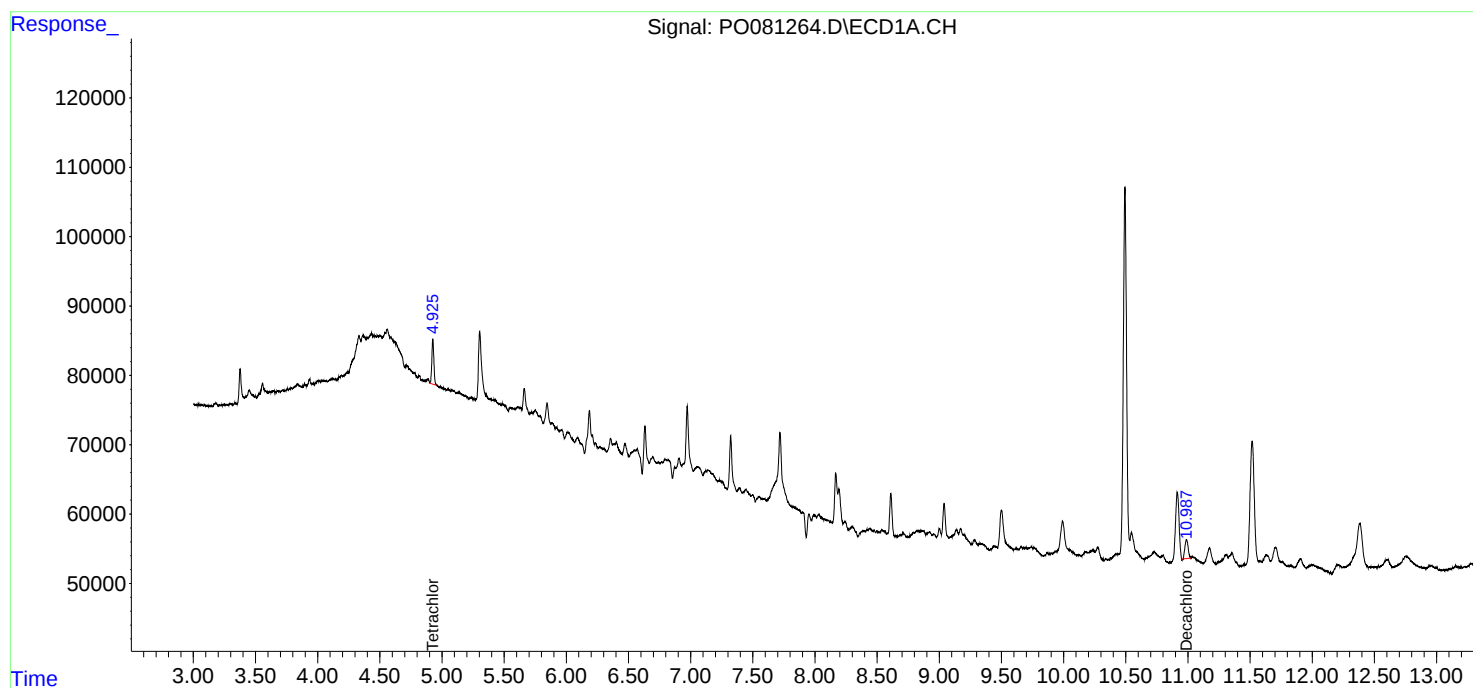

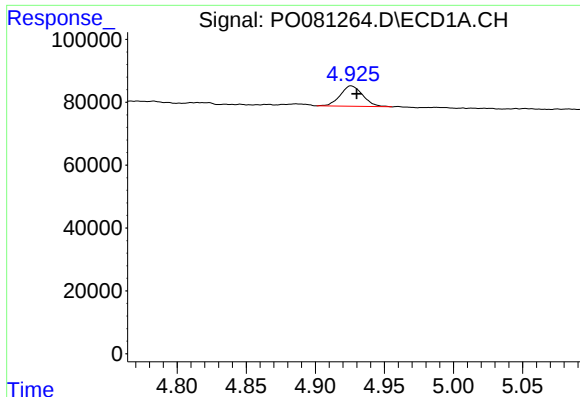


#1 Tetrachloro-m-xylene

R.T.: 4.925 min
Delta R.T.: -0.005 min
Response: 73728
Conc: 0.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
869141B-3B-END-1-2


Manual Integrations
APPROVED

mohammad
9/16/2021 1:27:58 PM

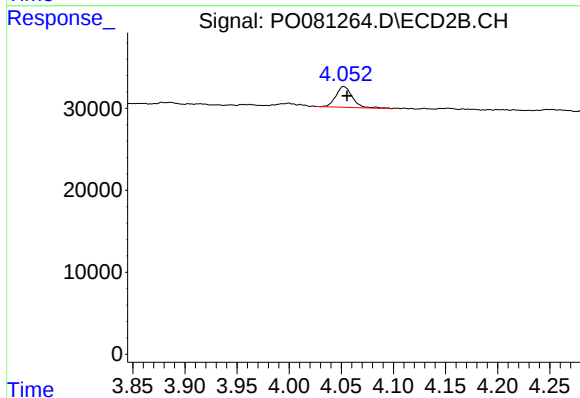


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: -0.003 min
Response: 27766
Conc: 1.12 ng/ml

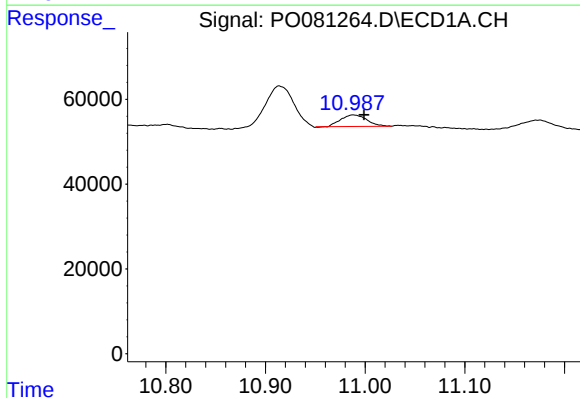

#2 Decachlorobiphenyl

R.T.: 10.988 min
Delta R.T.: -0.011 min
Response: 50046
Conc: 0.84 ng/ml

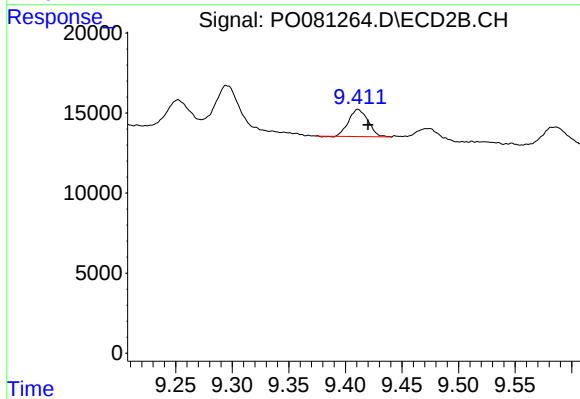

#2 Decachlorobiphenyl

R.T.: 9.411 min
Delta R.T.: -0.009 min
Response: 20348
Conc: 0.87 ng/ml