

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091525\
 Data File : P0113753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2025 23:37
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 DDT ANALOG

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2025
 Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:18:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
30) L6 AR-1254-5	6.741	6.705	4506.5E6	1834.8E6	6054.364m	5977.169m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO091525\
Data File : PO113753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2025 23:37
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
DDT ANALOG


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:18:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

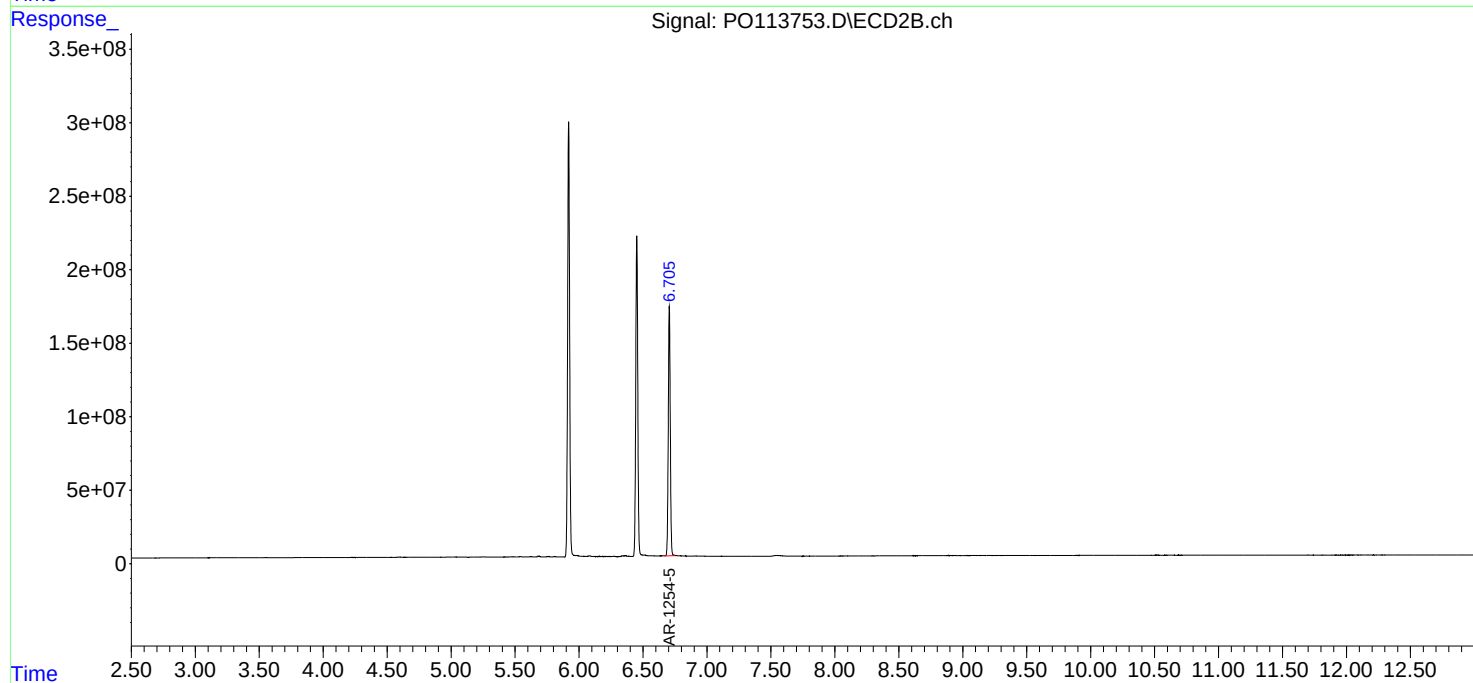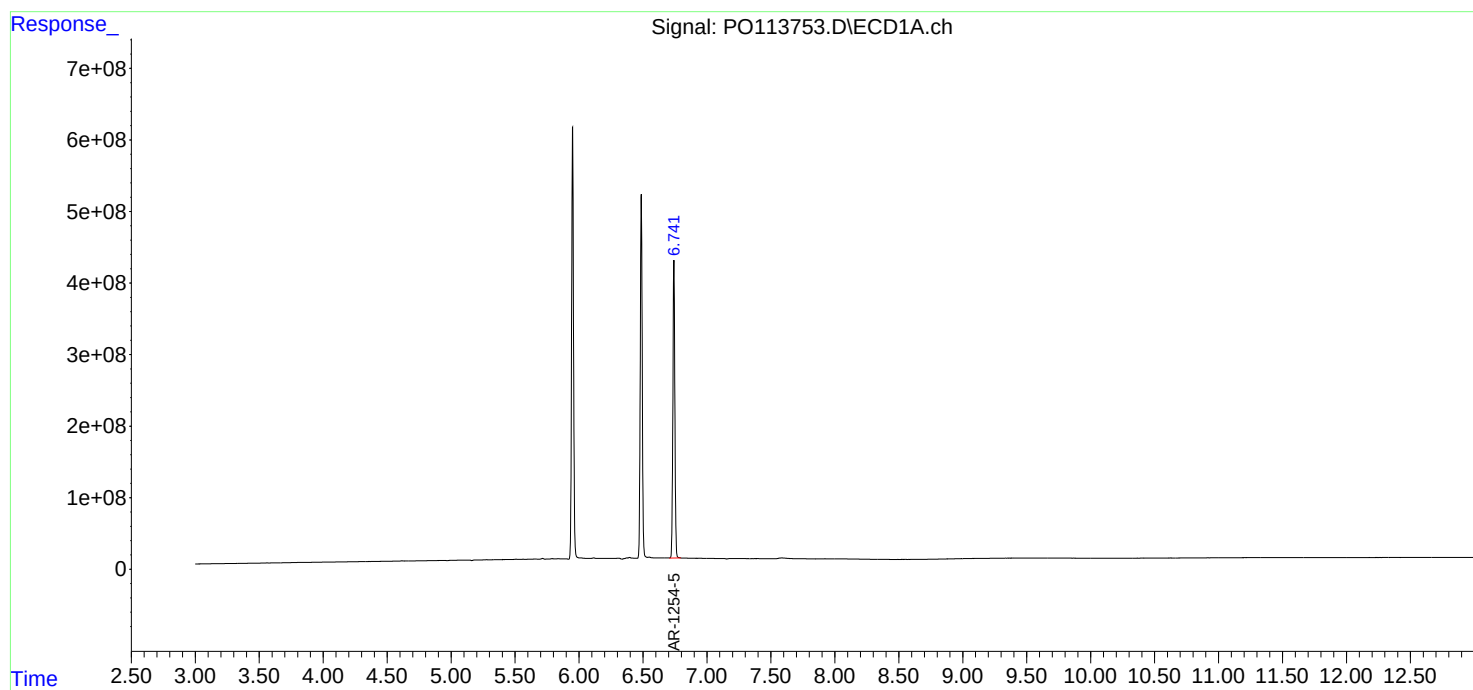

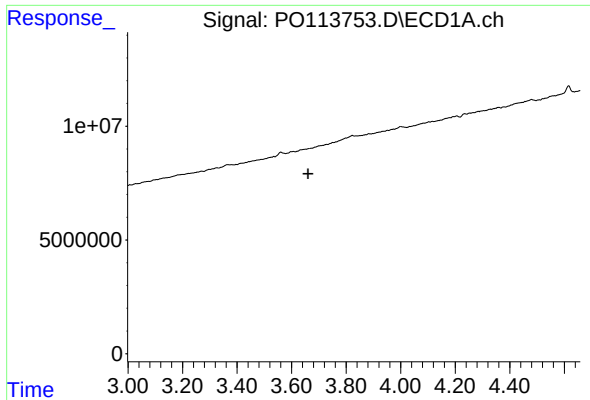


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

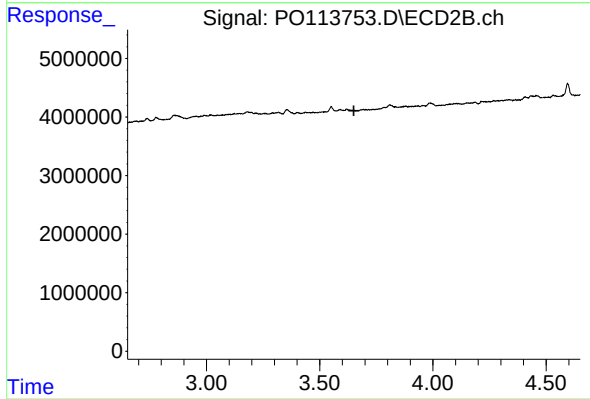


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.651 min
Response: 0
Conc: N.D.

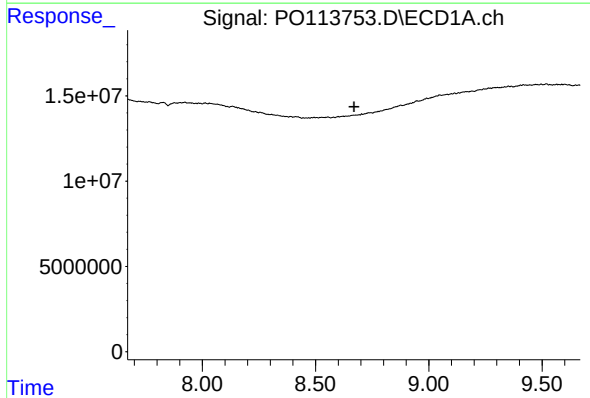


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.670 min
Response: 0
Conc: N.D.

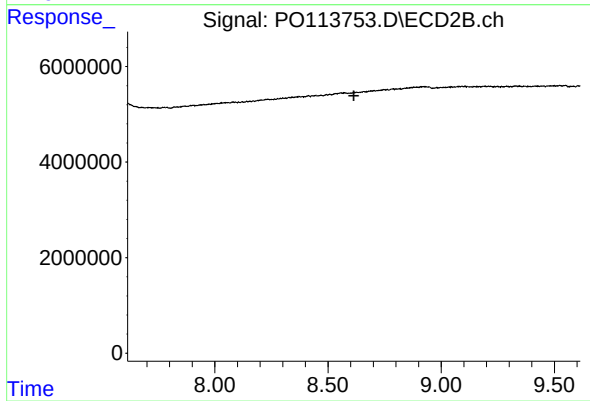

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.614 min
Response: 0
Conc: N.D.

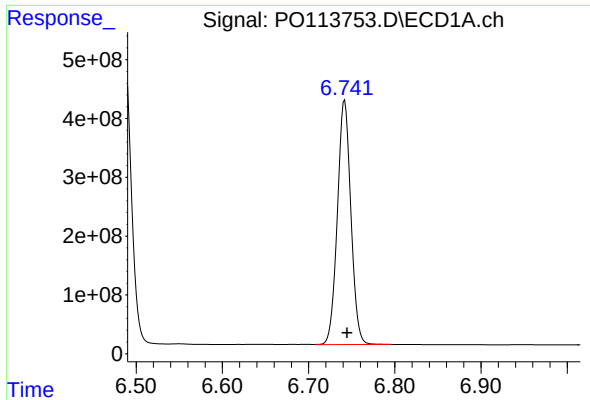


#30 AR-1254-5

R.T.: 6.741 min
Delta R.T.: -0.004 min
Response: 4506485827
Conc: 6054.36 ng/m

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

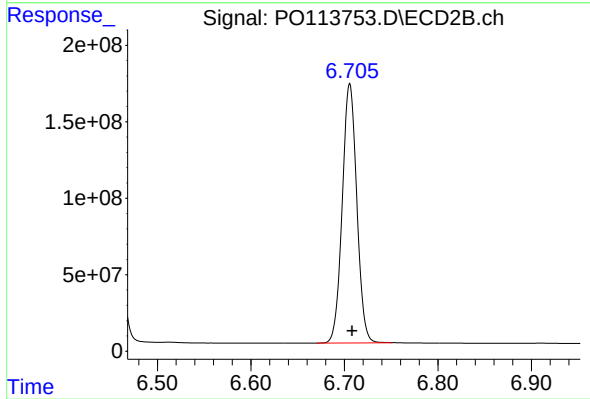

#30 AR-1254-5

R.T.: 6.705 min
Delta R.T.: -0.003 min
Response: 1834824111
Conc: 5977.17 ng/ml m