

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091619\
 Data File : P0060931.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Sep 2019 13:52
 Operator : SM/AJ
 Sample : K4570-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOUTH-AVENUE-3-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:12:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.366	3.530	848229	647045	23.055	23.173
2)	SA Decachlor...	10.029	8.409	708822	580710	15.427	16.567

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091619\
Data File : P0060931.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2019 13:52
Operator : SM/AJ
Sample : K4570-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SOUTH-AVENUE-3-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:12:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

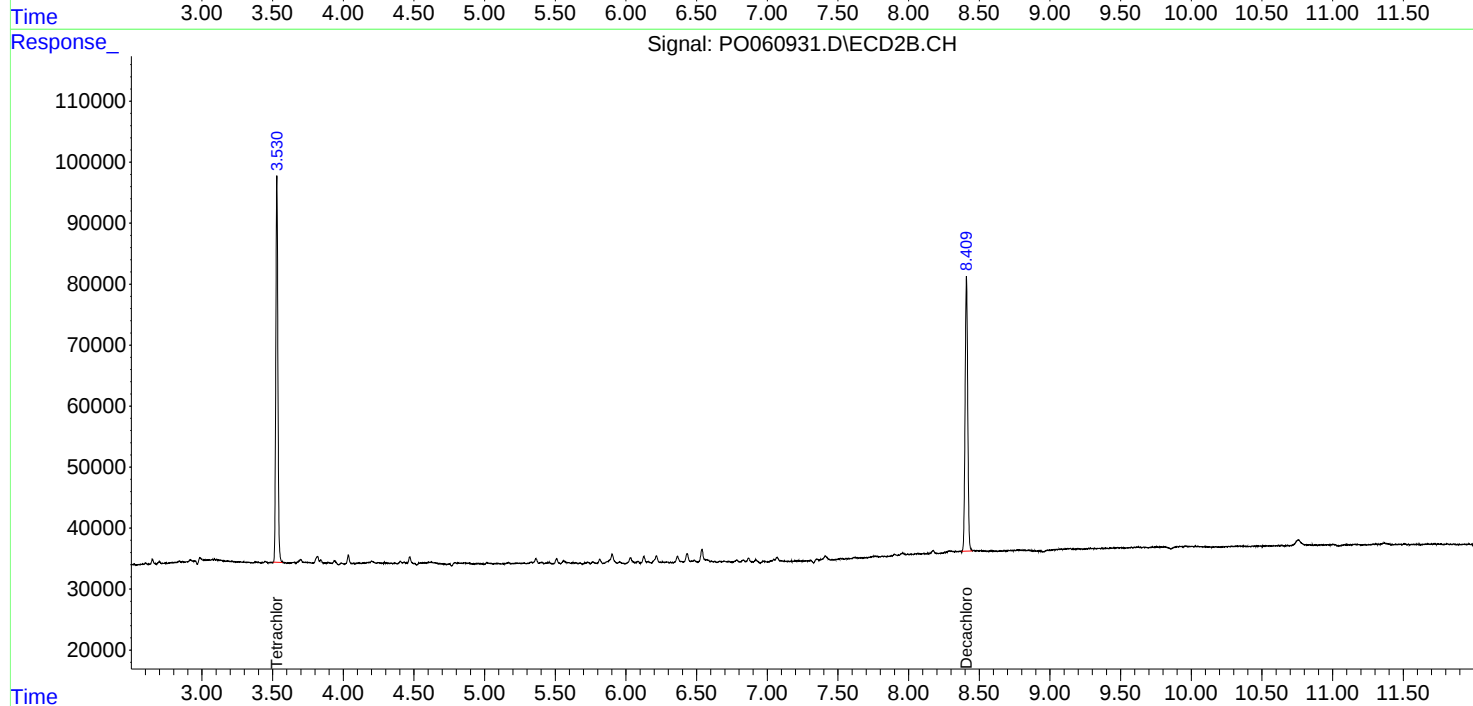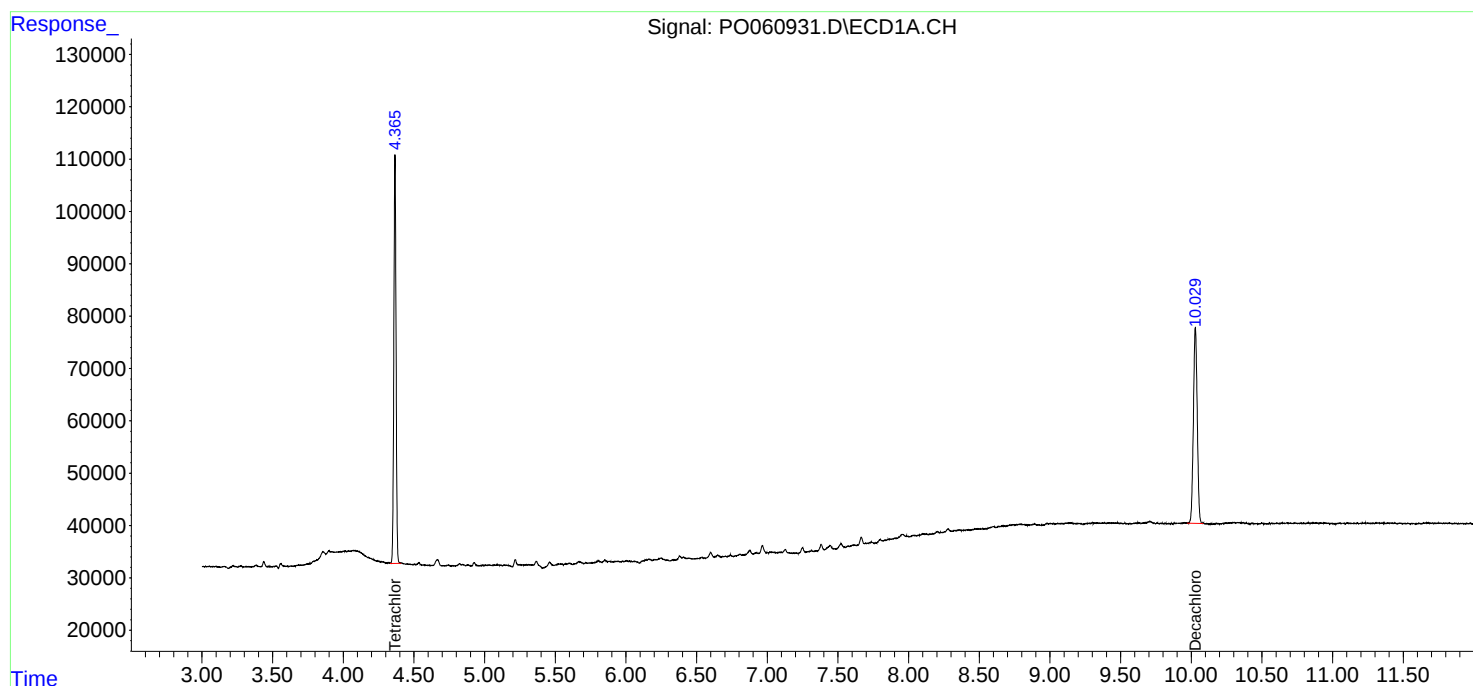


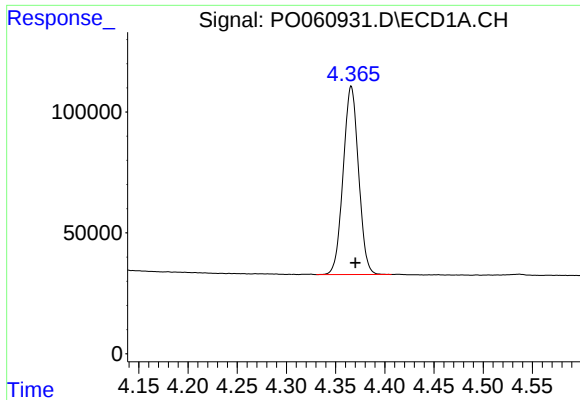

#1 Tetrachloro-m-xylene


R.T.: 4.366 min
Delta R.T.: -0.004 min
Response: 848229
Conc: 23.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
SOUTH-AVENUE-3-ABCD

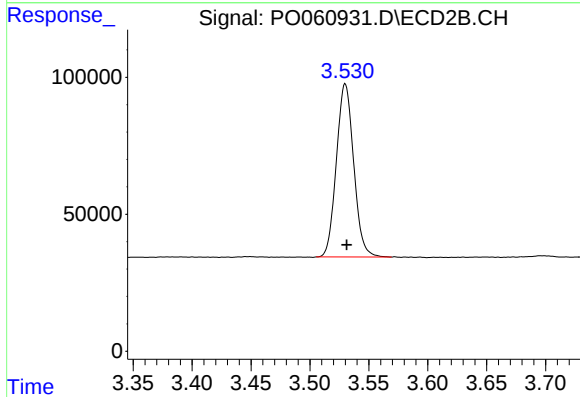


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.001 min
Response: 647045
Conc: 23.17 ng/ml

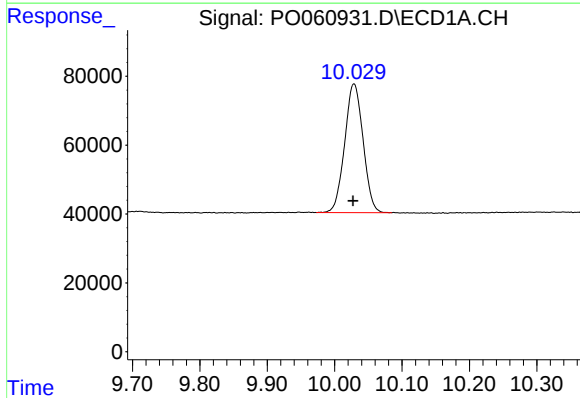

#2 Decachlorobiphenyl

R.T.: 10.029 min
Delta R.T.: 0.001 min
Response: 708822
Conc: 15.43 ng/ml

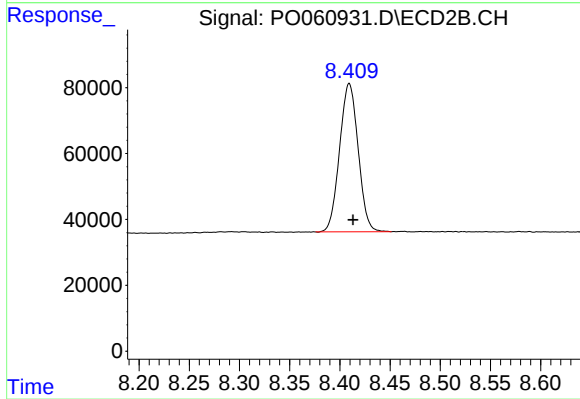

#2 Decachlorobiphenyl

R.T.: 8.409 min
Delta R.T.: -0.004 min
Response: 580710
Conc: 16.57 ng/ml