

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091619\
Data File : P0060948.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2019 19:08
Operator : SM/AJ
Sample : K4871-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
VE-3-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:28:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.366	3.530	466669	407246	12.684	14.585
2)	SA Decachlor...	10.028	8.409	383410	328702	8.345	9.378

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091619\
Data File : PO060948.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2019 19:08
Operator : SM/AJ
Sample : K4871-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
VE-3-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:28:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

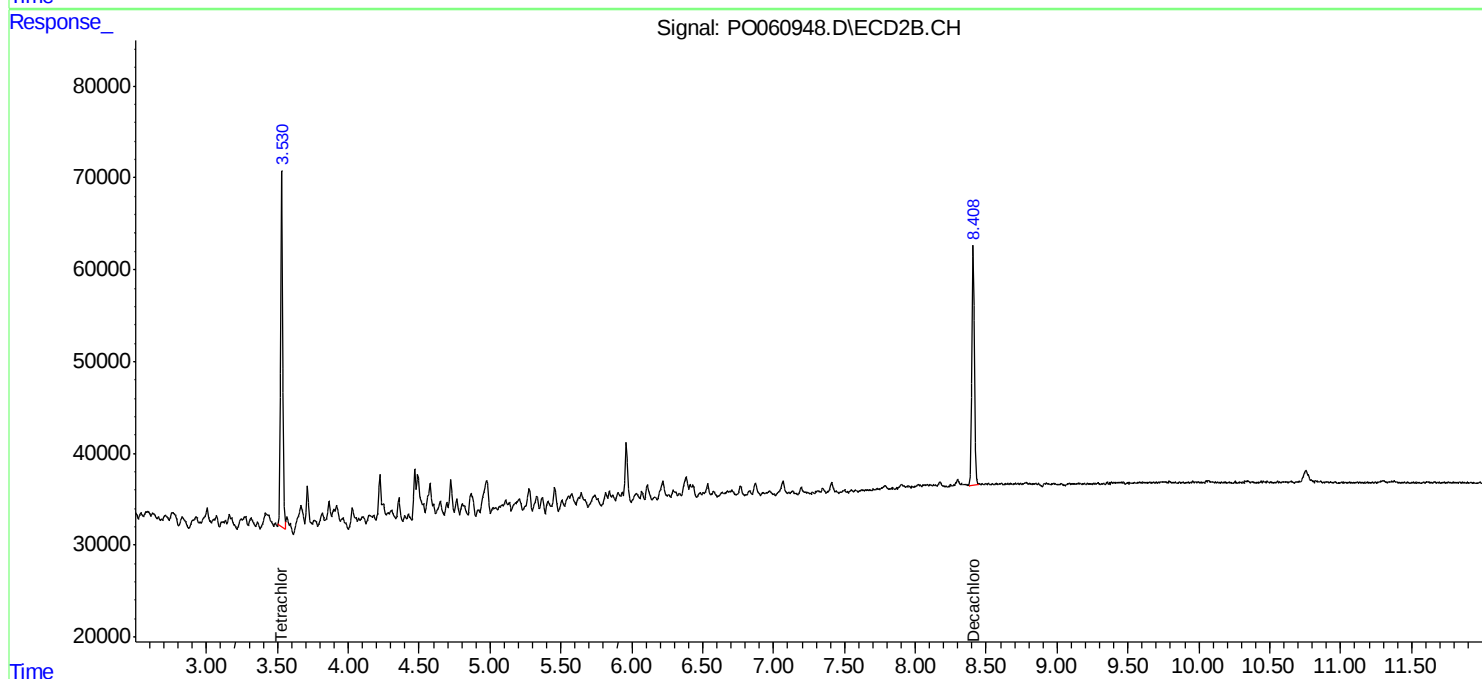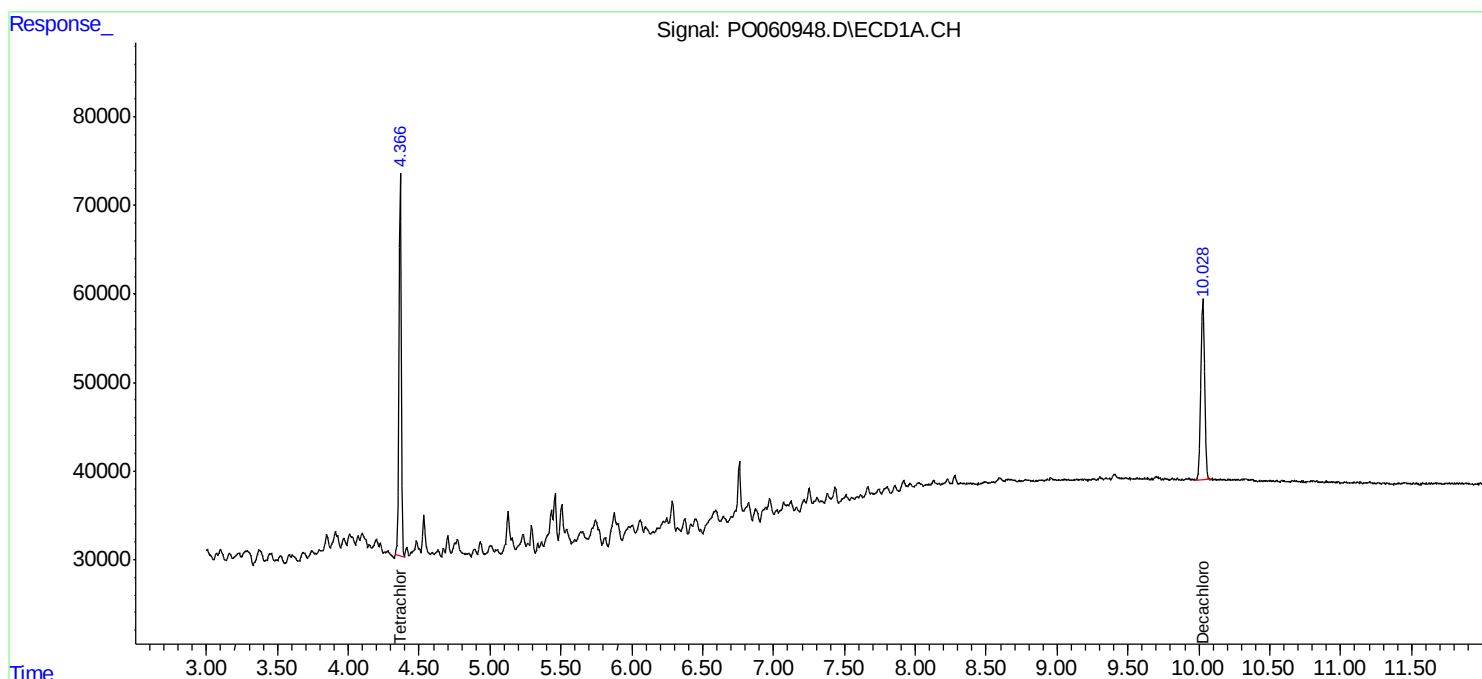


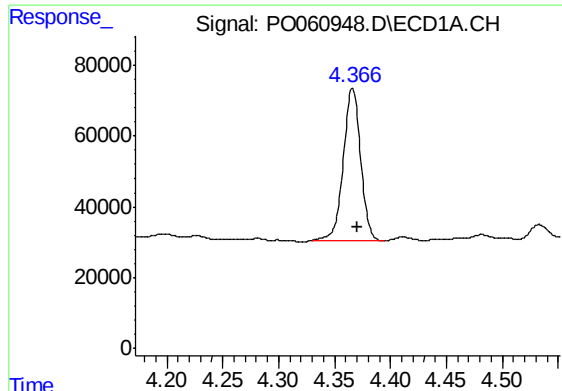

#1 Tetrachloro-m-xylene


R.T.: 4.366 min
Delta R.T.: -0.004 min
Response: 466669
Conc: 12.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
VE-3-1

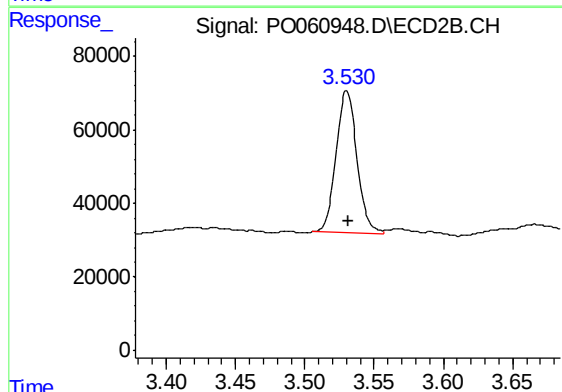


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.001 min
Response: 407246
Conc: 14.59 ng/ml

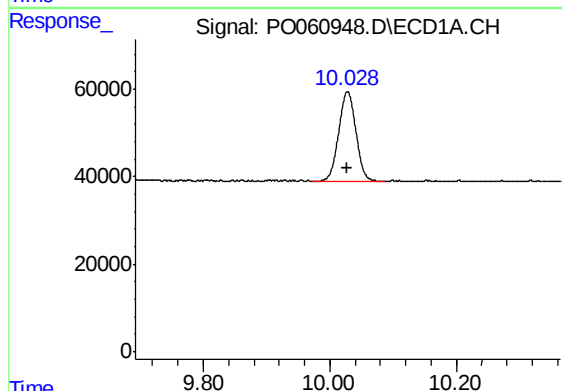

#2 Decachlorobiphenyl

R.T.: 10.028 min
Delta R.T.: 0.000 min
Response: 383410
Conc: 8.34 ng/ml

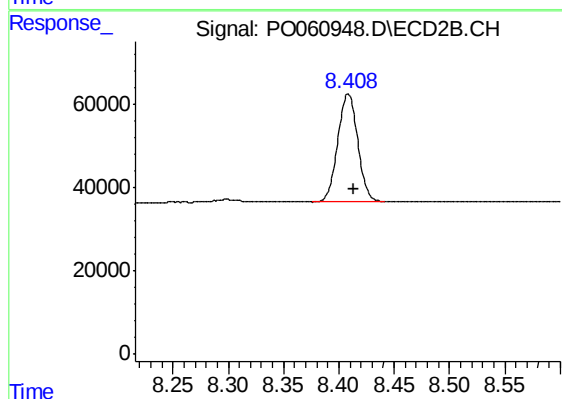

#2 Decachlorobiphenyl

R.T.: 8.409 min
Delta R.T.: -0.005 min
Response: 328702
Conc: 9.38 ng/ml