

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091619\
 Data File : P0060952.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Sep 2019 20:12
 Operator : SM/AJ
 Sample : K4884-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 6INCH-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 02:29:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.365	3.529	886012	668022	24.082	23.924
2)	SA Decachlor...	10.027	8.408	753187	622718	16.393	17.766

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091619\
Data File : PO060952.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2019 20:12
Operator : SM/AJ
Sample : K4884-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
6INCH-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:29:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

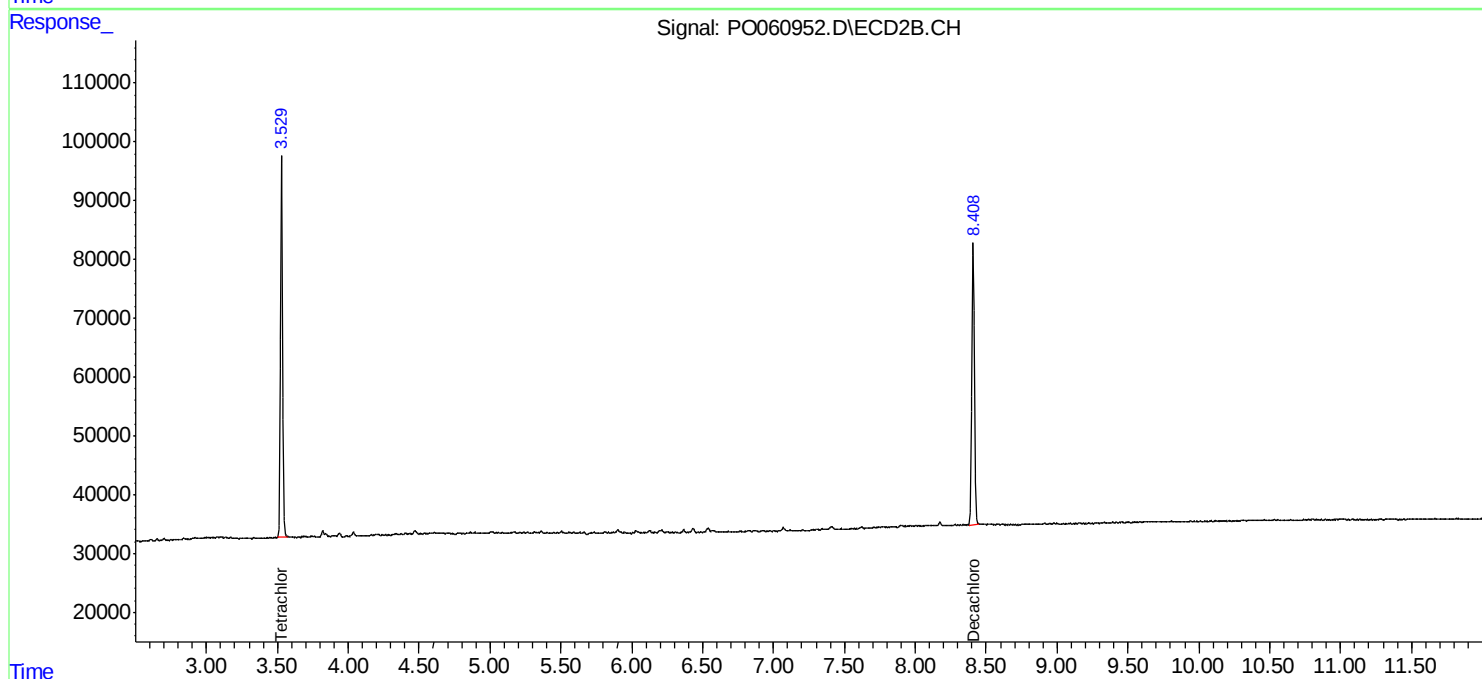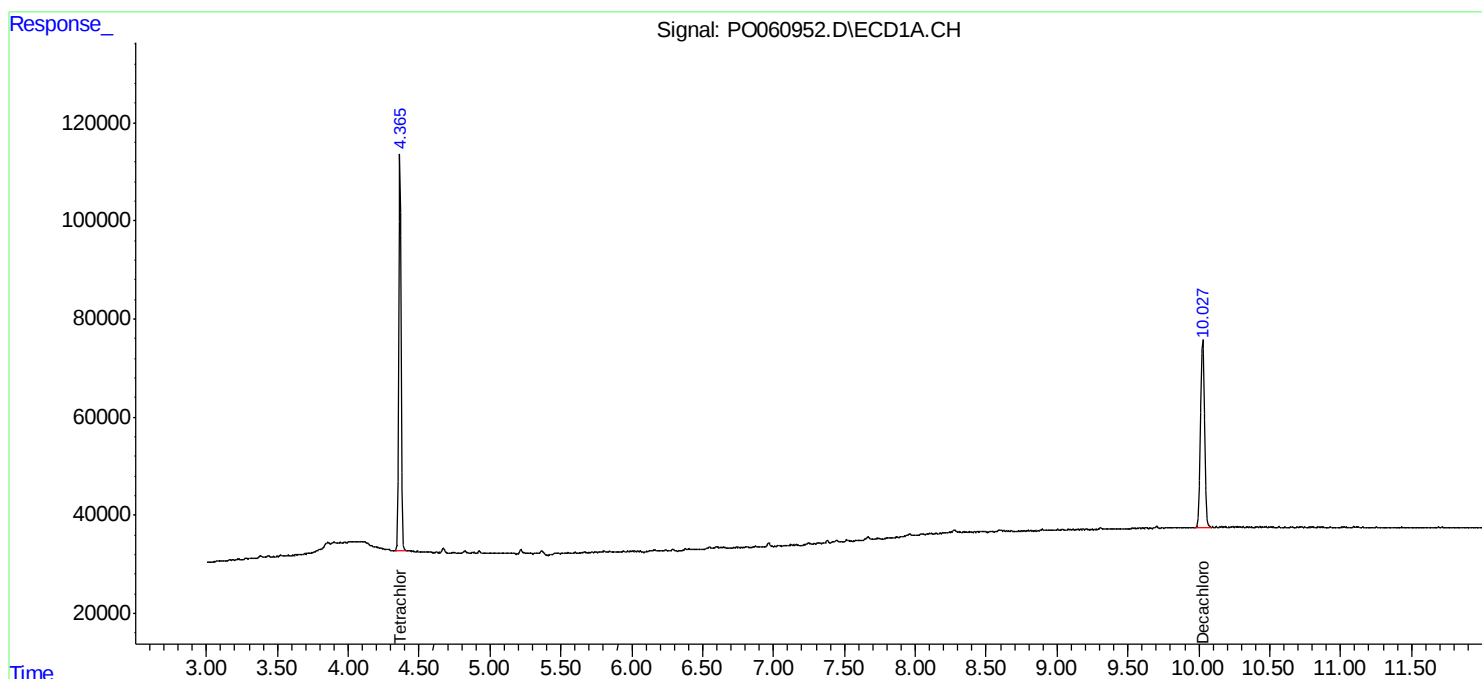


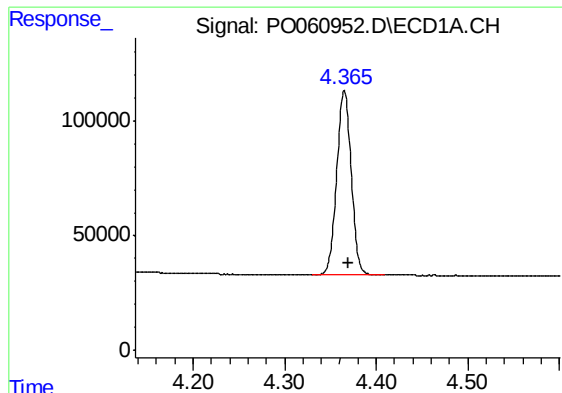

#1 Tetrachloro-m-xylene


R.T.: 4.365 min
Delta R.T.: -0.005 min
Response: 886012
Conc: 24.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
6INCH-PIT

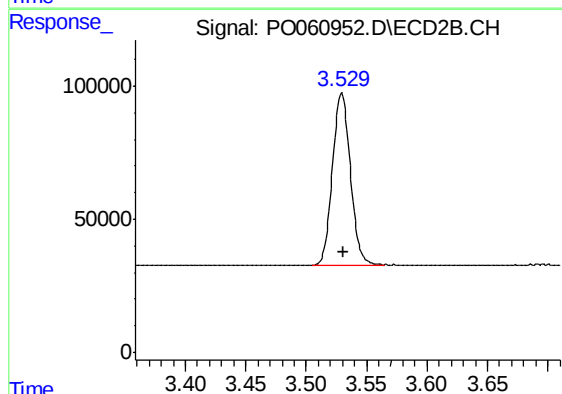


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.002 min
Response: 668022
Conc: 23.92 ng/ml

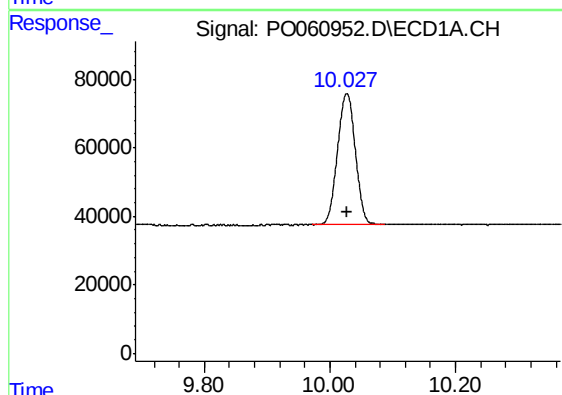

#2 Decachlorobiphenyl

R.T.: 10.027 min
Delta R.T.: 0.000 min
Response: 753187
Conc: 16.39 ng/ml

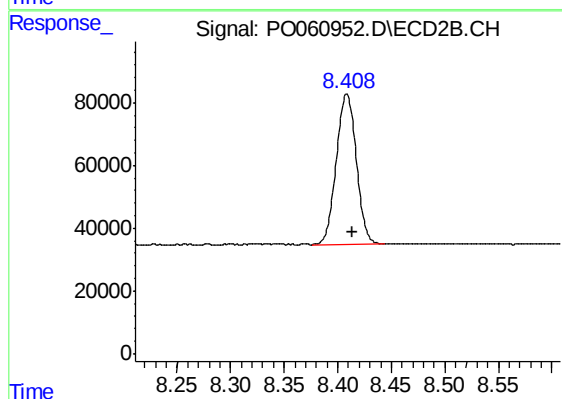

#2 Decachlorobiphenyl

R.T.: 8.408 min
Delta R.T.: -0.005 min
Response: 622718
Conc: 17.77 ng/ml