

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091619\
 Data File : P0060967.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 00:13
 Operator : SM/AJ
 Sample : K4918-02
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-3

Manual Integrations
 APPROVED

Ankita
 9/17/2019 9:25:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 02:34:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.364	3.528	697525	576360	18.959	20.642
2)	SA Decachlor...	10.025	8.407	669926	542964	14.581	15.490
Target Compounds							
31)	L7 AR-1260-1	7.123	6.030	36477	61888	14.983m	29.423m#
32)	L7 AR-1260-2	7.376	6.215	55519	34192	18.363	13.255m#
33)	L7 AR-1260-3	7.736	6.365	26971	37047	11.302m	15.385 #
34)	L7 AR-1260-4	7.954	6.830	54397	27171	19.443m	12.695 #
35)	L7 AR-1260-5	8.276	7.068	45874	53240	8.424m	11.017 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091619\
Data File : PO060967.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2019 00:13
Operator : SM/AJ
Sample : K4918-02
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-3


Manual Integrations
APPROVED

Ankita
9/17/2019 9:25:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:34:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

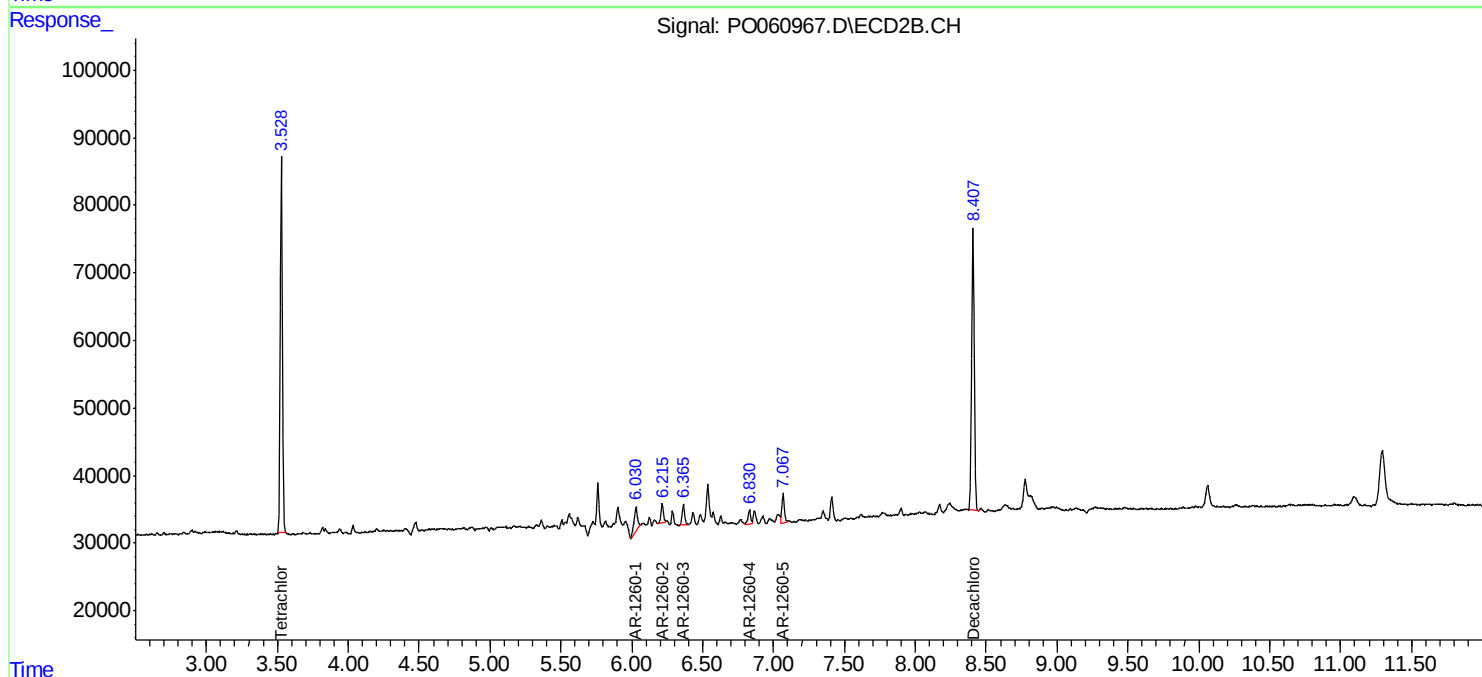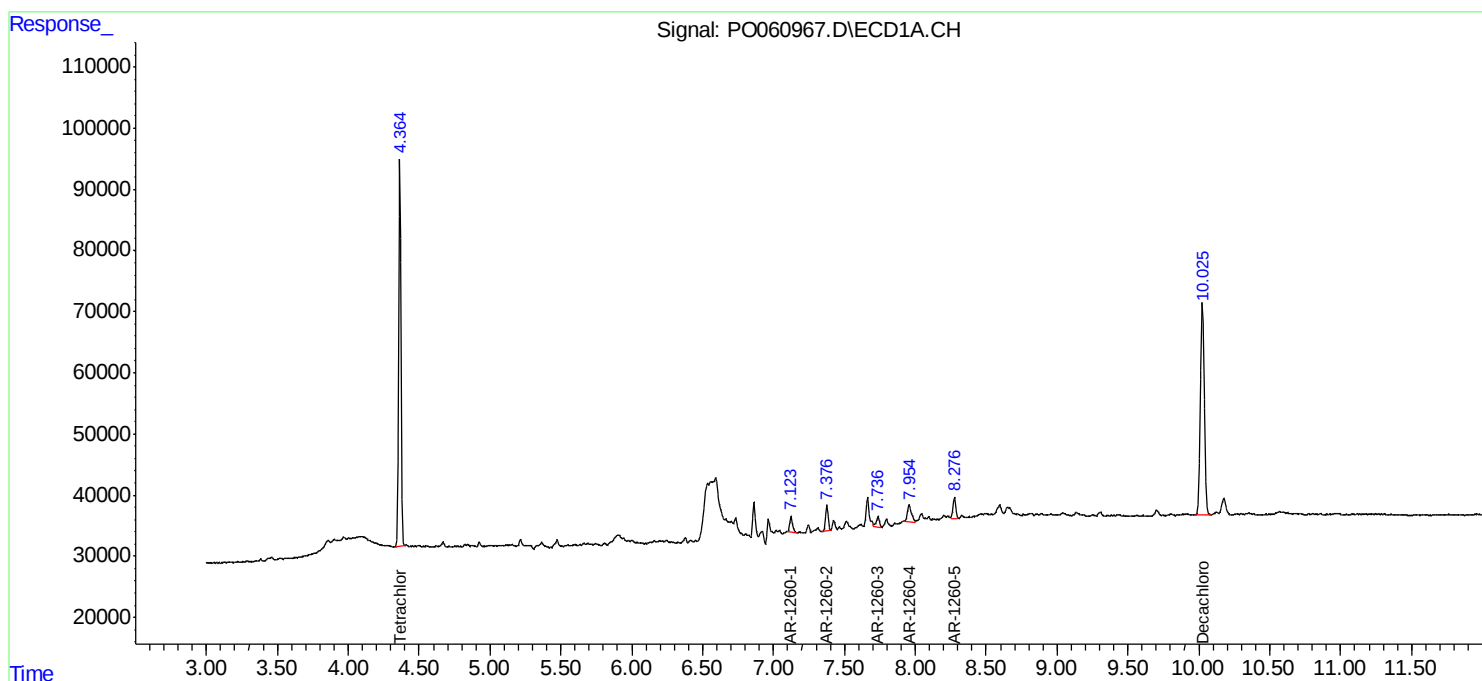

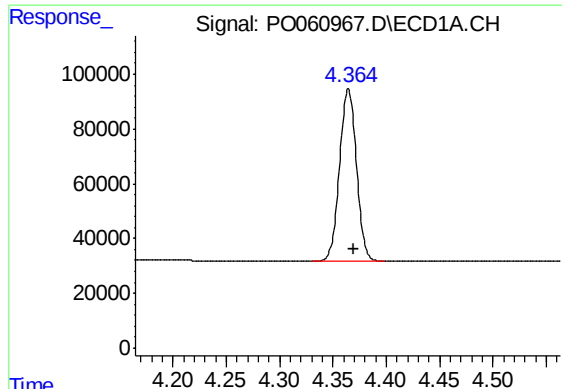


#1 Tetrachloro-m-xylene

R.T.: 4.364 min
Delta R.T.: -0.006 min
Response: 697525
Conc: 18.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-3


Manual Integrations
APPROVED

Ankita
9/17/2019 9:25:49 AM

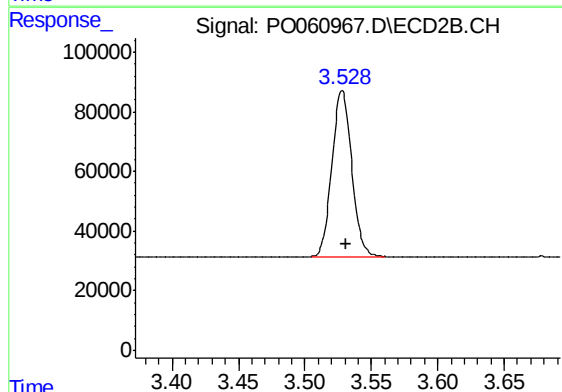


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: -0.003 min
Response: 576360
Conc: 20.64 ng/ml

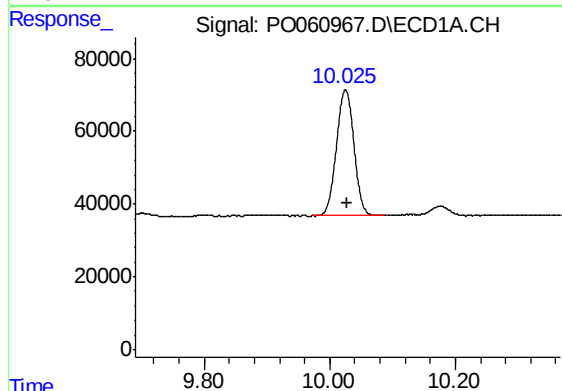


#2 Decachlorobiphenyl

R.T.: 10.025 min
Delta R.T.: -0.002 min
Response: 669926
Conc: 14.58 ng/ml

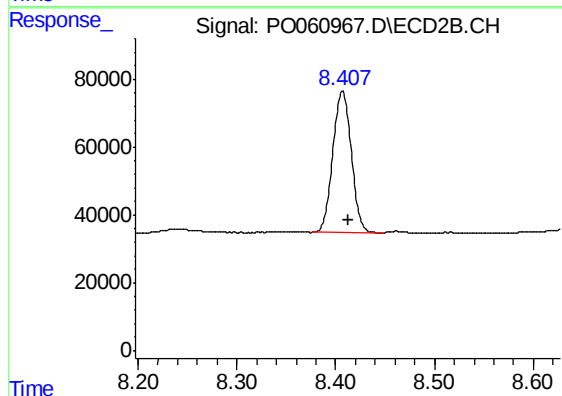

#2 Decachlorobiphenyl

R.T.: 8.407 min
Delta R.T.: -0.006 min
Response: 542964
Conc: 15.49 ng/ml

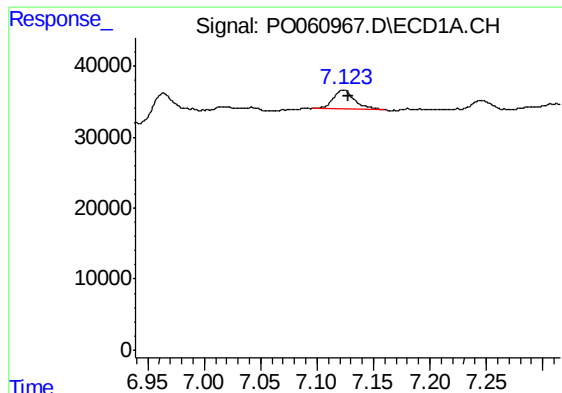


#31 AR-1260-1

R.T.: 7.123 min
Delta R.T.: -0.005 min
Response: 36477
Conc: 14.98 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-3


Manual Integrations
APPROVED

Ankita
9/17/2019 9:25:49 AM

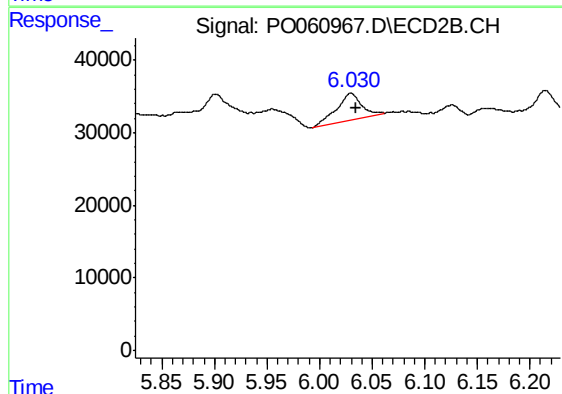


#31 AR-1260-1

R.T.: 6.030 min
Delta R.T.: -0.005 min
Response: 61888
Conc: 29.42 ng/ml m

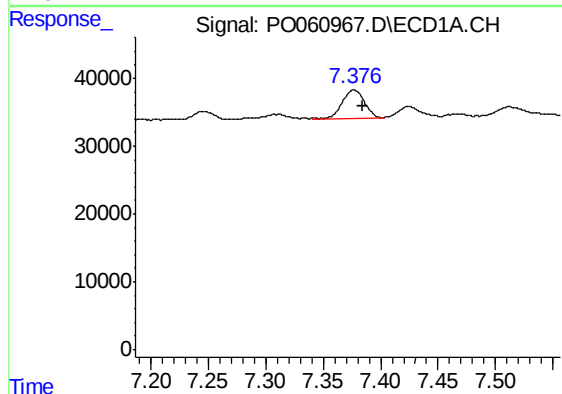


#32 AR-1260-2

R.T.: 7.376 min
Delta R.T.: -0.008 min
Response: 55519
Conc: 18.36 ng/ml

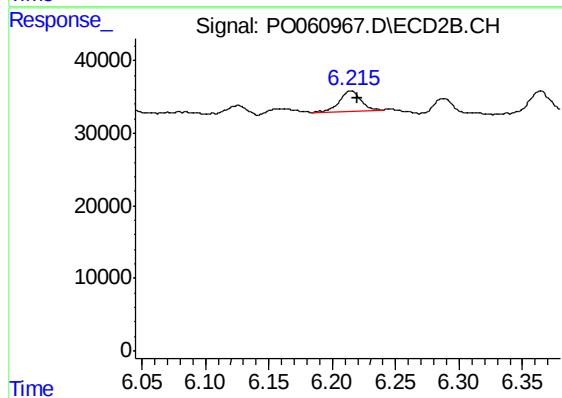

#32 AR-1260-2

R.T.: 6.215 min
Delta R.T.: -0.005 min
Response: 34192
Conc: 13.26 ng/ml m

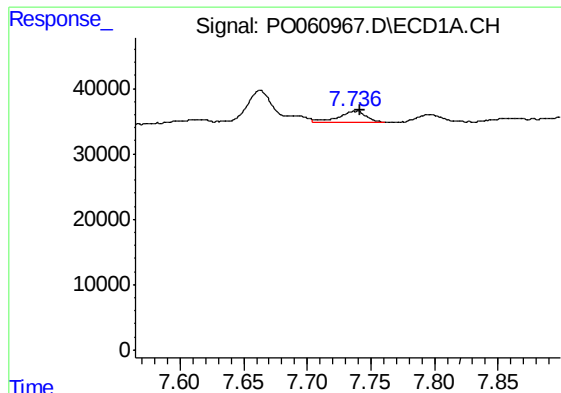


#33 AR-1260-3

R.T.: 7.736 min
Delta R.T.: -0.005 min
Response: 26971
Conc: 11.30 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-3


Manual Integrations
APPROVED

Ankita
9/17/2019 9:25:49 AM

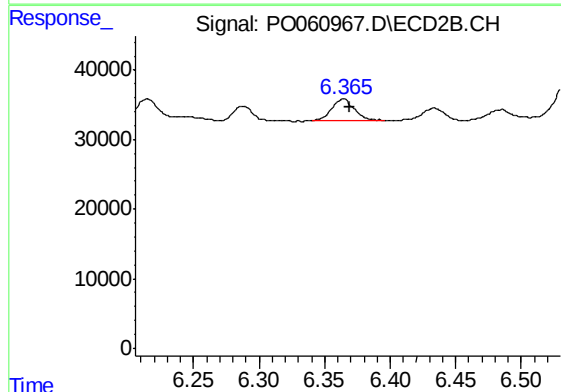


#33 AR-1260-3

R.T.: 6.365 min
Delta R.T.: -0.005 min
Response: 37047
Conc: 15.38 ng/ml

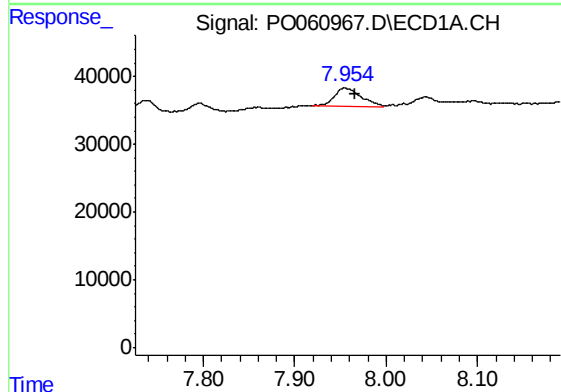


#34 AR-1260-4

R.T.: 7.954 min
Delta R.T.: -0.011 min
Response: 54397
Conc: 19.44 ng/ml m

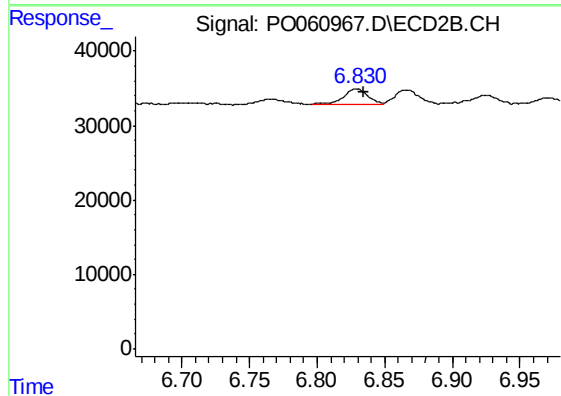

#34 AR-1260-4

R.T.: 6.830 min
Delta R.T.: -0.005 min
Response: 27171
Conc: 12.70 ng/ml

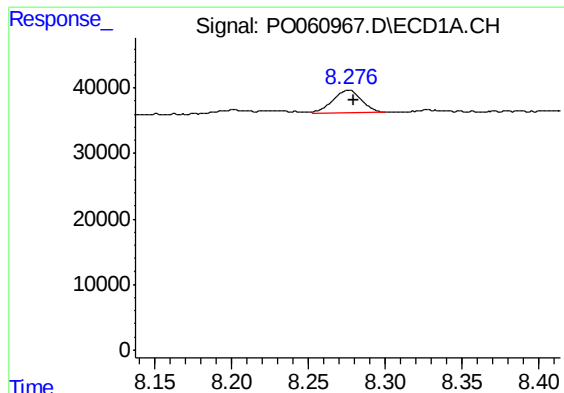


#35 AR-1260-5

R.T.: 8.276 min
Delta R.T.: -0.003 min
Response: 45874
Conc: 8.42 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-3

Manual Integrations
APPROVED

Ankita
9/17/2019 9:25:49 AM

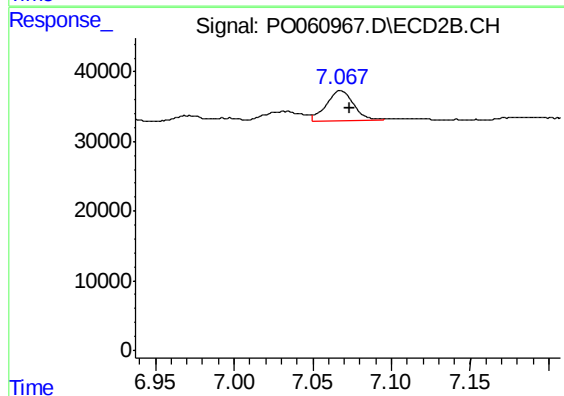

#35 AR-1260-5

R.T.: 7.068 min
Delta R.T.: -0.006 min
Response: 53240
Conc: 11.02 ng/ml