

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091620\
 Data File : P0071370.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Sep 2020 10:48
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 14:02:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
20)	L4	AR-1242-5	6.605	5.625	42381	261264	19.102 188.785 #
24)	L5	AR-1248-4	6.547f	0.000	920491	0	253.304 N.D. #
25)	L5	AR-1248-5	6.605	5.625f	42381	261264	12.736 152.433 #
26)	L6	AR-1254-1	6.547	5.625f	920491	261264	262.367 98.220 #
28)	L6	AR-1254-3	7.167f	0.000	210601	0	35.412 N.D. #
30)	L6	AR-1254-5	7.876f	0.000	26459	0	4.743 N.D. #
35)	L7	AR-1260-5	8.465	0.000	47852	0	3.774 N.D. #
37)	L8	AR-1262-2	8.465	0.000	47852	0	3.315 N.D. #
45)	L9	AR-1268-5	9.714f	0.000	29213	0	0.838 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091620\
Data File : PO071370.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2020 10:48
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 14:02:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

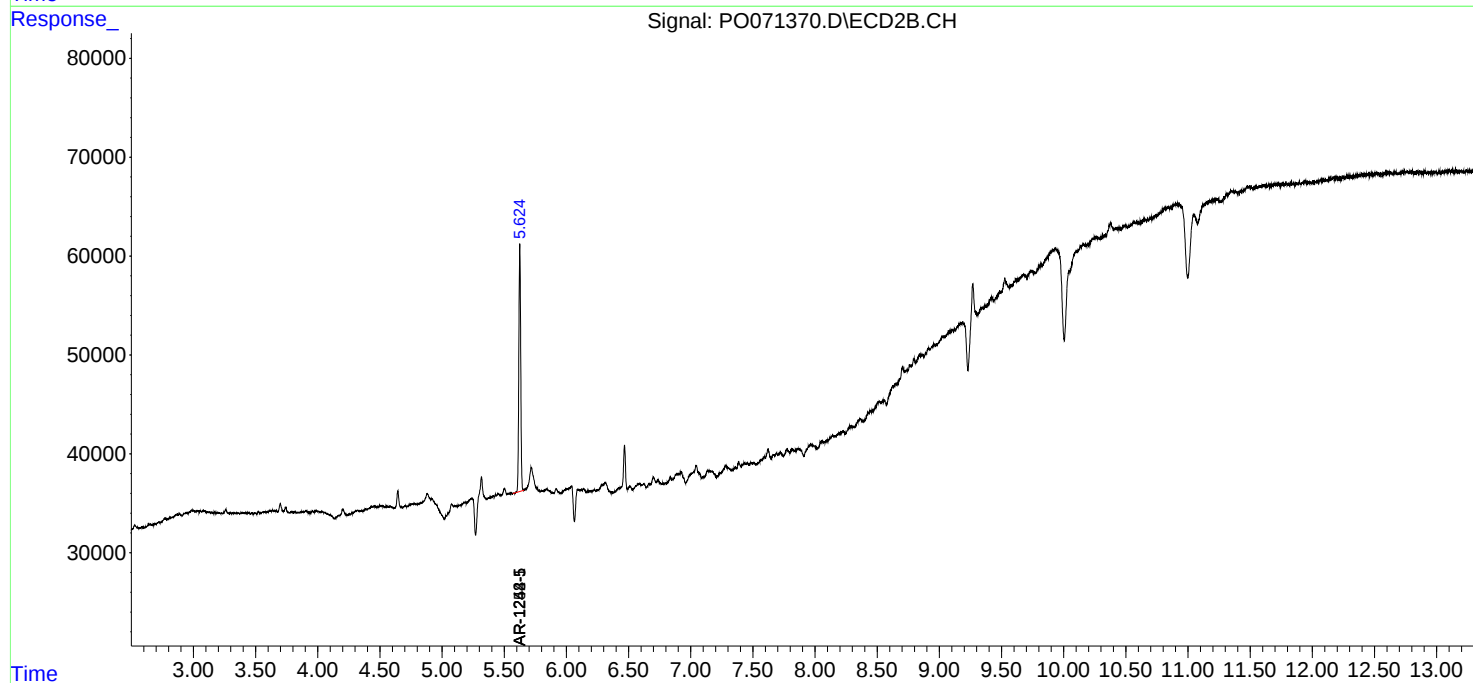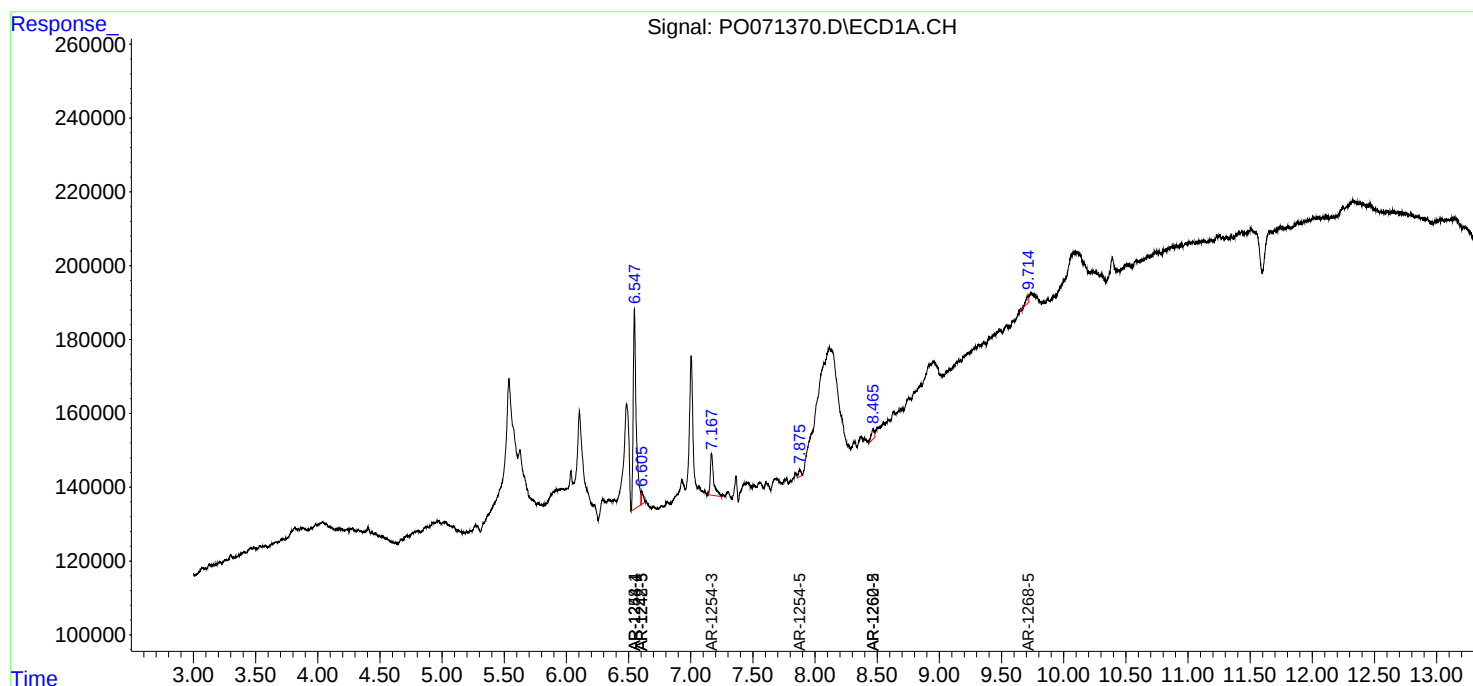


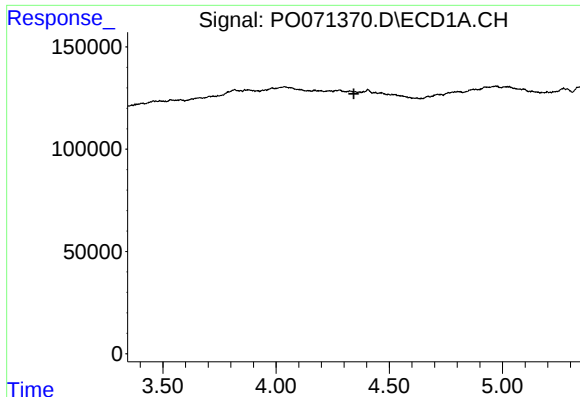

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

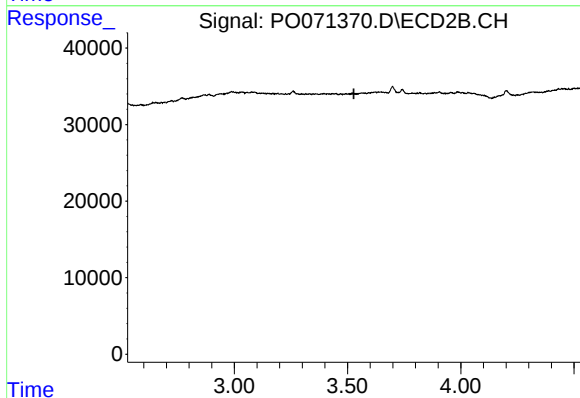


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.528 min
Response: 0
Conc: N.D.

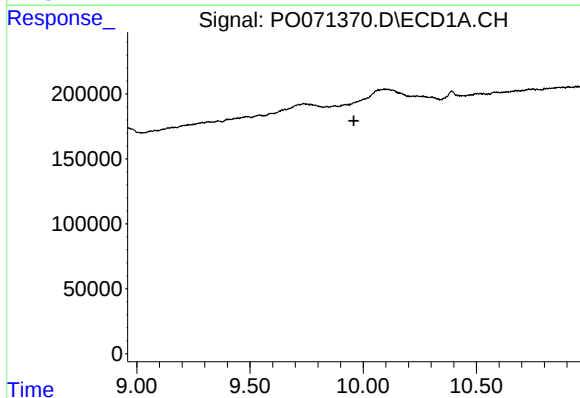


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.959 min
Response: 0
Conc: N.D.

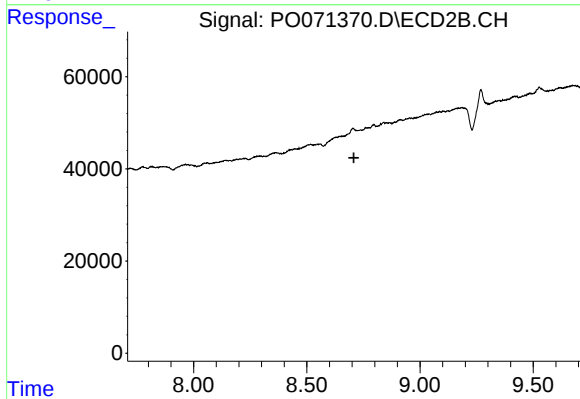

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.708 min
Response: 0
Conc: N.D.

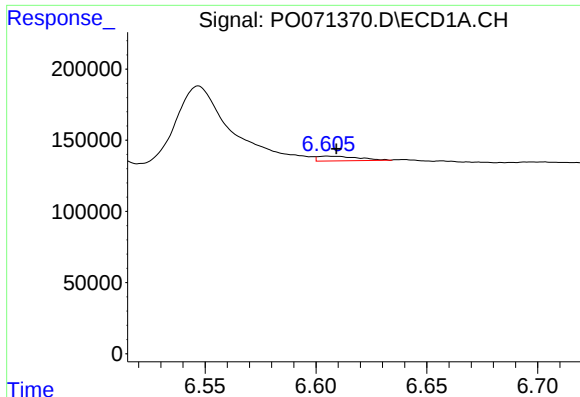

#20 AR-1242-5


R.T.: 6.605 min
Delta R.T.: -0.004 min
Response: 42381
Conc: 19.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

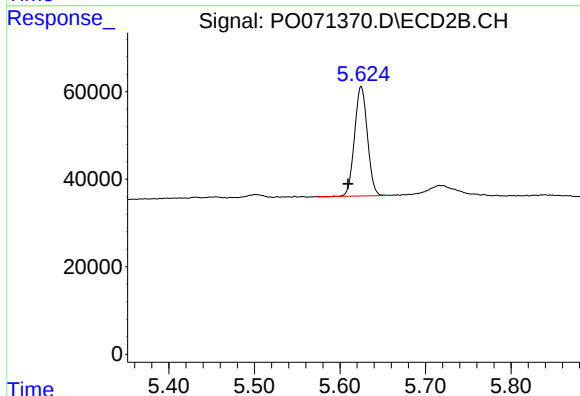


#20 AR-1242-5

R.T.: 5.625 min
Delta R.T.: 0.015 min
Response: 261264
Conc: 188.79 ng/ml

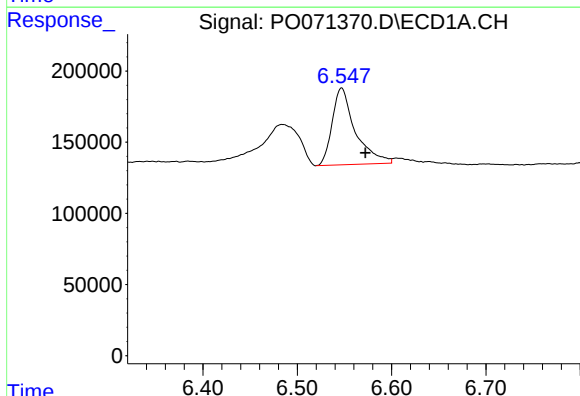


#24 AR-1248-4

R.T.: 6.547 min
Delta R.T.: -0.025 min
Response: 920491
Conc: 253.30 ng/ml

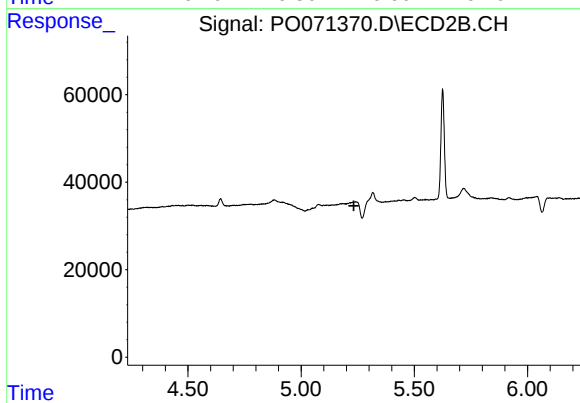

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.233 min
Response: 0
Conc: N.D.

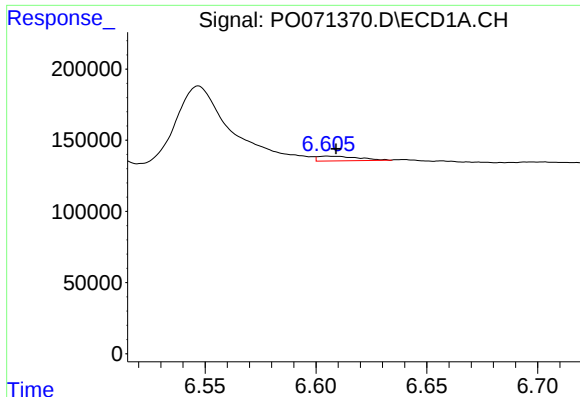

#25 AR-1248-5


R.T.: 6.605 min
Delta R.T.: -0.004 min
Response: 42381
Conc: 12.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

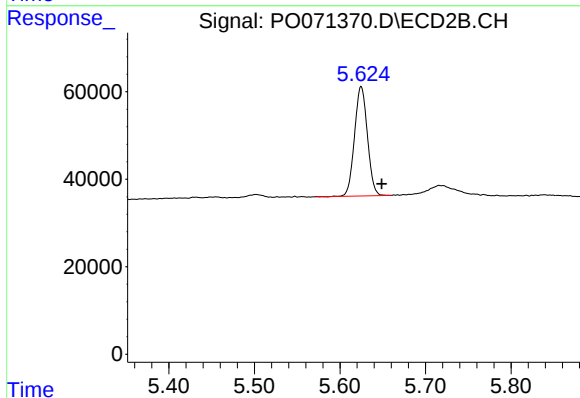


#25 AR-1248-5

R.T.: 5.625 min
Delta R.T.: -0.024 min
Response: 261264
Conc: 152.43 ng/ml

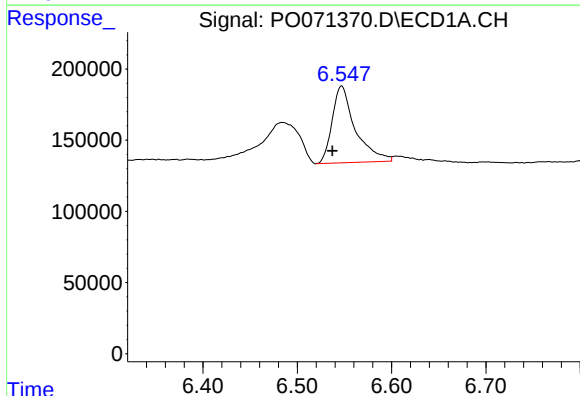


#26 AR-1254-1

R.T.: 6.547 min
Delta R.T.: 0.010 min
Response: 920491
Conc: 262.37 ng/ml

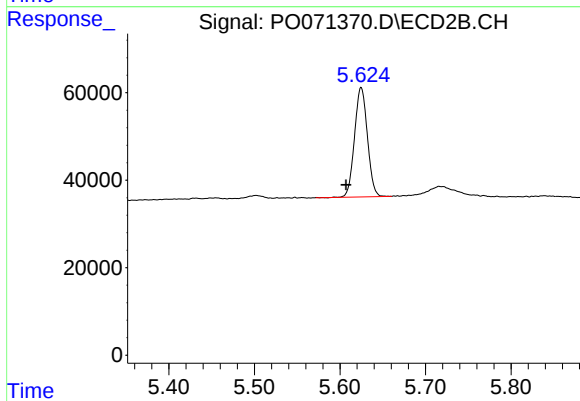

#26 AR-1254-1


R.T.: 5.625 min
Delta R.T.: 0.018 min
Response: 261264
Conc: 98.22 ng/ml

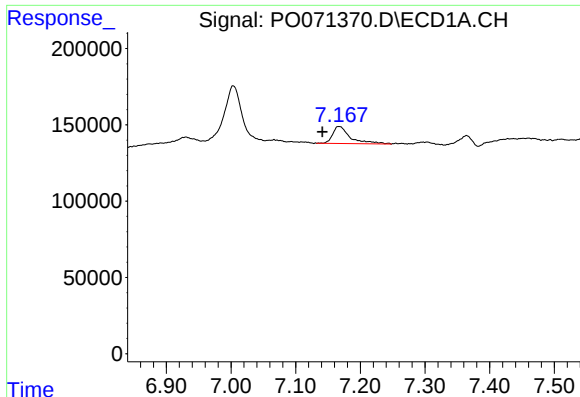

#28 AR-1254-3


R.T.: 7.167 min
Delta R.T.: 0.025 min
Response: 210601
Conc: 35.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

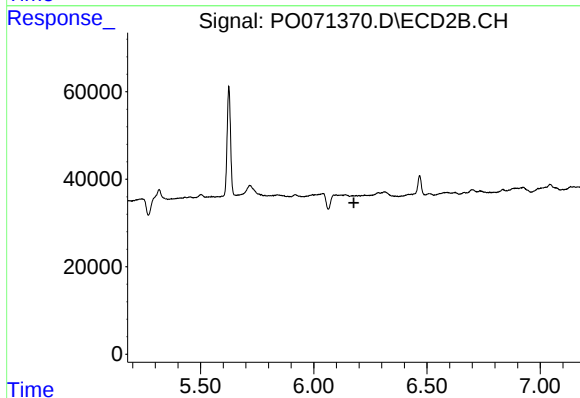


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.177 min
Response: 0
Conc: N.D.

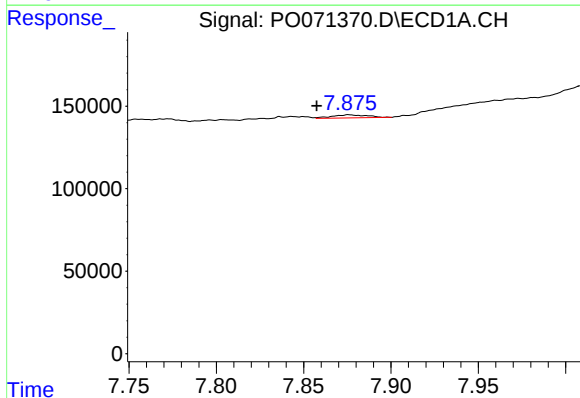


#30 AR-1254-5

R.T.: 7.876 min
Delta R.T.: 0.019 min
Response: 26459
Conc: 4.74 ng/ml

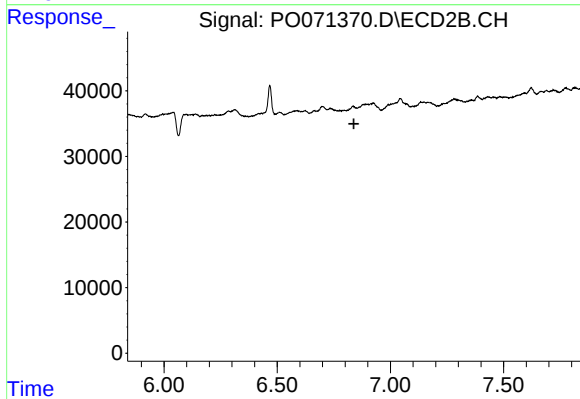

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.839 min
Response: 0
Conc: N.D.

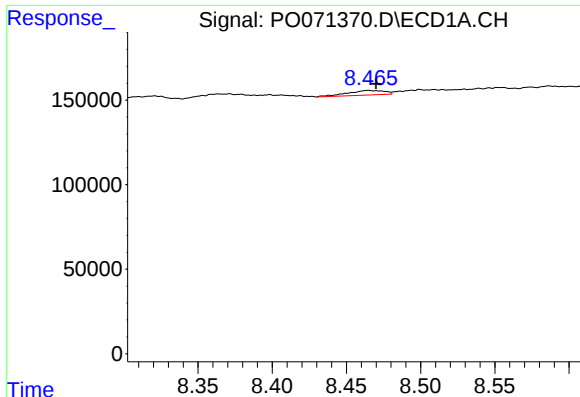

#35 AR-1260-5


R.T.: 8.465 min
Delta R.T.: -0.005 min
Response: 47852
Conc: 3.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

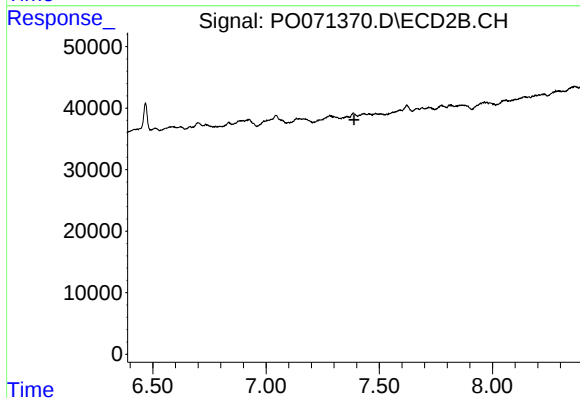


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

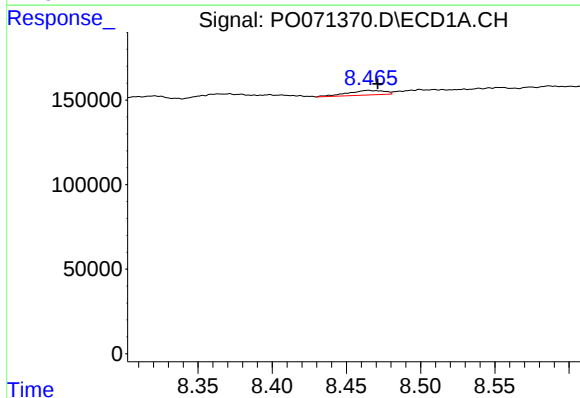


#37 AR-1262-2

R.T.: 8.465 min
Delta R.T.: -0.006 min
Response: 47852
Conc: 3.31 ng/ml

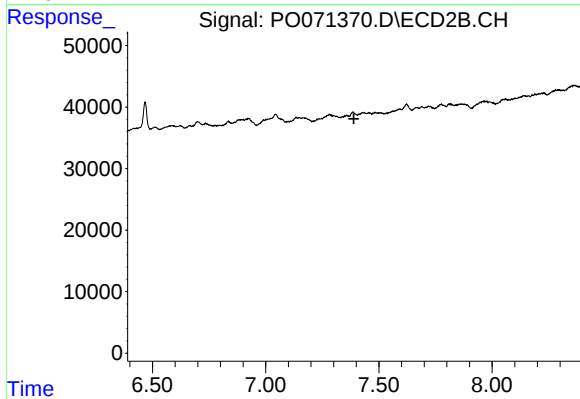

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

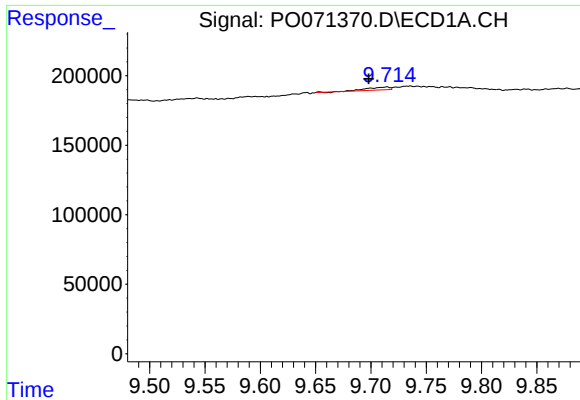

#45 AR-1268-5

R.T.: 9.714 min
Delta R.T.: 0.016 min
Response: 29213
Conc: 0.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

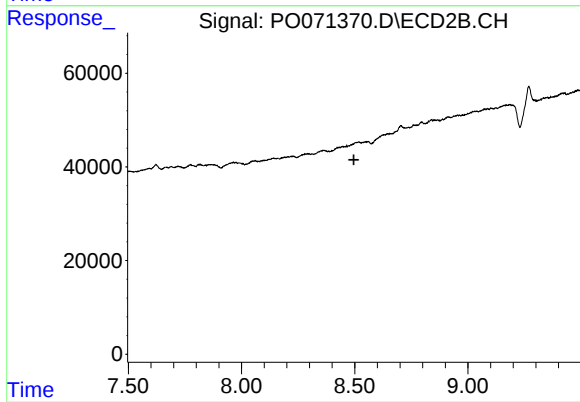

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.496 min
Response: 0
Conc: N.D.