

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091620\
 Data File : P0071371.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Sep 2020 11:06
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 14:03:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.343	3.527	1240562	671623	17.506	17.203
2)	SA Decachlor...	9.957	8.708	1528569	952613	16.391	17.294
Target Compounds							
16)	L4 AR-1242-1	5.601f	0.000	153639	0	65.648	N.D. #
20)	L4 AR-1242-5	0.000	5.628f	0	64639	N.D.	46.707 #
24)	L5 AR-1248-4	6.551f	0.000	544813	0	149.924	N.D. #
25)	L5 AR-1248-5	0.000	5.628f	0	64639	N.D.	37.713 #
26)	L6 AR-1254-1	6.551	5.628f	544813	64639	155.287	24.300 #
28)	L6 AR-1254-3	7.170f	0.000	98912	0	16.632	N.D. #
39)	L8 AR-1262-4	8.808	0.000	79527	0	12.508	N.D. #
42)	L9 AR-1268-2	8.808	0.000	79527	0	5.689	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091620\
Data File : PO071371.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2020 11:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 14:03:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

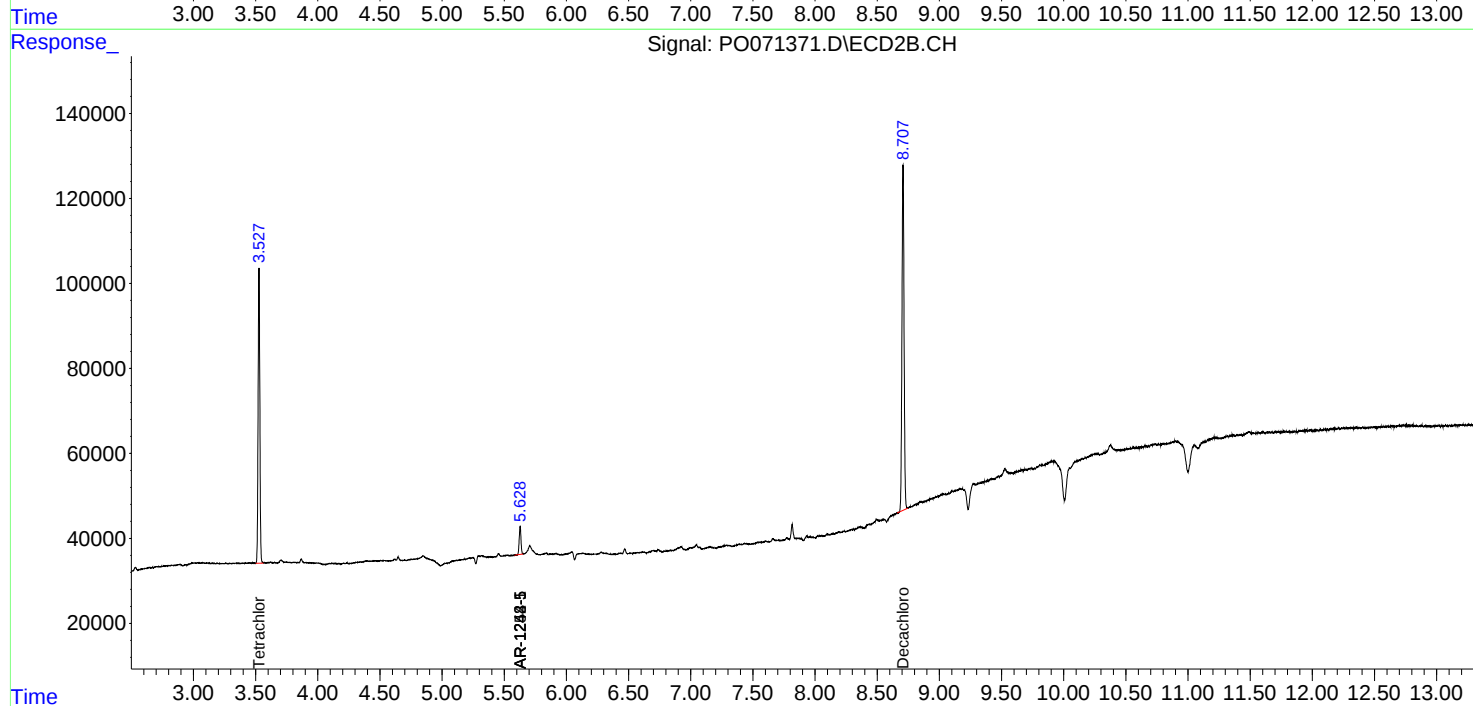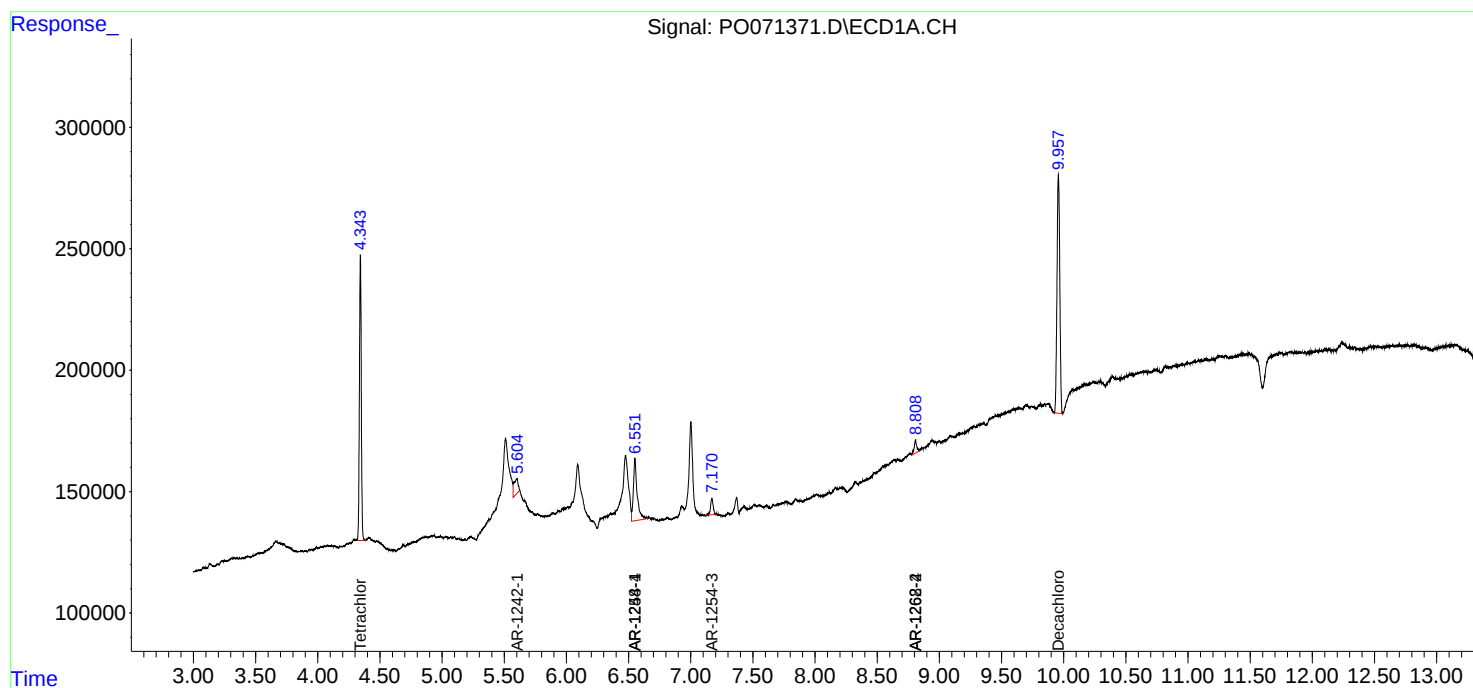


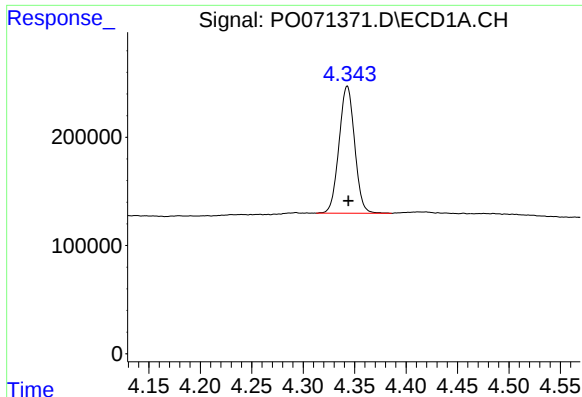

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: -0.001 min
Response: 1240562
Conc: 17.51 ng/ml

Instrument :
ECD_O
ClientSampleId :

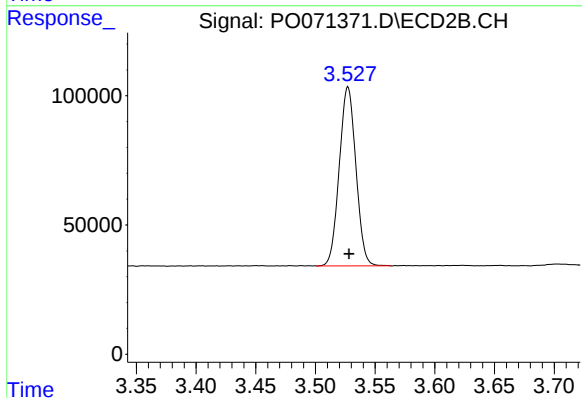


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 671623
Conc: 17.20 ng/ml

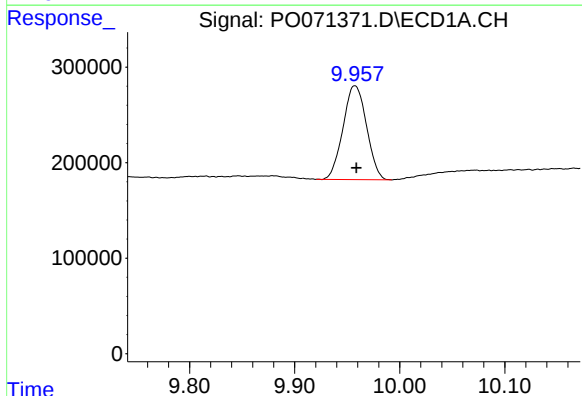


#2 Decachlorobiphenyl

R.T.: 9.957 min
Delta R.T.: -0.001 min
Response: 1528569
Conc: 16.39 ng/ml

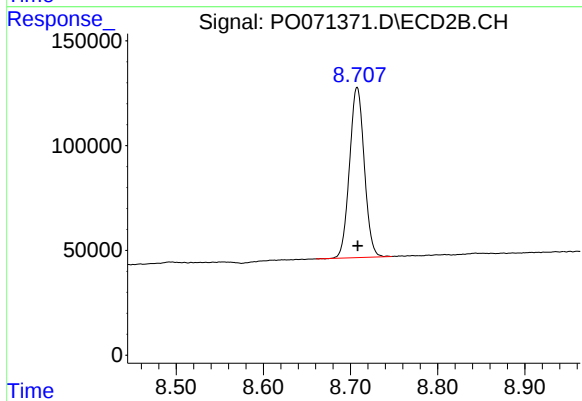

#2 Decachlorobiphenyl


R.T.: 8.708 min
Delta R.T.: 0.000 min
Response: 952613
Conc: 17.29 ng/ml

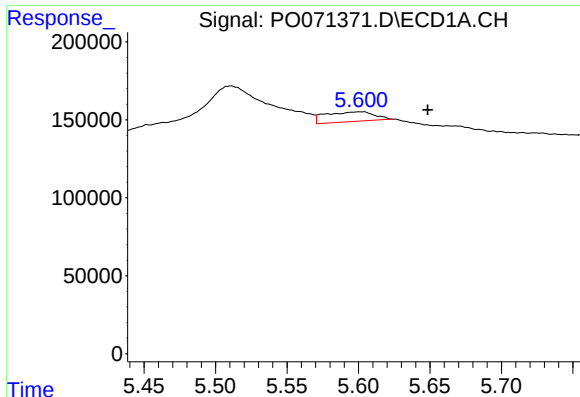

#16 AR-1242-1


R.T.: 5.601 min
Delta R.T.: -0.047 min
Response: 153639
Conc: 65.65 ng/ml

Instrument :
ECD_O
ClientSampleId :

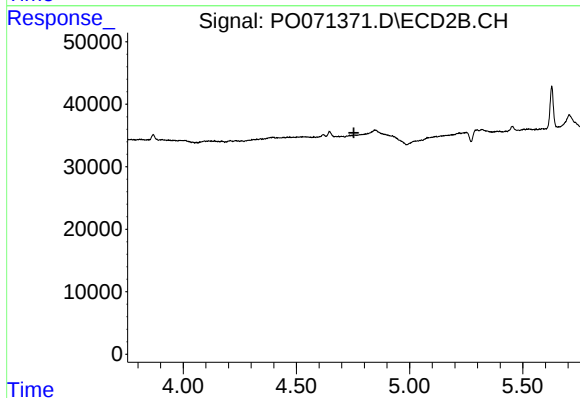


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.754 min
Response: 0
Conc: N.D.

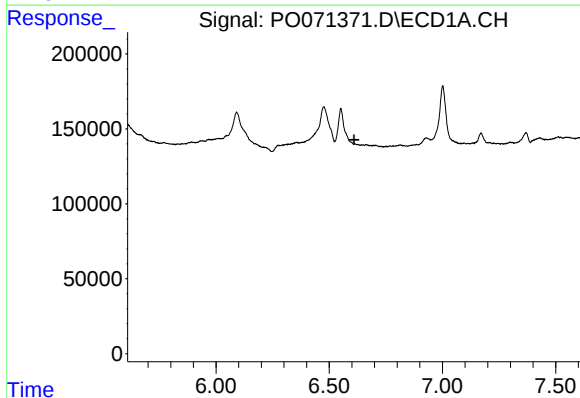


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.609 min
Response: 0
Conc: N.D.

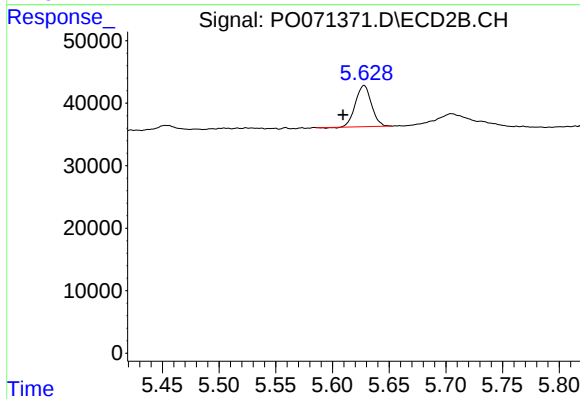

#20 AR-1242-5


R.T.: 5.628 min
Delta R.T.: 0.018 min
Response: 64639
Conc: 46.71 ng/ml

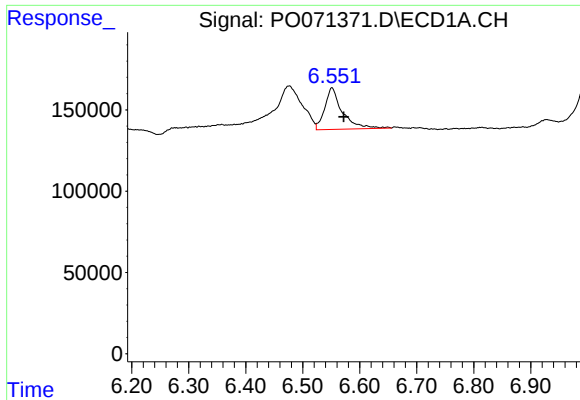

#24 AR-1248-4


R.T.: 6.551 min
Delta R.T.: -0.021 min
Response: 544813
Conc: 149.92 ng/ml

Instrument :
ECD_O
ClientSampleId :

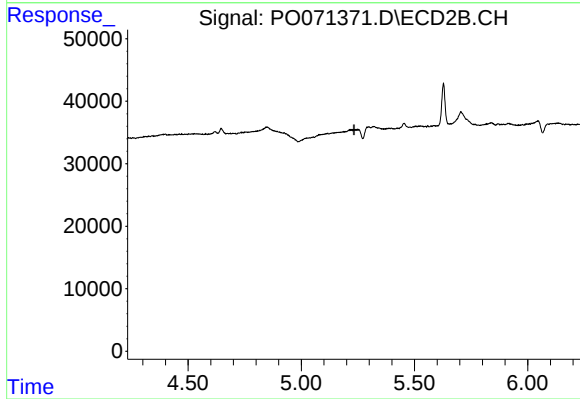


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

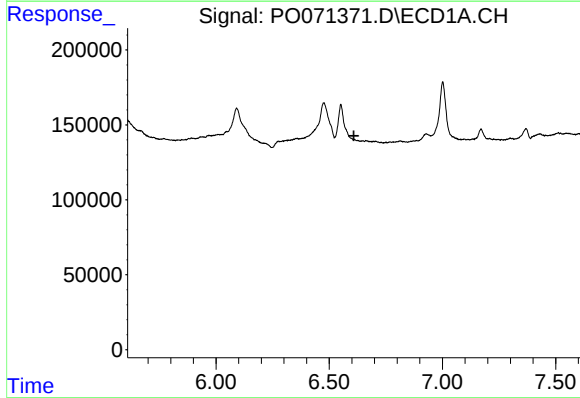


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.609 min
Response: 0
Conc: N.D.

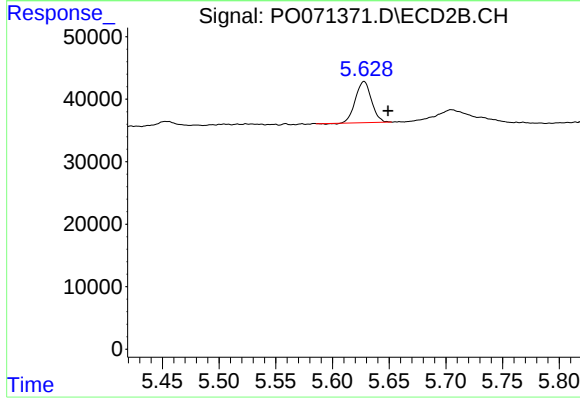

#25 AR-1248-5


R.T.: 5.628 min
Delta R.T.: -0.021 min
Response: 64639
Conc: 37.71 ng/ml

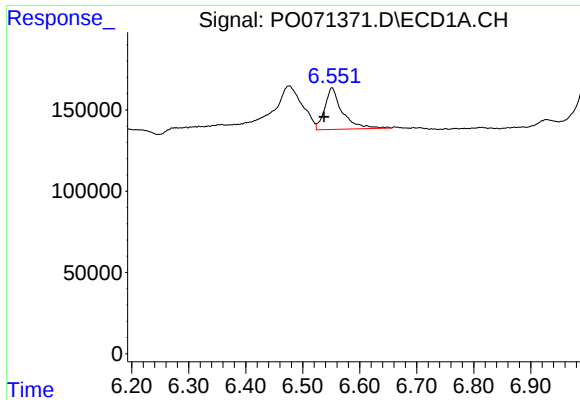

#26 AR-1254-1


R.T.: 6.551 min
Delta R.T.: 0.014 min
Response: 544813
Conc: 155.29 ng/ml

Instrument :
ECD_O
ClientSampleId :

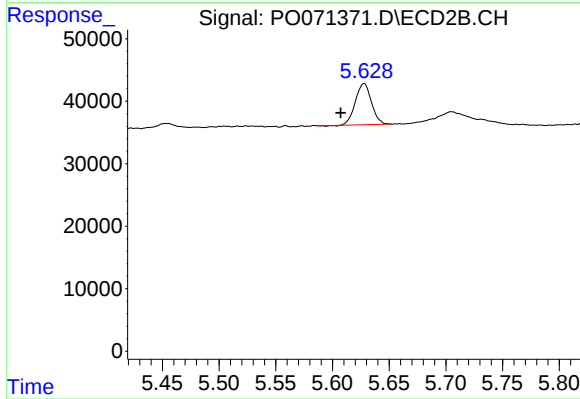


#26 AR-1254-1

R.T.: 5.628 min
Delta R.T.: 0.021 min
Response: 64639
Conc: 24.30 ng/ml

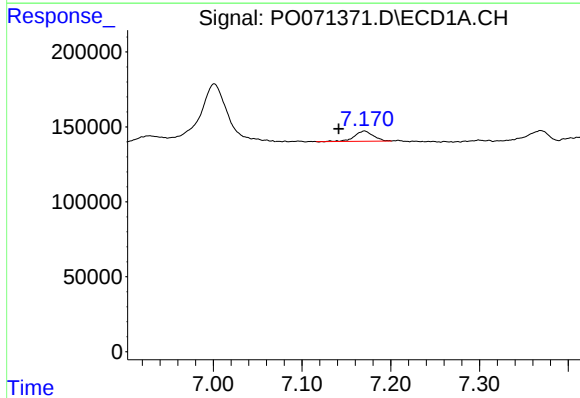


#28 AR-1254-3

R.T.: 7.170 min
Delta R.T.: 0.029 min
Response: 98912
Conc: 16.63 ng/ml

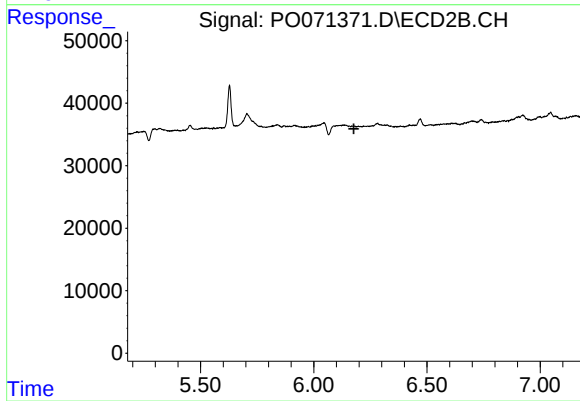

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.177 min
Response: 0
Conc: N.D.

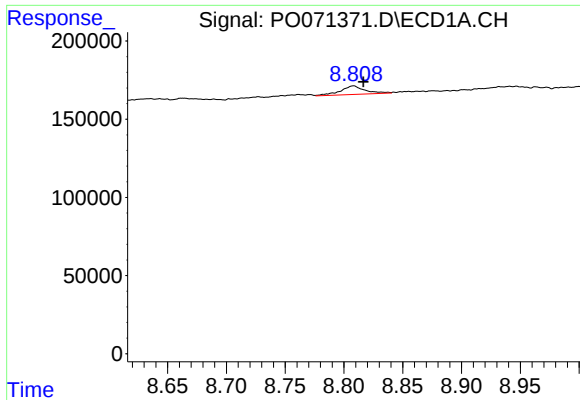

#39 AR-1262-4


R.T.: 8.808 min
Delta R.T.: -0.008 min
Response: 79527
Conc: 12.51 ng/ml

Instrument :
ECD_O
ClientSampleId :

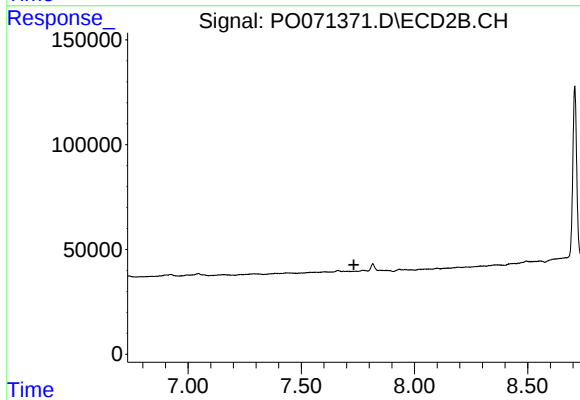


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.732 min
Response: 0
Conc: N.D.

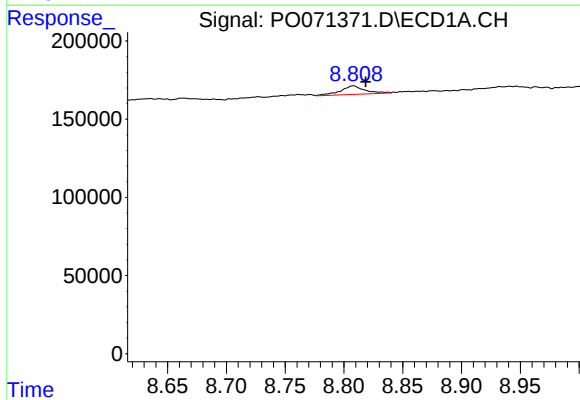

#42 AR-1268-2

R.T.: 8.808 min
Delta R.T.: -0.011 min
Response: 79527
Conc: 5.69 ng/ml

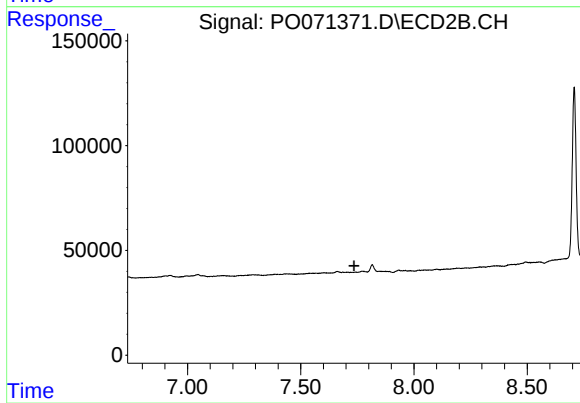

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.735 min
Response: 0
Conc: N.D.