

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091620\
 Data File : P0071383.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Sep 2020 14:45
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 15:30:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.357	3.533	1458797	755400	20.585	19.349
2)	SA Decachlor...	9.968	8.712	1859497	1021485	19.940	18.544
Target Compounds							
20)	L4 AR-1242-5	0.000	5.633f	0	84149	N.D.	60.804 #
24)	L5 AR-1248-4	6.562	0.000	801444	0	220.544	N.D. #
25)	L5 AR-1248-5	0.000	5.633f	0	84149	N.D.	49.096 #
26)	L6 AR-1254-1	6.562f	5.633f	801444	84149	228.435	31.635 #
35)	L7 AR-1260-5	8.495f	0.000	4022	0	0.317	N.D. #
37)	L8 AR-1262-2	8.495f	0.000	4022	0	0.279	N.D. #
39)	L8 AR-1262-4	8.815	0.000	93824	0	14.756	N.D. #
42)	L9 AR-1268-2	8.815	0.000	93824	0	6.711	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091620\
Data File : PO071383.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2020 14:45
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 15:30:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

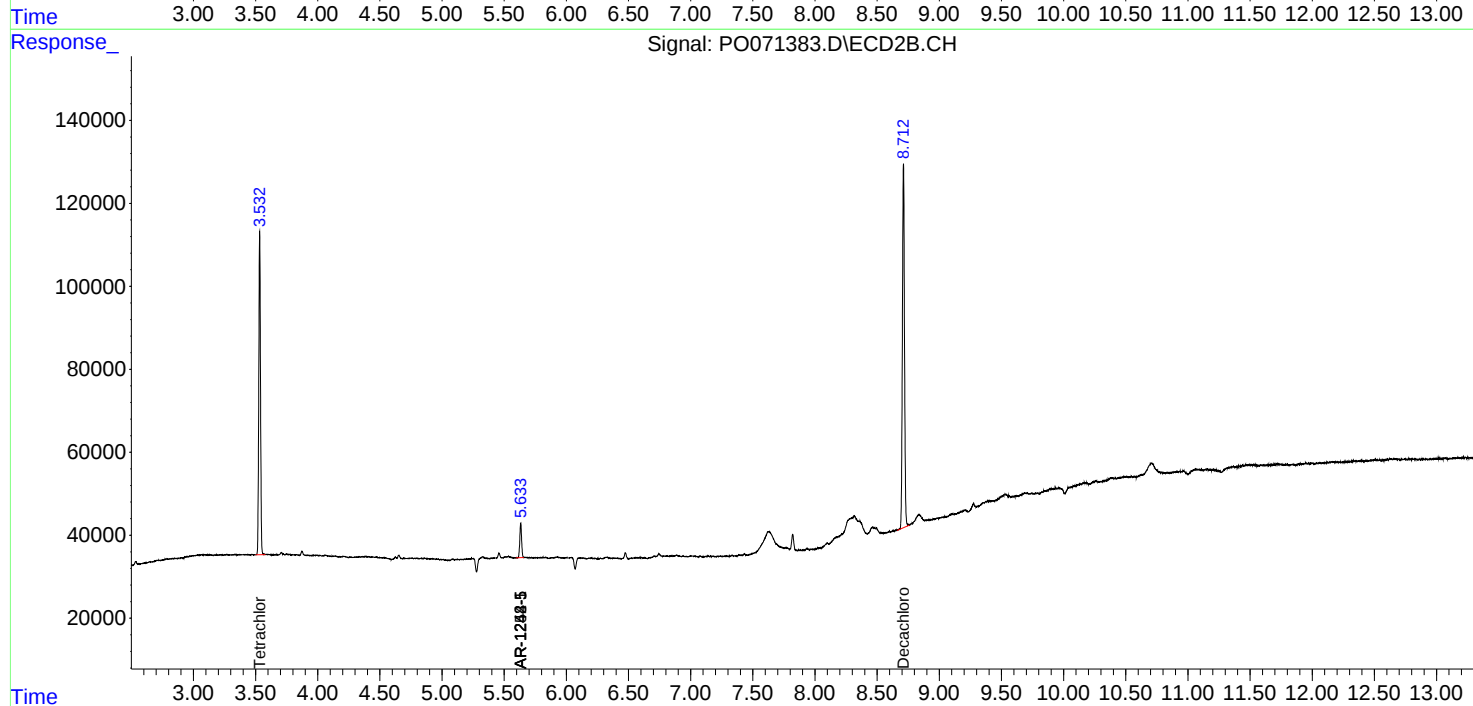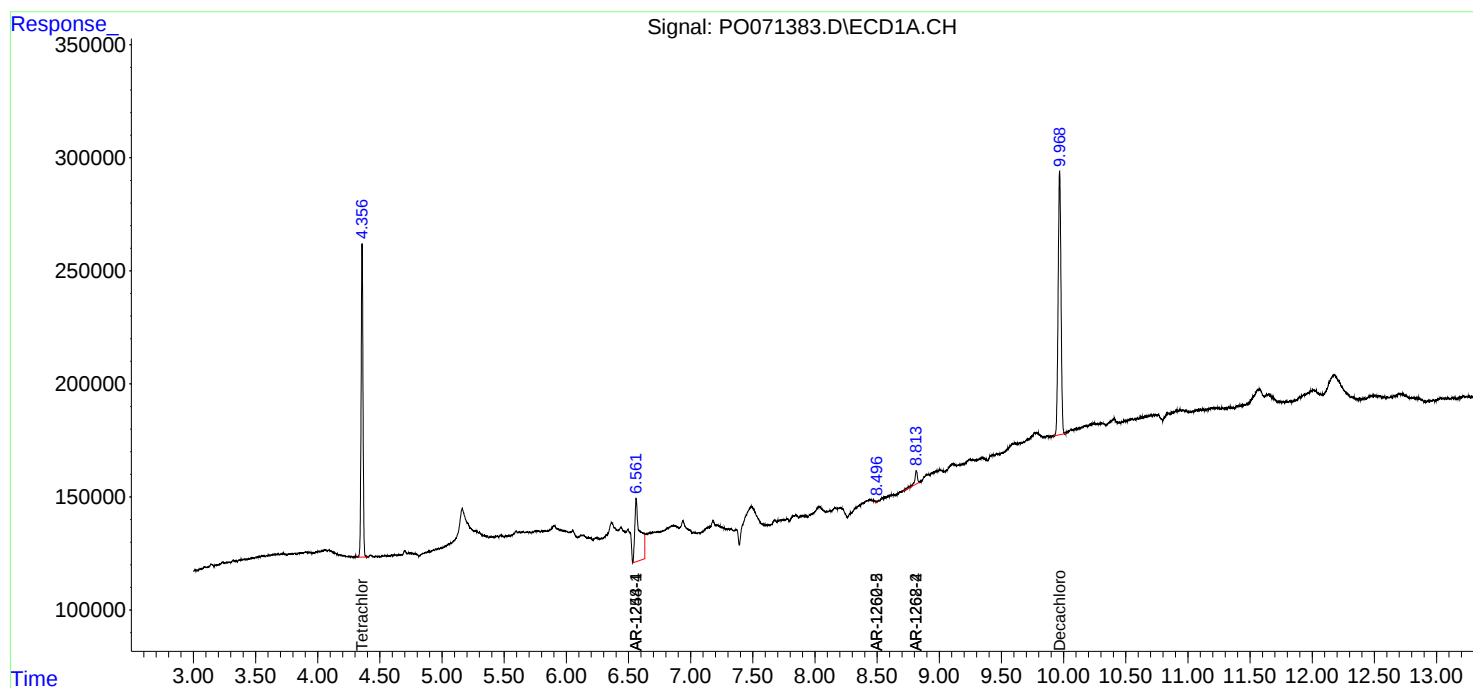


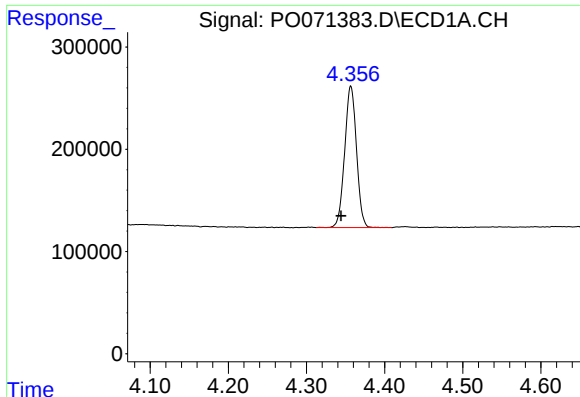

#1 Tetrachloro-m-xylene


R.T.: 4.357 min
Delta R.T.: 0.013 min
Response: 1458797
Conc: 20.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

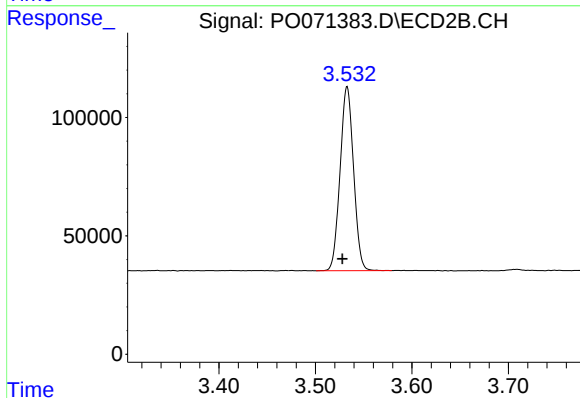


#1 Tetrachloro-m-xylene

R.T.: 3.533 min
Delta R.T.: 0.005 min
Response: 755400
Conc: 19.35 ng/ml

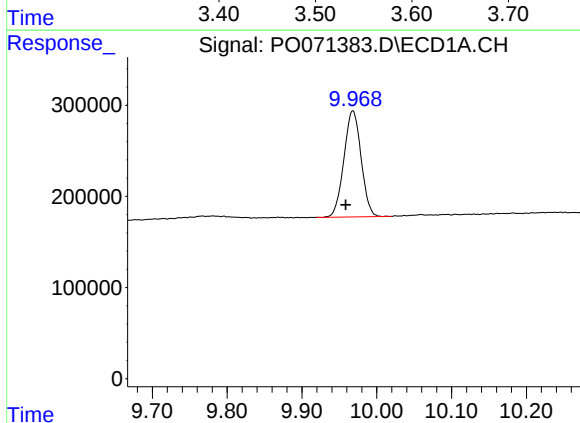


#2 Decachlorobiphenyl

R.T.: 9.968 min
Delta R.T.: 0.009 min
Response: 1859497
Conc: 19.94 ng/ml

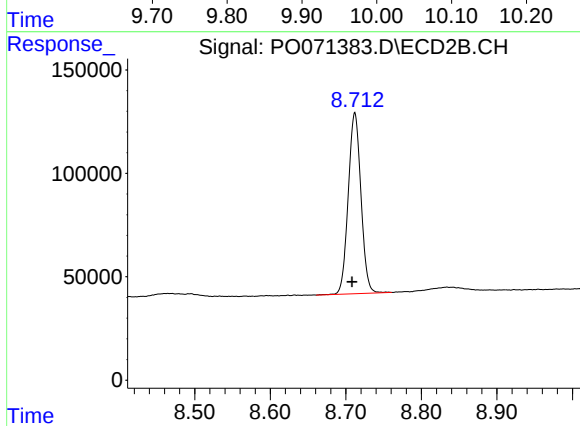

#2 Decachlorobiphenyl


R.T.: 8.712 min
Delta R.T.: 0.004 min
Response: 1021485
Conc: 18.54 ng/ml

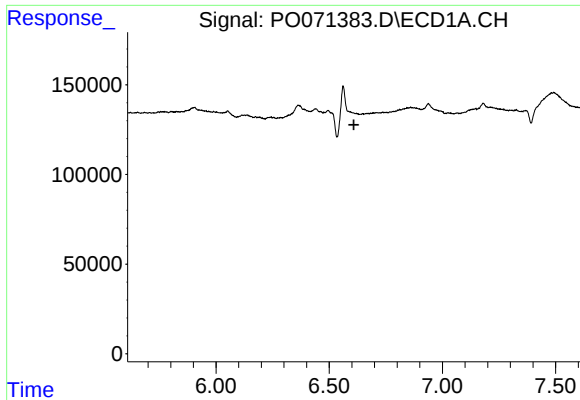

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.609 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

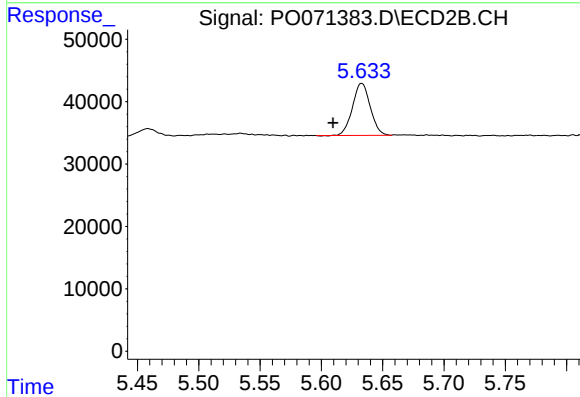


#20 AR-1242-5

R.T.: 5.633 min
Delta R.T.: 0.024 min
Response: 84149
Conc: 60.80 ng/ml

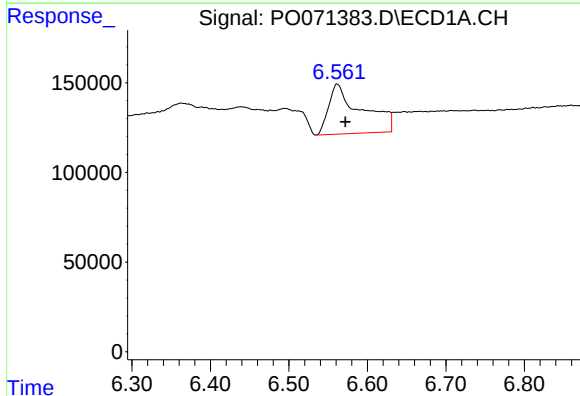


#24 AR-1248-4

R.T.: 6.562 min
Delta R.T.: -0.011 min
Response: 801444
Conc: 220.54 ng/ml

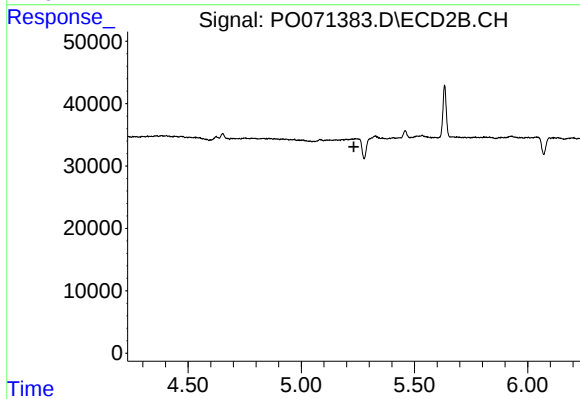

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.233 min
Response: 0
Conc: N.D.

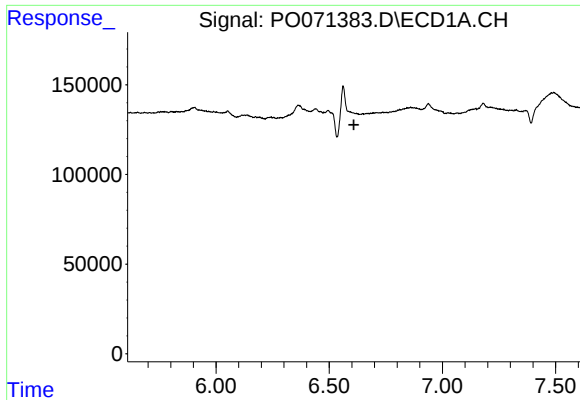

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.609 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

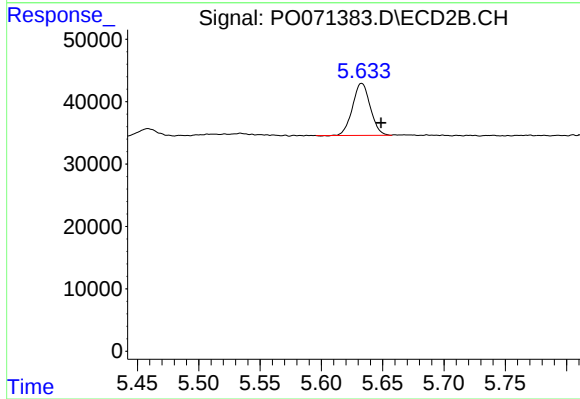


#25 AR-1248-5

R.T.: 5.633 min
Delta R.T.: -0.016 min
Response: 84149
Conc: 49.10 ng/ml

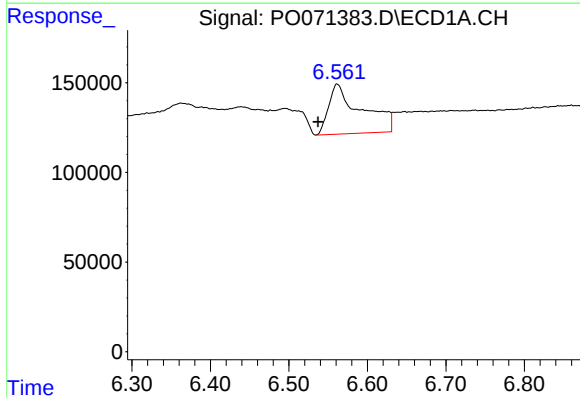


#26 AR-1254-1

R.T.: 6.562 min
Delta R.T.: 0.024 min
Response: 801444
Conc: 228.43 ng/ml

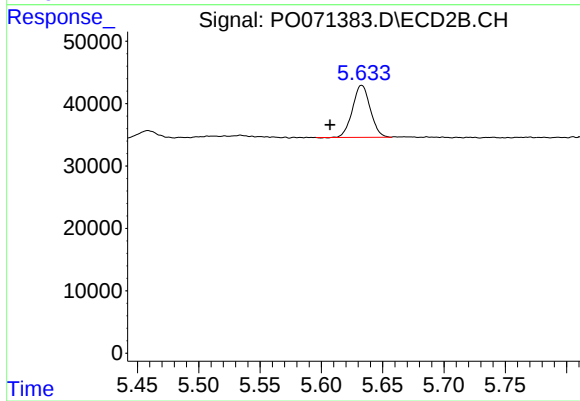

#26 AR-1254-1


R.T.: 5.633 min
Delta R.T.: 0.026 min
Response: 84149
Conc: 31.63 ng/ml

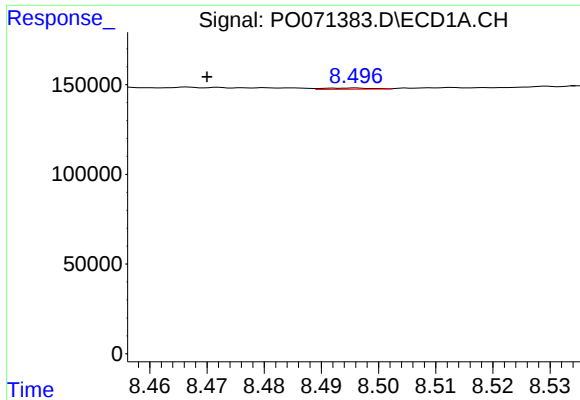

#35 AR-1260-5


R.T.: 8.495 min
Delta R.T.: 0.025 min
Response: 4022
Conc: 0.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

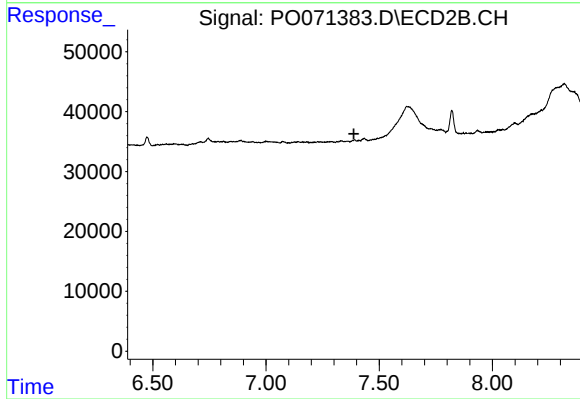


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

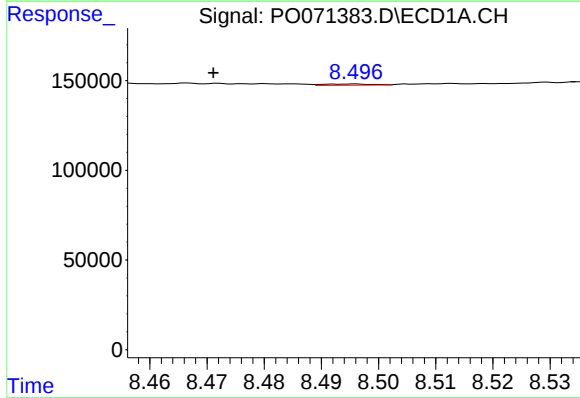


#37 AR-1262-2

R.T.: 8.495 min
Delta R.T.: 0.024 min
Response: 4022
Conc: 0.28 ng/ml

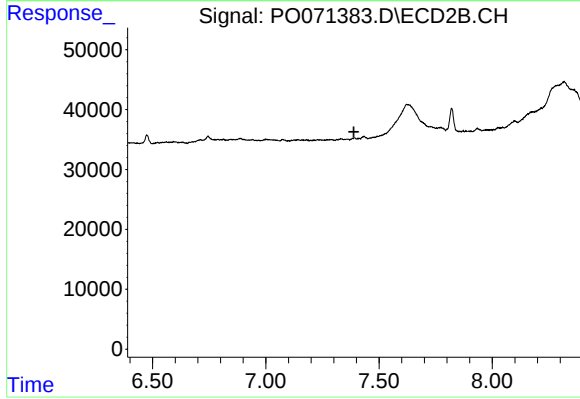

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

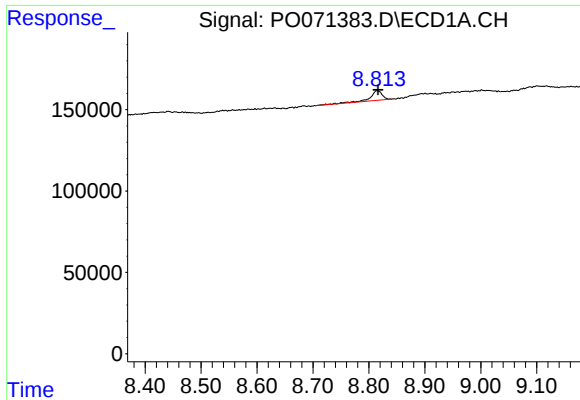

#39 AR-1262-4


R.T.: 8.815 min
Delta R.T.: -0.001 min
Response: 93824
Conc: 14.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

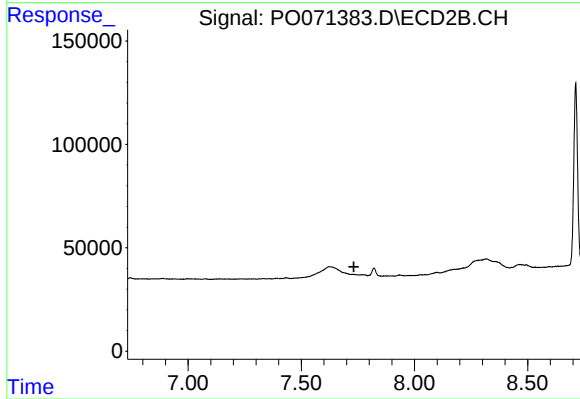


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.732 min
Response: 0
Conc: N.D.

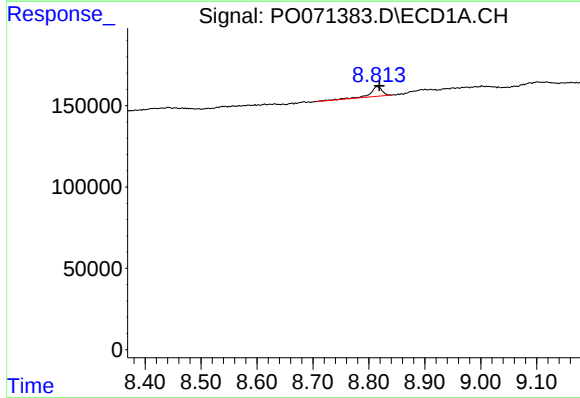

#42 AR-1268-2

R.T.: 8.815 min
Delta R.T.: -0.003 min
Response: 93824
Conc: 6.71 ng/ml

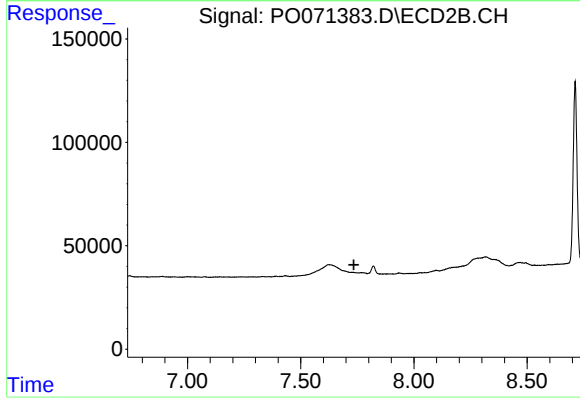

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.735 min
Response: 0
Conc: N.D.