

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091620\
 Data File : P0071378.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Sep 2020 13:06
 Operator : DD\AJ
 Sample : L4015-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 REACTOR-6E-(A-D-0-4)

Manual Integrations
 APPROVED

Ankita
 9/17/2020 1:51:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 14:05:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.528	1593141	883983	22.481	22.642m
2) SA Decachlor...	9.958	8.707	1879629	1077199	20.156	19.556
Target Compounds						
31) L7 AR-1260-1	7.305	6.313	11431988	6042577	2521.183	2168.843
32) L7 AR-1260-2	7.570	6.514	20135651	8932419	2888.334m	2471.093
33) L7 AR-1260-3	7.929	6.660	14121192	6462485	2330.124	2002.649
34) L7 AR-1260-4	8.155	7.136	13929081	5663955	2433.301	1955.197
35) L7 AR-1260-5	8.471	7.388	34599478	16738198	2728.574	2207.436

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091620\
Data File : PO071378.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2020 13:06
Operator : DD\AJ
Sample : L4015-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
REACTOR-6E-(A-D-0-4)


Manual Integrations
APPROVED

Ankita
9/17/2020 1:51:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 14:05:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

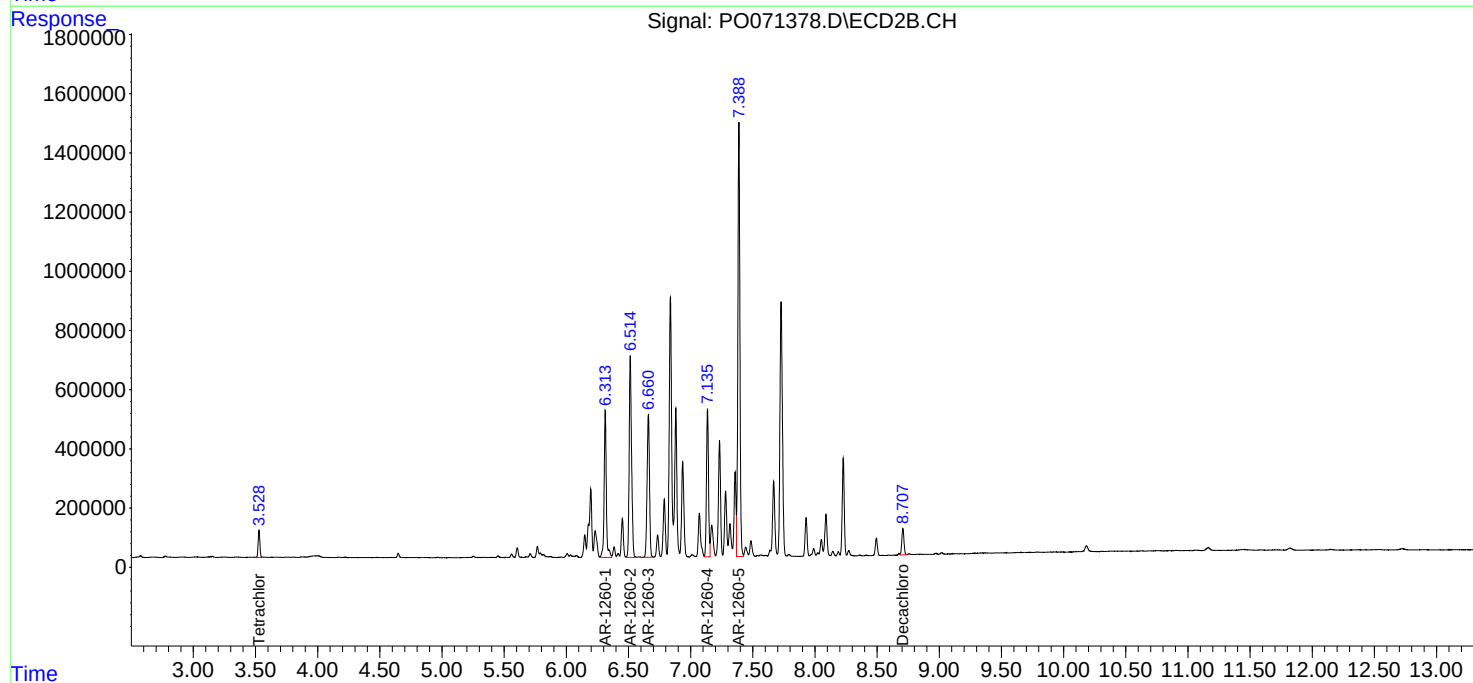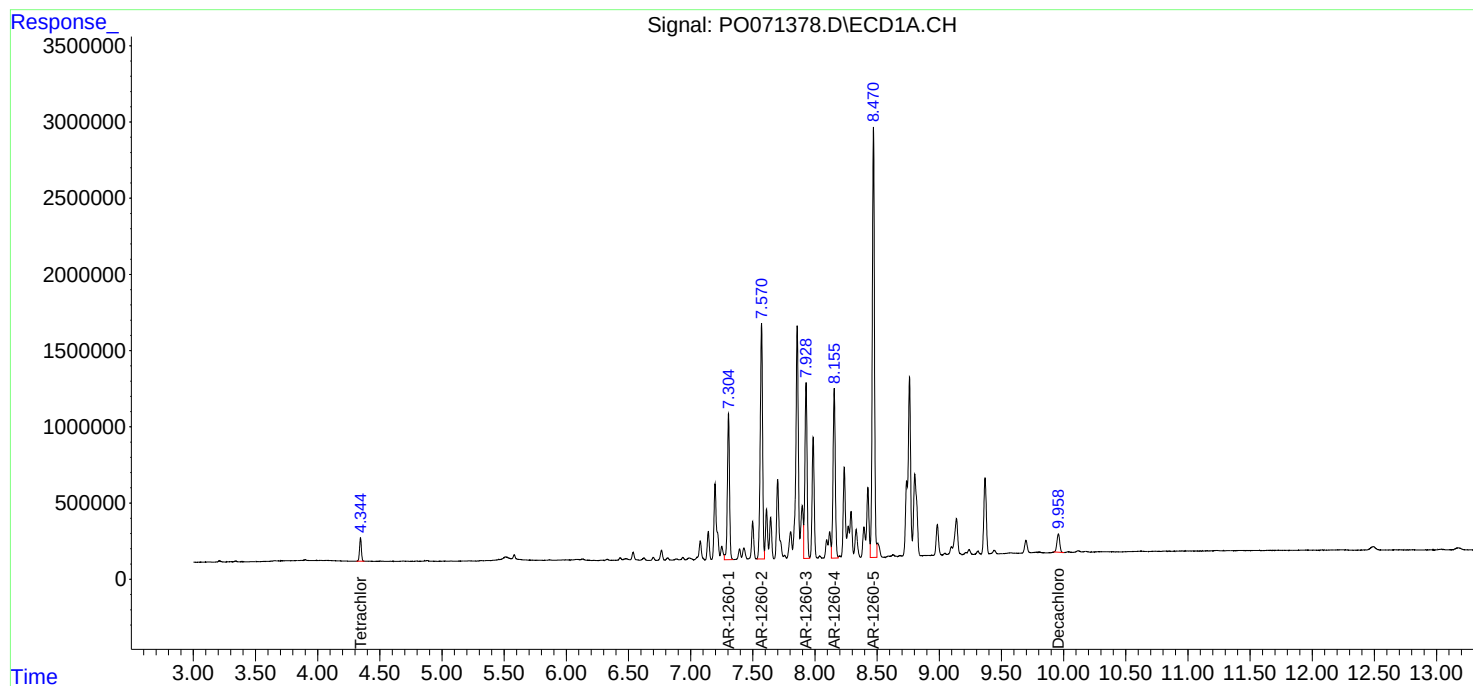

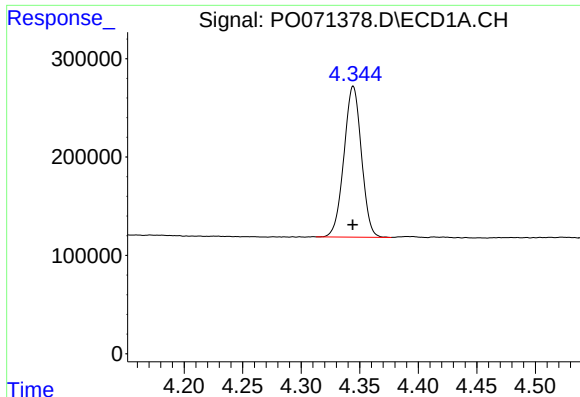


#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 1593141
Conc: 22.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
REACTOR-6E-(A-D-0-4)


Manual Integrations
APPROVED

Ankita
9/17/2020 1:51:55 PM

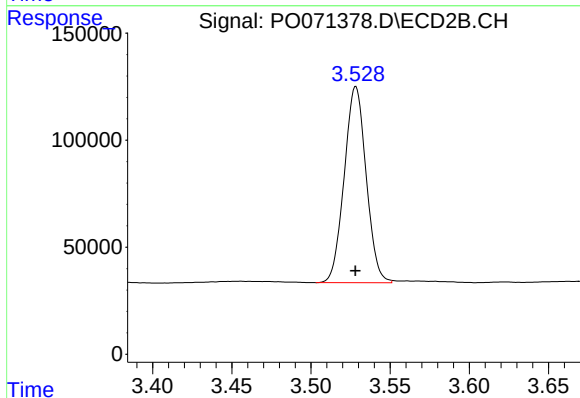


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 883983
Conc: 22.64 ng/ml m

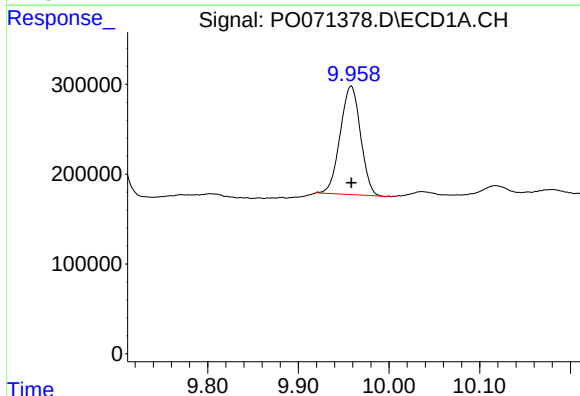


#2 Decachlorobiphenyl

R.T.: 9.958 min
Delta R.T.: 0.000 min
Response: 1879629
Conc: 20.16 ng/ml

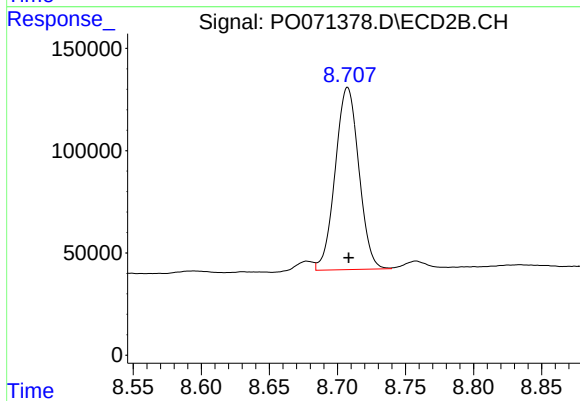

#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.000 min
Response: 1077199
Conc: 19.56 ng/ml

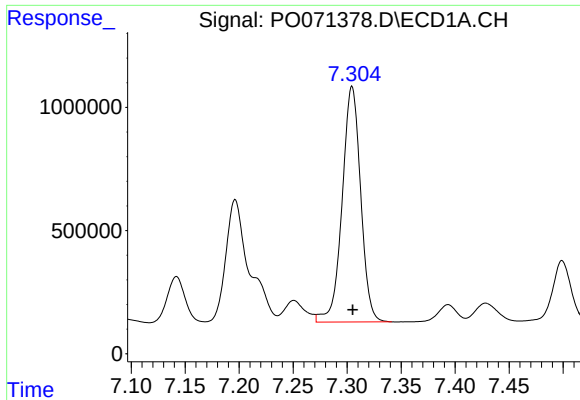


#31 AR-1260-1

R.T.: 7.305 min
Delta R.T.: 0.000 min
Response: 11431988
Conc: 2521.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
REACTOR-6E-(A-D-0-4)


Manual Integrations
APPROVED

Ankita
9/17/2020 1:51:55 PM

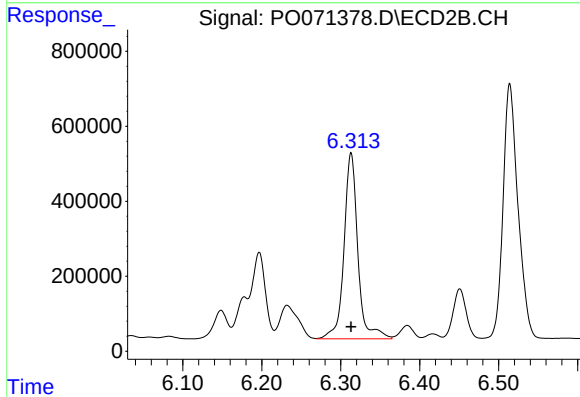


#31 AR-1260-1

R.T.: 6.313 min
Delta R.T.: 0.000 min
Response: 6042577
Conc: 2168.84 ng/ml

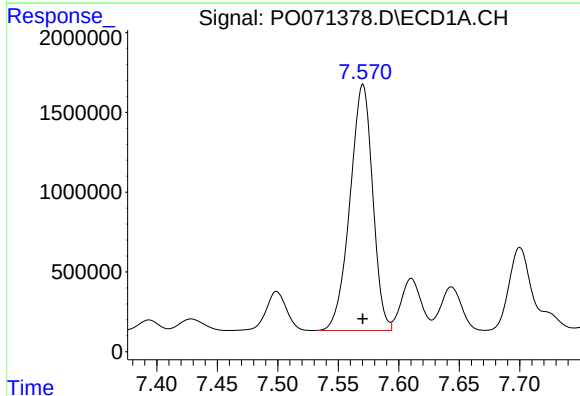


#32 AR-1260-2

R.T.: 7.570 min
Delta R.T.: 0.000 min
Response: 20135651
Conc: 2888.33 ng/ml m

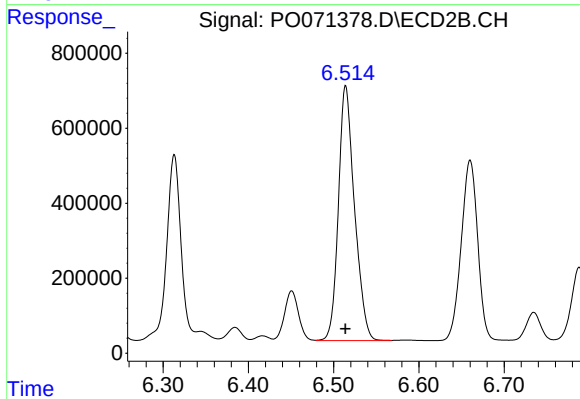

#32 AR-1260-2

R.T.: 6.514 min
Delta R.T.: 0.000 min
Response: 8932419
Conc: 2471.09 ng/ml

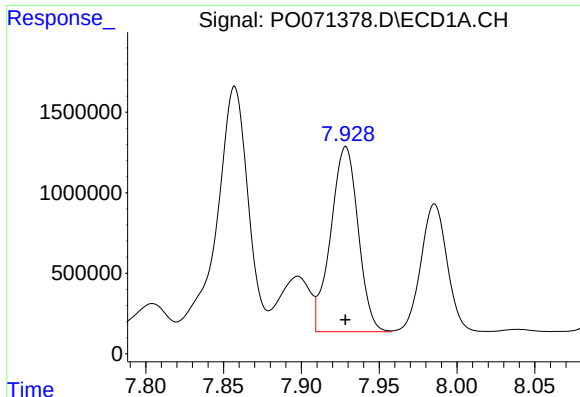


#33 AR-1260-3

R.T.: 7.929 min
Delta R.T.: 0.000 min
Response: 14121192
Conc: 2330.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
REACTOR-6E-(A-D-0-4)


Manual Integrations
APPROVED

Ankita
9/17/2020 1:51:55 PM

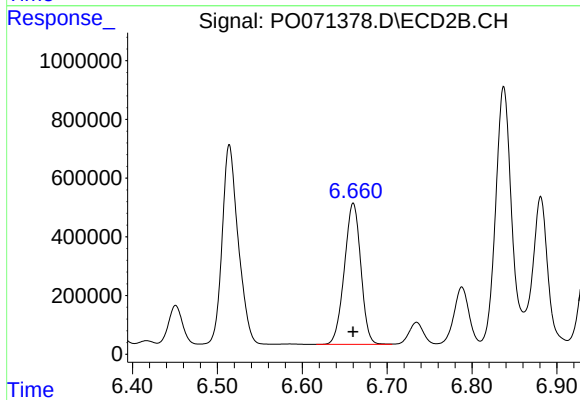


#33 AR-1260-3

R.T.: 6.660 min
Delta R.T.: 0.000 min
Response: 6462485
Conc: 2002.65 ng/ml

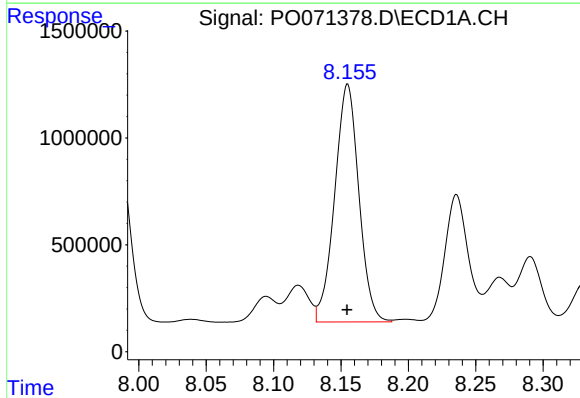


#34 AR-1260-4

R.T.: 8.155 min
Delta R.T.: 0.000 min
Response: 13929081
Conc: 2433.30 ng/ml

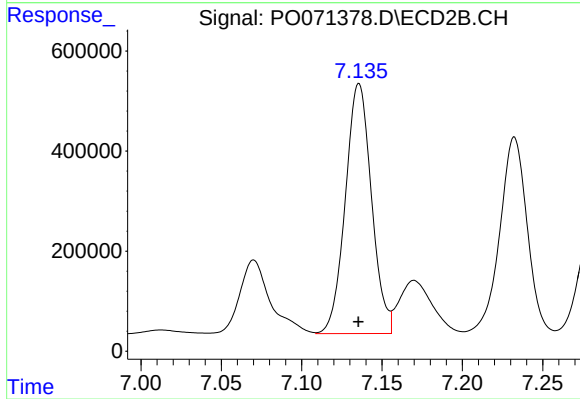

#34 AR-1260-4

R.T.: 7.136 min
Delta R.T.: 0.000 min
Response: 5663955
Conc: 1955.20 ng/ml

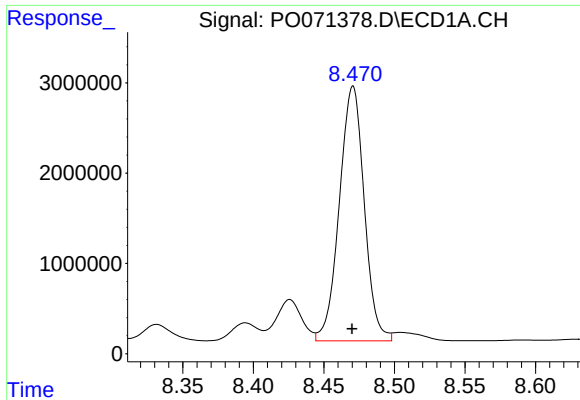


#35 AR-1260-5

R.T.: 8.471 min
Delta R.T.: 0.000 min
Response: 34599478
Conc: 2728.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
REACTOR-6E-(A-D-0-4)

Manual Integrations
APPROVED

Ankita
9/17/2020 1:51:55 PM

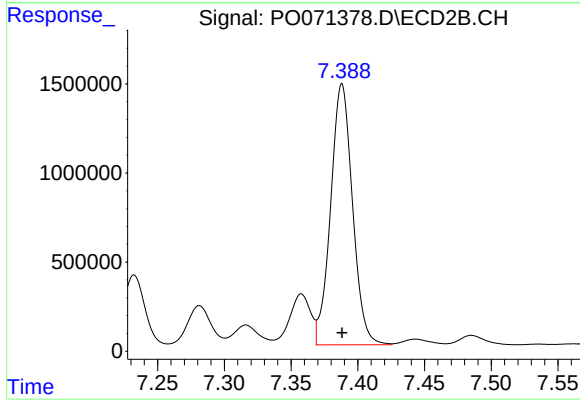

#35 AR-1260-5

R.T.: 7.388 min
Delta R.T.: 0.000 min
Response: 16738198
Conc: 2207.44 ng/ml