

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091620\
 Data File : P0071387.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Sep 2020 15:53
 Operator : DD\AJ
 Sample : L4015-01DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 REACTOR-6E-(A-D-0-4)DL

Manual Integrations
 APPROVED

Ankita
 9/17/2020 1:52:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 17:49:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.527	302174	171128	4.264	4.383
2) SA Decachlor...	9.955	8.706	385449	245136	4.133	4.450
Target Compounds						
31) L7 AR-1260-1	7.303	6.312	2512503	1300005	554.101	466.607
32) L7 AR-1260-2	7.568	6.513	4131134	1963091	592.585m	543.076
33) L7 AR-1260-3	7.927	6.659	2936665	1441234	484.576	446.622
34) L7 AR-1260-4	8.153	7.134	2905146	1251148	507.506	431.896
35) L7 AR-1260-5	8.468	7.387	6989790	3459292	551.227	456.212

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091620\
Data File : PO071387.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2020 15:53
Operator : DD\AJ
Sample : L4015-01DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
REACTOR-6E-(A-D-0-4)DL


Manual Integrations
APPROVED

Ankita
9/17/2020 1:52:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 17:49:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

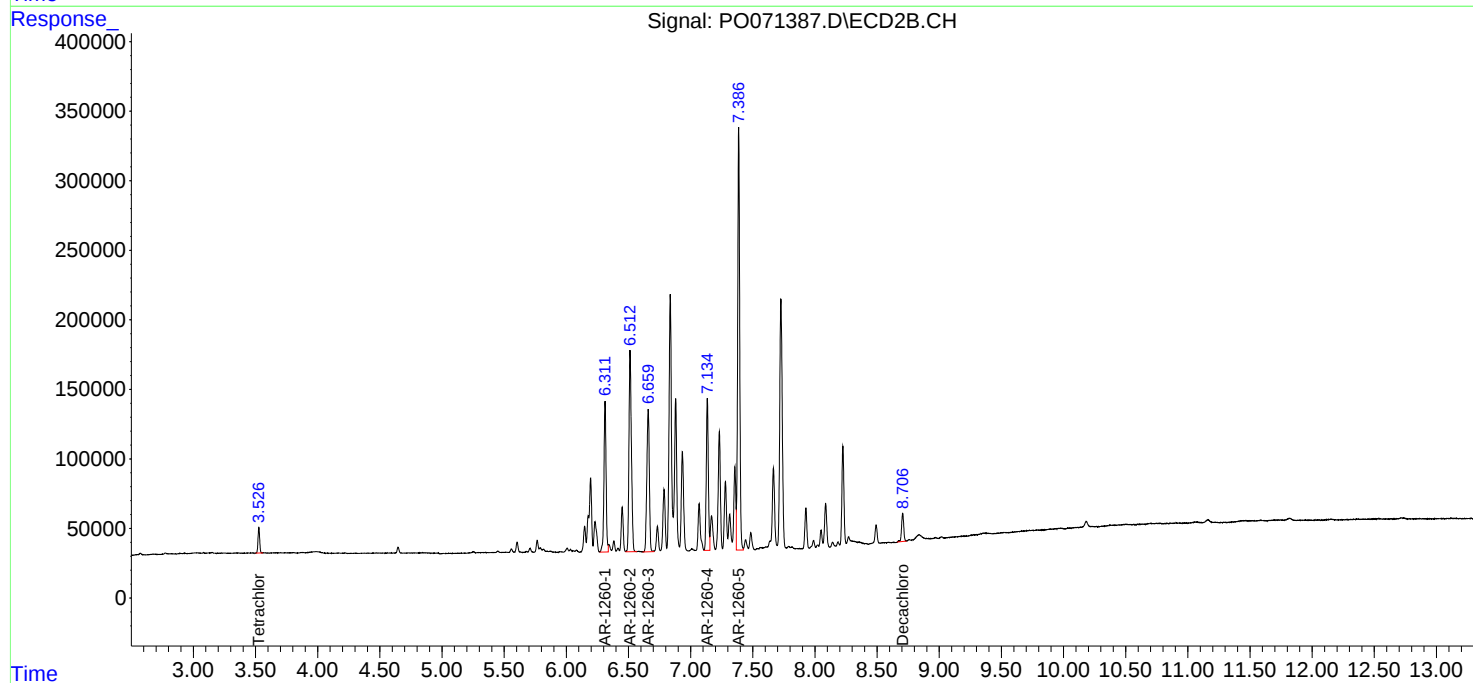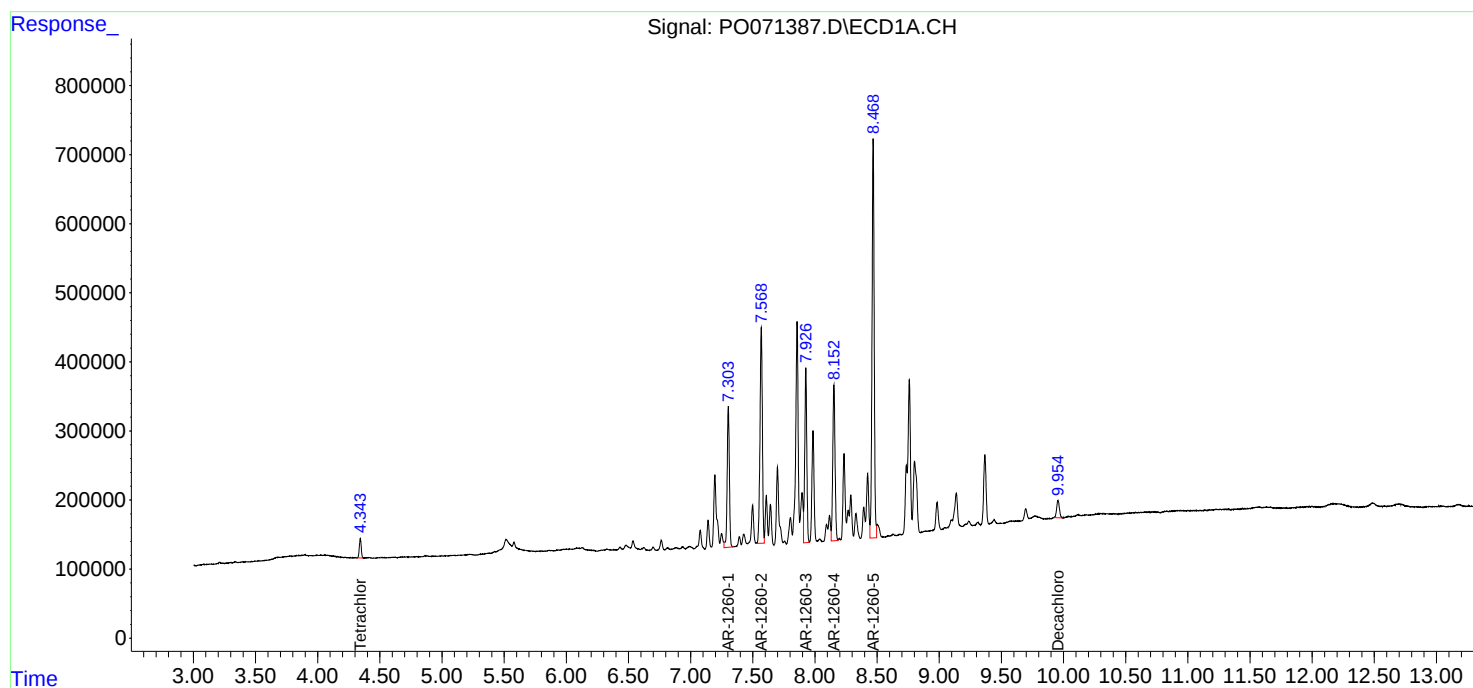

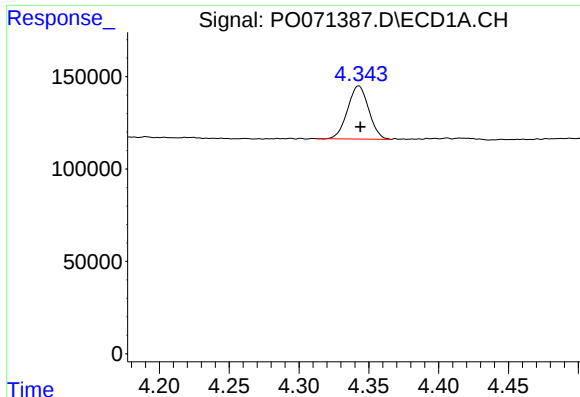


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: -0.001 min
Response: 302174
Conc: 4.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
REACTOR-6E-(A-D-0-4)DL


Manual Integrations
APPROVED

Ankita
9/17/2020 1:52:07 PM

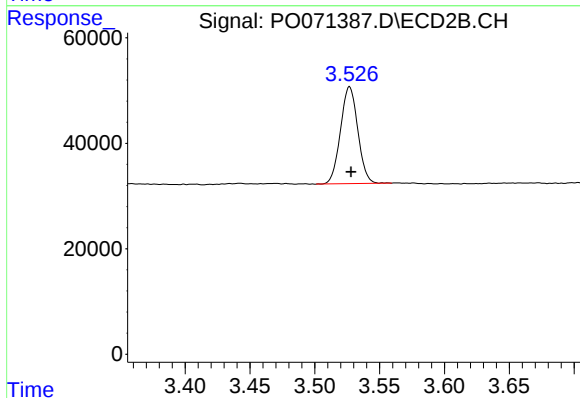


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: -0.001 min
Response: 171128
Conc: 4.38 ng/ml

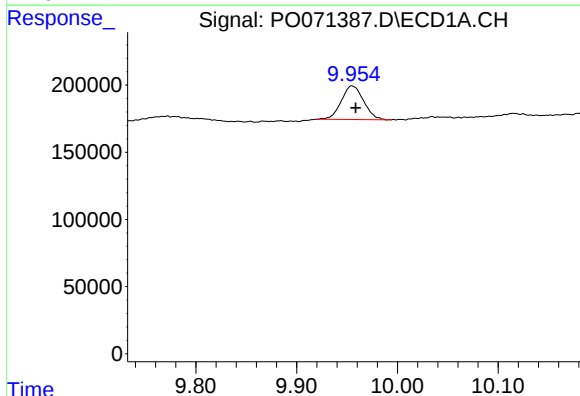


#2 Decachlorobiphenyl

R.T.: 9.955 min
Delta R.T.: -0.004 min
Response: 385449
Conc: 4.13 ng/ml

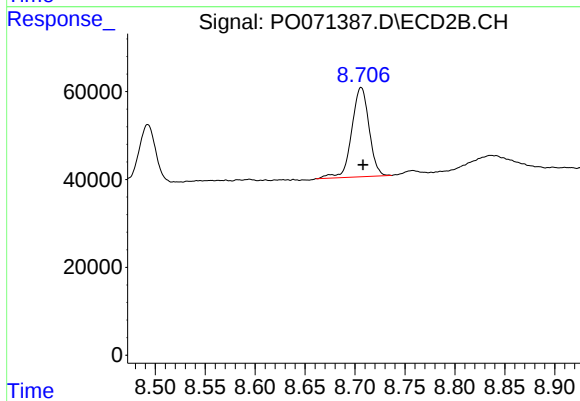

#2 Decachlorobiphenyl

R.T.: 8.706 min
Delta R.T.: -0.002 min
Response: 245136
Conc: 4.45 ng/ml

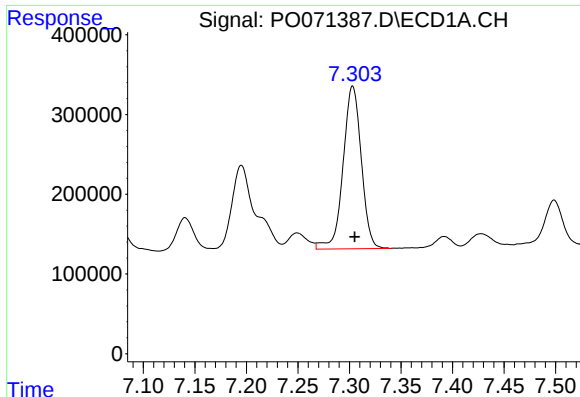


#31 AR-1260-1

R.T.: 7.303 min
Delta R.T.: -0.002 min
Response: 2512503
Conc: 554.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
REACTOR-6E-(A-D-0-4)DL


Manual Integrations
APPROVED

Ankita
9/17/2020 1:52:07 PM

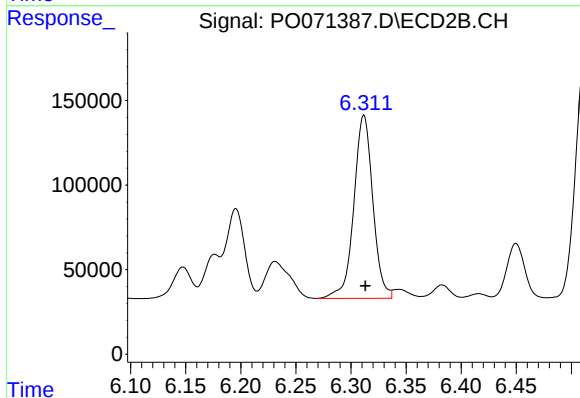


#31 AR-1260-1

R.T.: 6.312 min
Delta R.T.: -0.001 min
Response: 1300005
Conc: 466.61 ng/ml

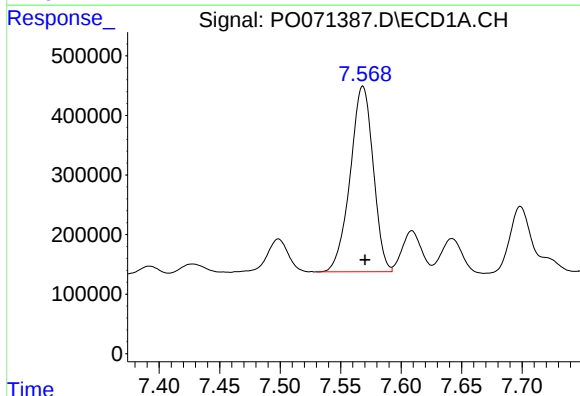


#32 AR-1260-2

R.T.: 7.568 min
Delta R.T.: -0.002 min
Response: 4131134
Conc: 592.59 ng/ml m

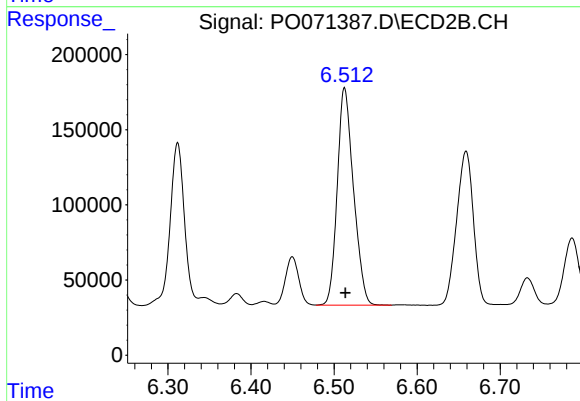

#32 AR-1260-2

R.T.: 6.513 min
Delta R.T.: 0.000 min
Response: 1963091
Conc: 543.08 ng/ml

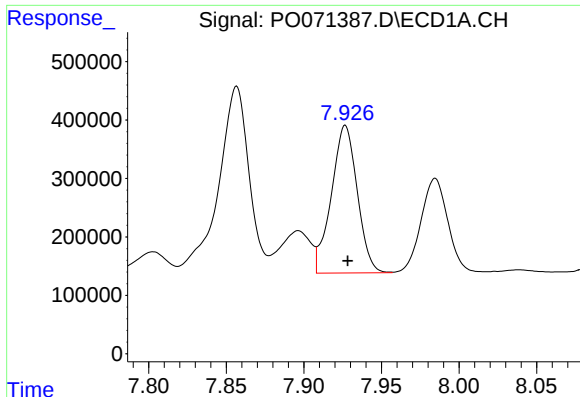


#33 AR-1260-3

R.T.: 7.927 min
Delta R.T.: -0.002 min
Response: 2936665
Conc: 484.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
REACTOR-6E-(A-D-0-4)DL


Manual Integrations
APPROVED

Ankita
9/17/2020 1:52:07 PM

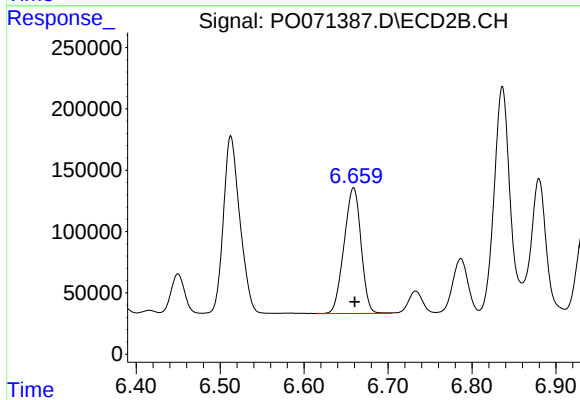


#33 AR-1260-3

R.T.: 6.659 min
Delta R.T.: -0.001 min
Response: 1441234
Conc: 446.62 ng/ml

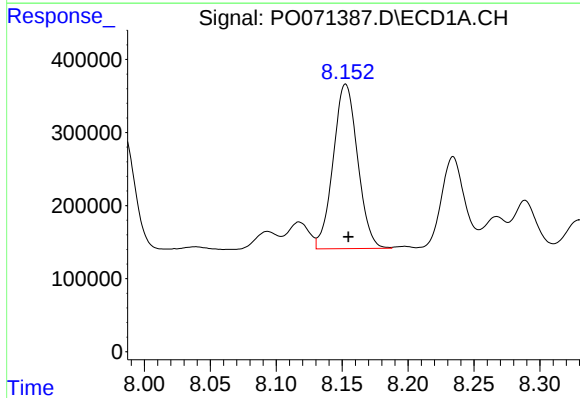


#34 AR-1260-4

R.T.: 8.153 min
Delta R.T.: -0.002 min
Response: 2905146
Conc: 507.51 ng/ml

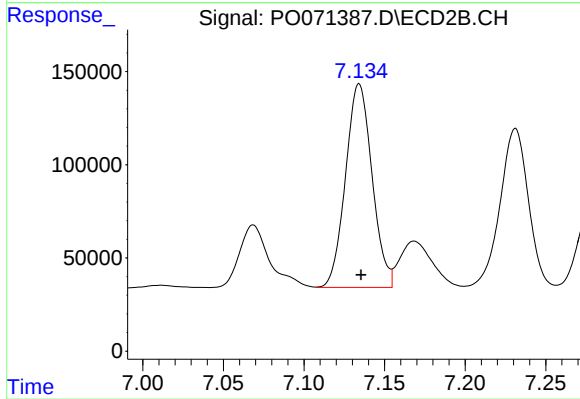

#34 AR-1260-4

R.T.: 7.134 min
Delta R.T.: -0.001 min
Response: 1251148
Conc: 431.90 ng/ml

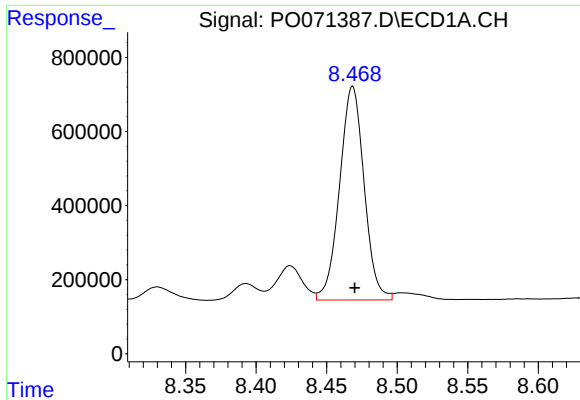


#35 AR-1260-5

R.T.: 8.468 min
Delta R.T.: -0.002 min
Response: 6989790
Conc: 551.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
REACTOR-6E-(A-D-0-4)DL

Manual Integrations
APPROVED

Ankita
9/17/2020 1:52:07 PM

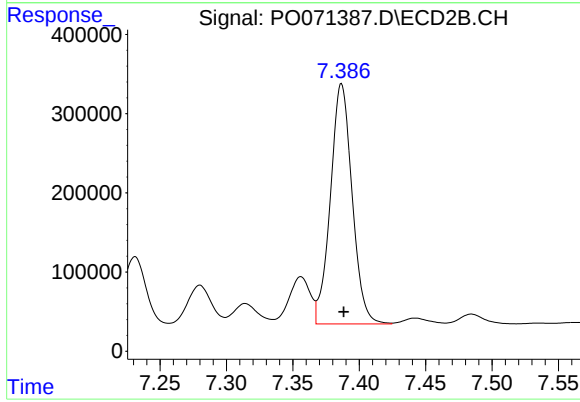

#35 AR-1260-5

R.T.: 7.387 min
Delta R.T.: -0.002 min
Response: 3459292
Conc: 456.21 ng/ml