

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091621\
 Data File : P0081314.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Sep 2021 18:35
 Operator : AJ\MA
 Sample : M3765-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:36:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.926	4.051	1381364	439873	17.498	17.800
2)	SA Decachlor...	10.985	9.410	1073837	436950	18.085	18.718
Target Compounds							
6)	L1 AR-1016-4	0.000	5.617f	0	4111	N.D.	6.838 #
14)	L3 AR-1232-4	0.000	5.617f	0	4111	N.D.	13.630 #
19)	L4 AR-1242-4	0.000	5.617f	0	4111	N.D.	7.266 #
22)	L5 AR-1248-2	0.000	5.617f	0	4111	N.D.	4.949 #
23)	L5 AR-1248-3	0.000	5.617f	0	4111	N.D.	4.843 #
32)	L7 AR-1260-2	8.196f	0.000	97833	0	21.952	N.D. #
33)	L7 AR-1260-3	0.000	7.291	0	30831	N.D.	16.841 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091621\
Data File : PO081314.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2021 18:35
Operator : AJ\MA
Sample : M3765-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:36:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

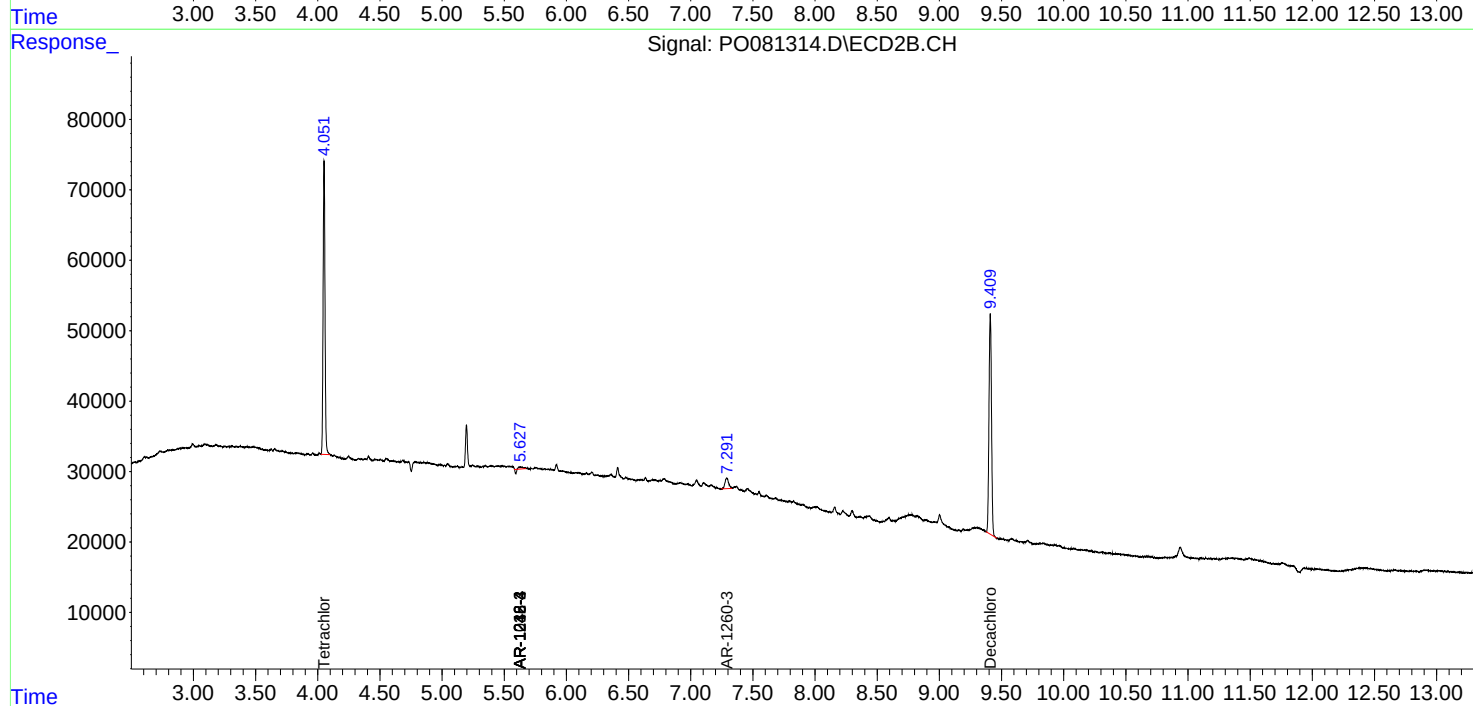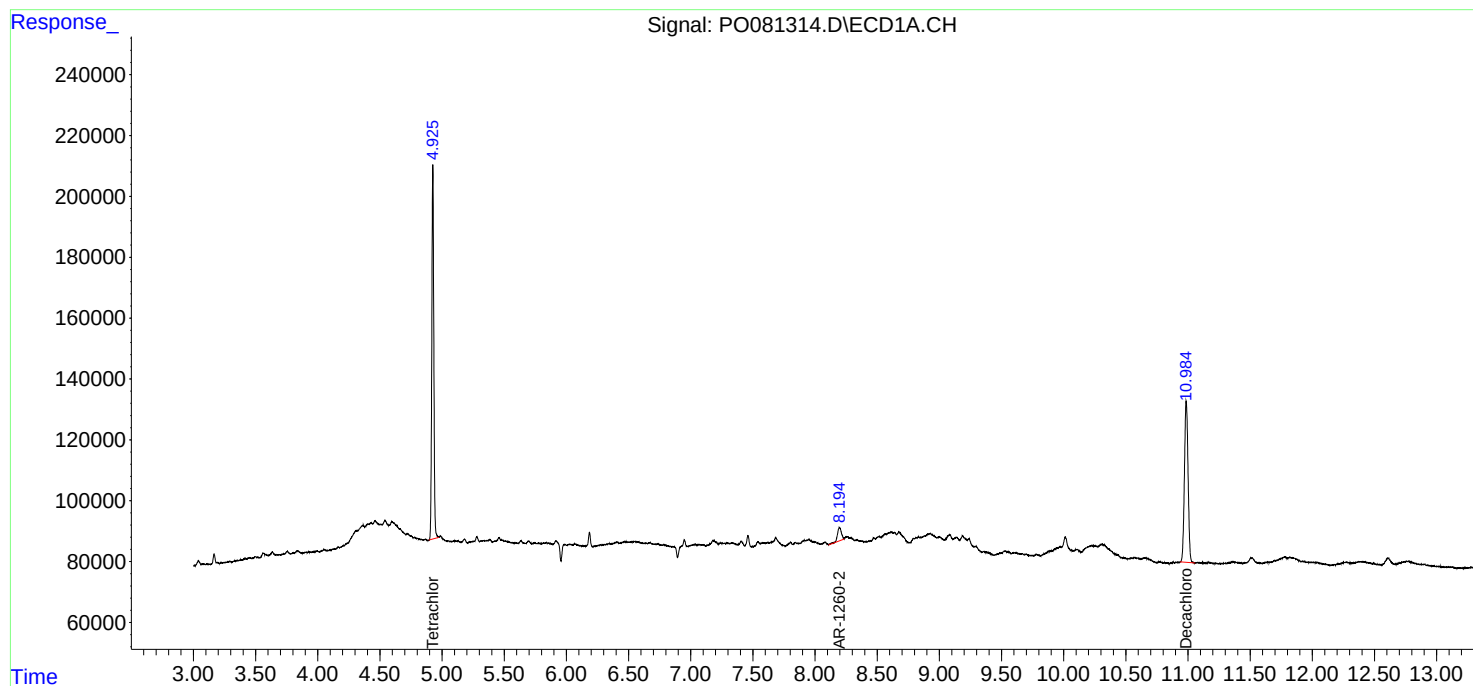


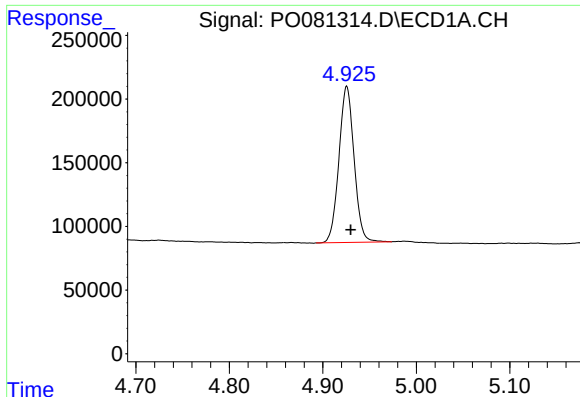

#1 Tetrachloro-m-xylene


R.T.: 4.926 min
Delta R.T.: -0.004 min
Response: 1381364
Conc: 17.50 ng/ml

Instrument :
ECD_O
ClientSampleId :

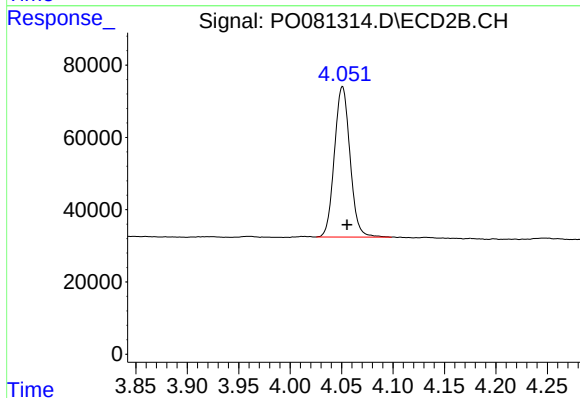


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: -0.004 min
Response: 439873
Conc: 17.80 ng/ml

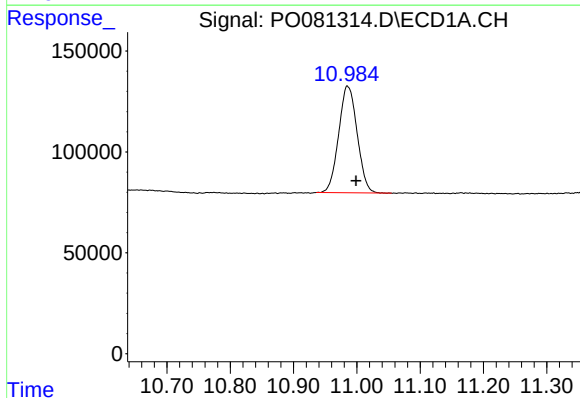


#2 Decachlorobiphenyl

R.T.: 10.985 min
Delta R.T.: -0.014 min
Response: 1073837
Conc: 18.09 ng/ml

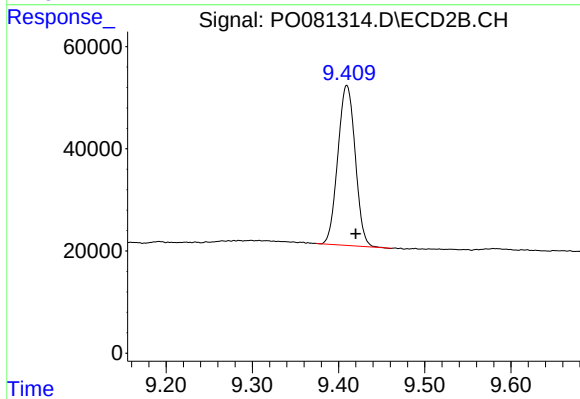

#2 Decachlorobiphenyl


R.T.: 9.410 min
Delta R.T.: -0.010 min
Response: 436950
Conc: 18.72 ng/ml

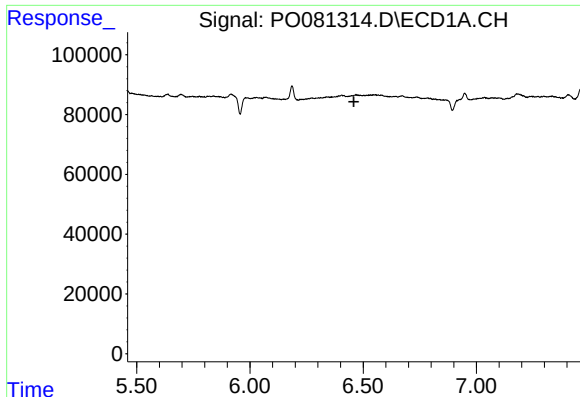

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T.: 6.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

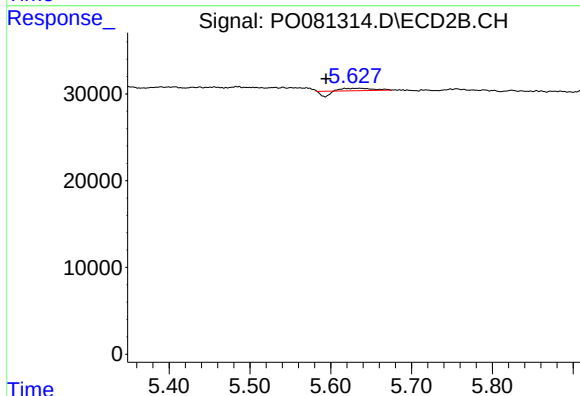


#6 AR-1016-4

R.T.: 5.617 min
Delta R.T.: 0.023 min
Response: 4111
Conc: 6.84 ng/ml

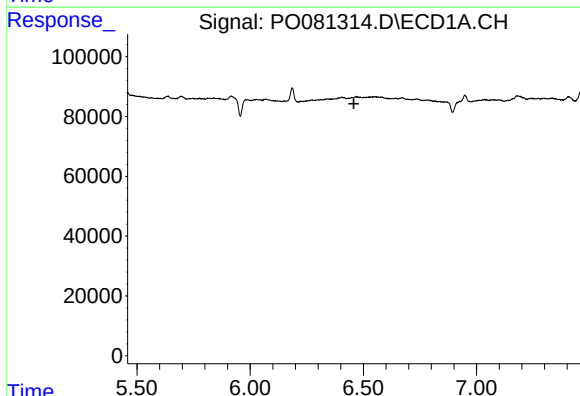


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

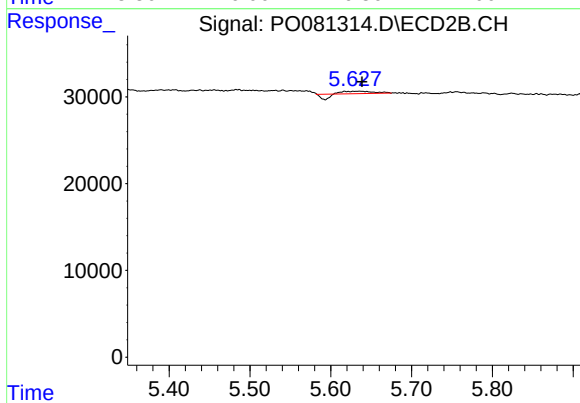

#14 AR-1232-4


R.T.: 5.617 min
Delta R.T.: -0.021 min
Response: 4111
Conc: 13.63 ng/ml

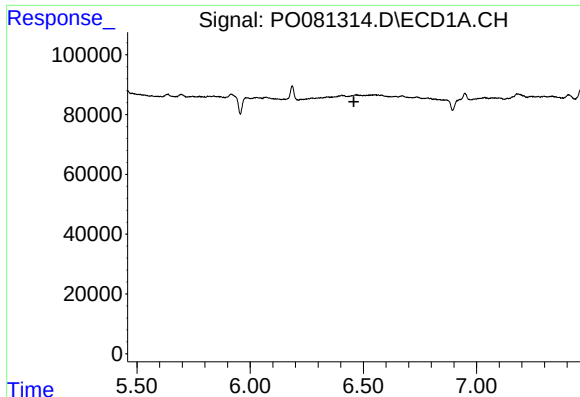

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

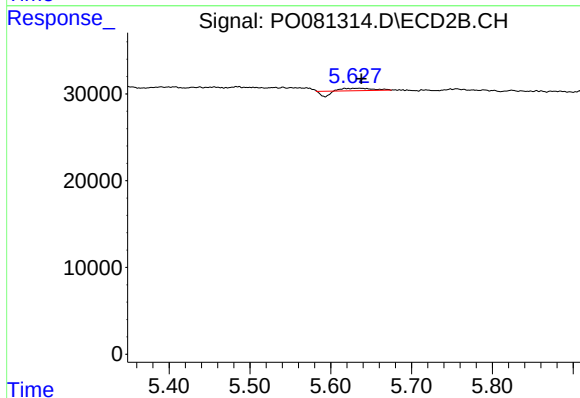


#19 AR-1242-4

R.T.: 5.617 min
Delta R.T.: -0.021 min
Response: 4111
Conc: 7.27 ng/ml

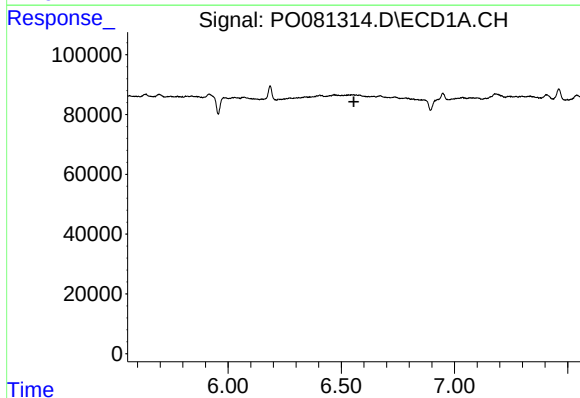


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 6.556 min
Response: 0
Conc: N.D.

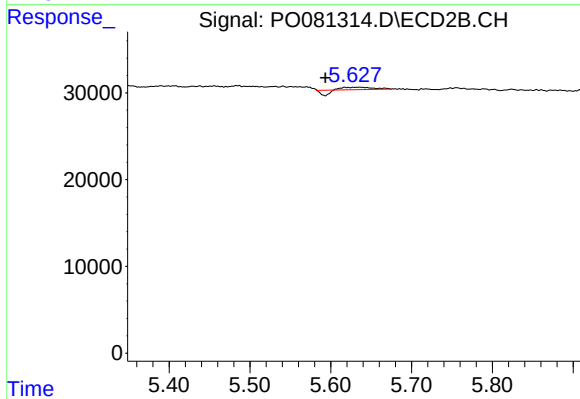

#22 AR-1248-2


R.T.: 5.617 min
Delta R.T.: 0.024 min
Response: 4111
Conc: 4.95 ng/ml

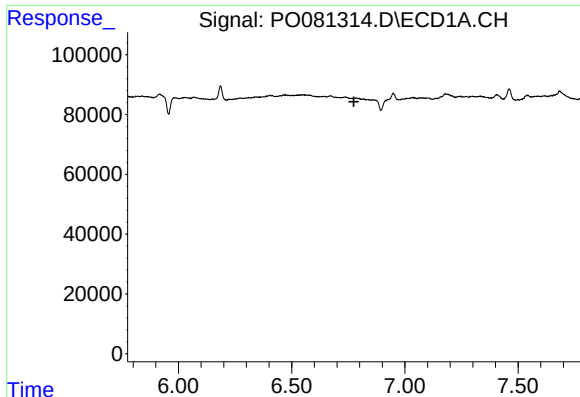

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.775 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

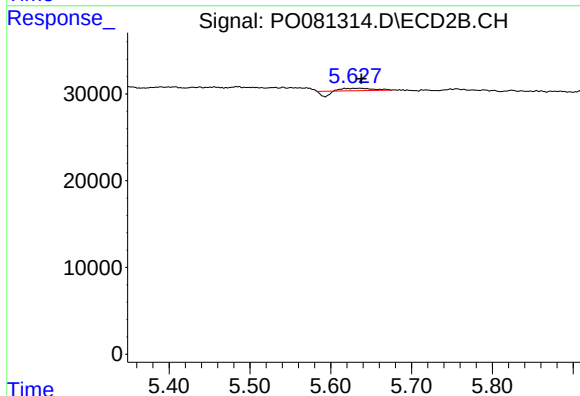


#23 AR-1248-3

R.T.: 5.617 min
Delta R.T.: -0.021 min
Response: 4111
Conc: 4.84 ng/ml

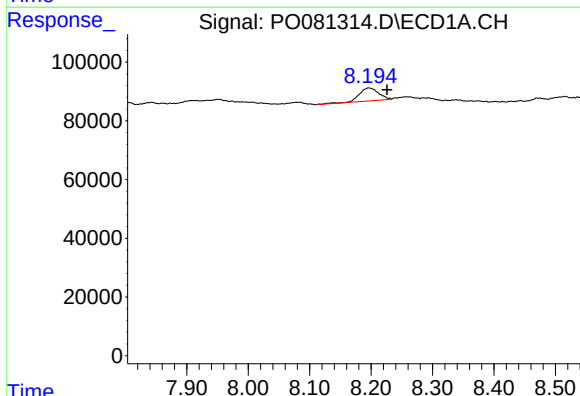


#32 AR-1260-2

R.T.: 8.196 min
Delta R.T.: -0.030 min
Response: 97833
Conc: 21.95 ng/ml

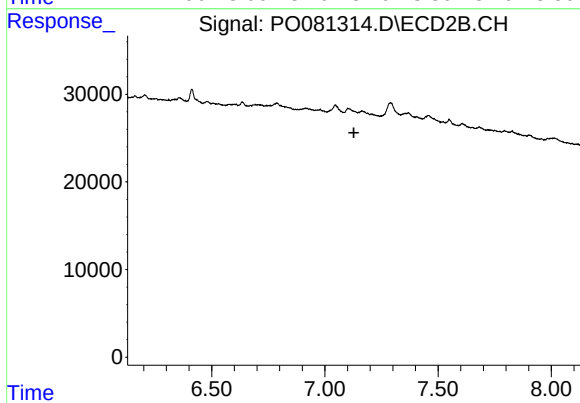

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.128 min
Response: 0
Conc: N.D.

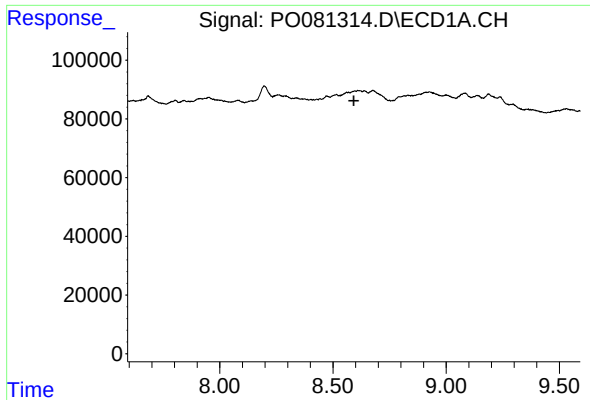

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

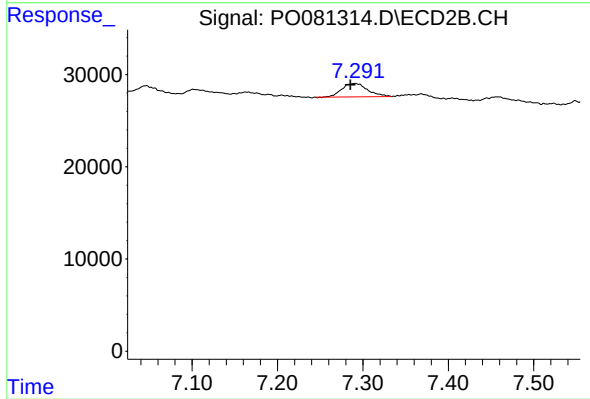

#33 AR-1260-3

R.T.: 7.291 min
Delta R.T.: 0.005 min
Response: 30831
Conc: 16.84 ng/ml