

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091621\
 Data File : P0081311.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Sep 2021 17:43
 Operator : AJ\MA
 Sample : M3759-15 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 41264

Manual Integrations
 APPROVED

mohammad
 9/17/2021 2:54:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:35:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	4.048	149921	117045	1.899m	4.736 #
2) SA Decachlor...	11.024f	9.412	429753	90691	7.238m	3.885 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091621\
Data File : P0081311.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2021 17:43
Operator : AJ\MA
Sample : M3759-15 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
41264


Manual Integrations
APPROVED

mohammad
9/17/2021 2:54:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:35:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

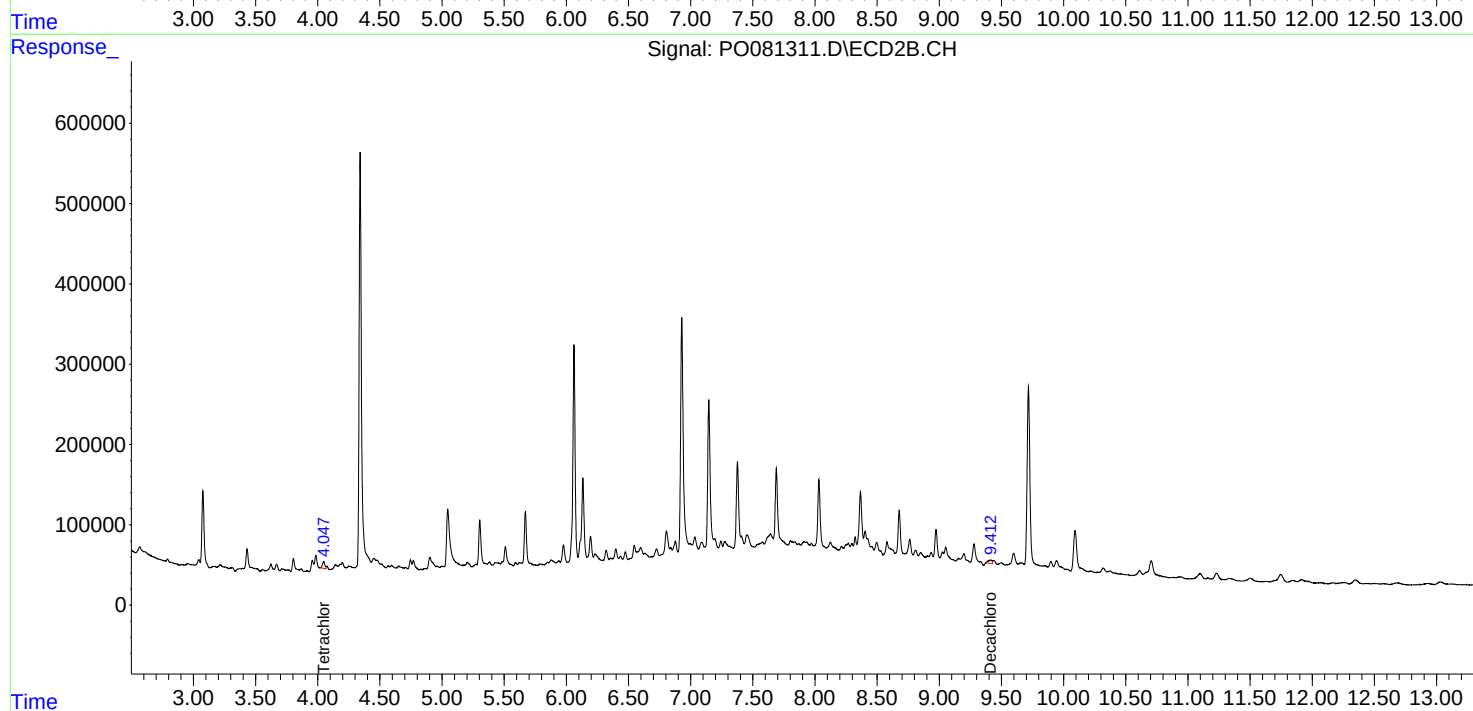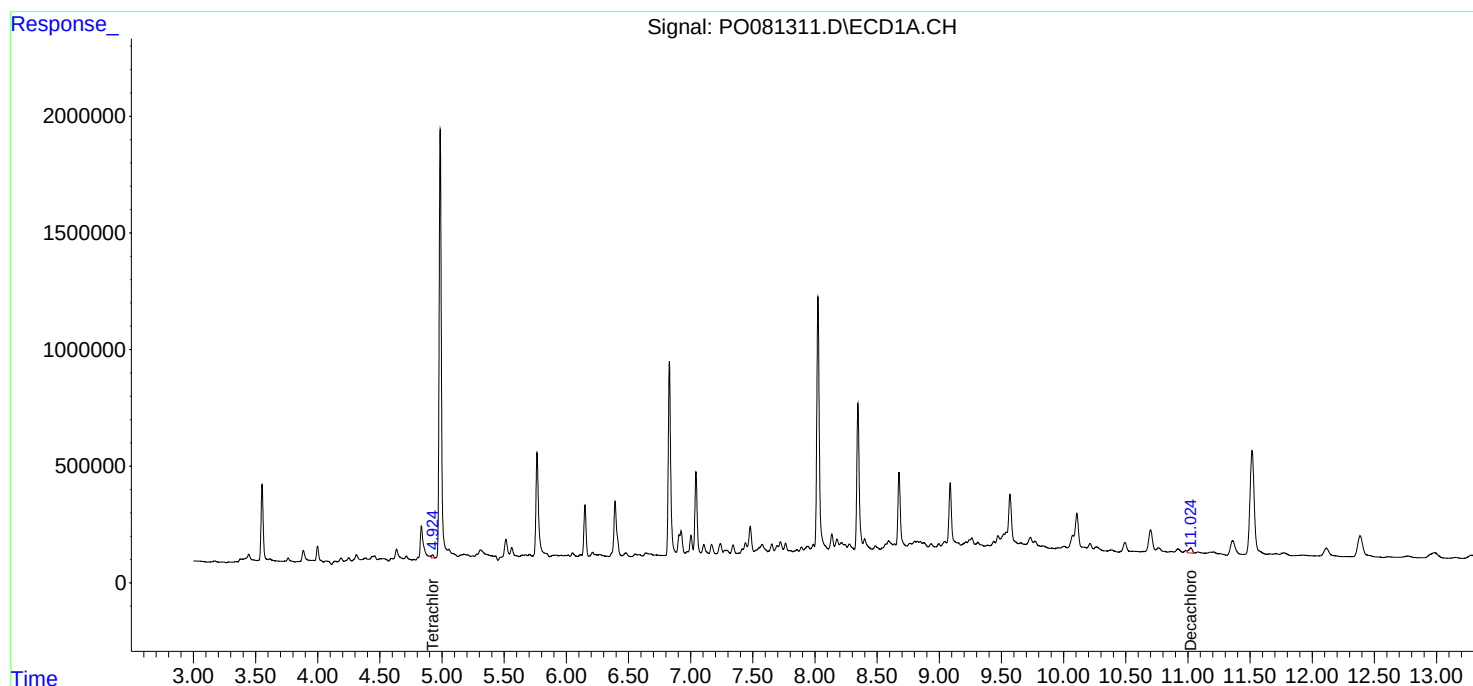

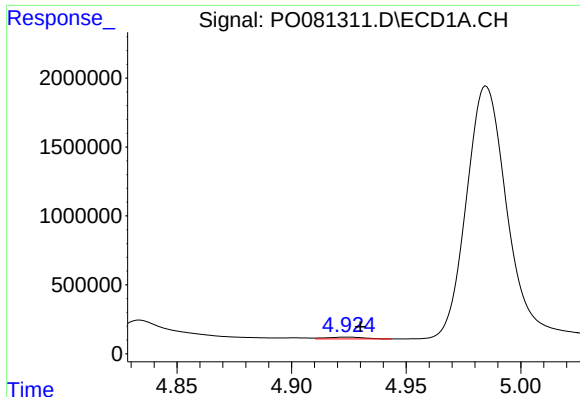


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: -0.006 min
Response: 149921
Conc: 1.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
41264


Manual Integrations
APPROVED

mohammad
9/17/2021 2:54:46 PM

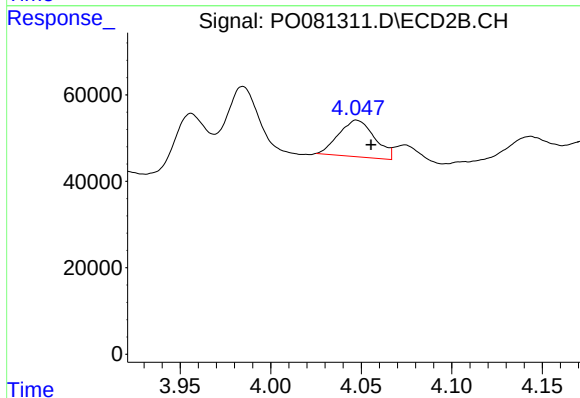


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: -0.008 min
Response: 117045
Conc: 4.74 ng/ml

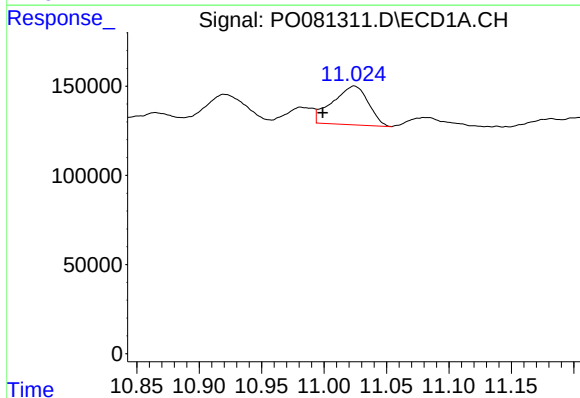

#2 Decachlorobiphenyl

R.T.: 11.024 min
Delta R.T.: 0.025 min
Response: 429753
Conc: 7.24 ng/ml m

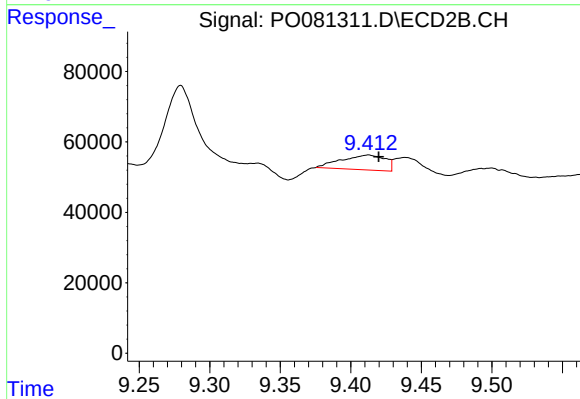

#2 Decachlorobiphenyl

R.T.: 9.412 min
Delta R.T.: -0.007 min
Response: 90691
Conc: 3.88 ng/ml