

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091621\
 Data File : P0081327.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Sep 2021 22:55
 Operator : AJ\MA
 Sample : M3761-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-20-20210915-1-2-WC

Manual Integrations
 APPROVED

mohammad
 9/17/2021 2:55:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:45:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	4.050	1694223	526221	21.462	21.294
2) SA Decachlor...	10.985	9.408	1201852	467221	20.241	20.014
Target Compounds						
31) L7 AR-1260-1	7.952	6.922	344244	125805	99.033m	85.722
32) L7 AR-1260-2	8.215	7.121	547370	79228	122.820	45.136 #
33) L7 AR-1260-3	8.586	7.276	191272	163388	72.888	89.250m
34) L7 AR-1260-4	8.815	7.763	572992	59312	179.002	50.205 #
35) L7 AR-1260-5	9.146	8.012	448821	178421	74.970	63.029m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091621\
Data File : PO081327.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Sep 2021 22:55
Operator : AJ\MA
Sample : M3761-02
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MW-20-20210915-1-2-WC


Manual Integrations
APPROVED

mohammad
9/17/2021 2:55:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:45:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

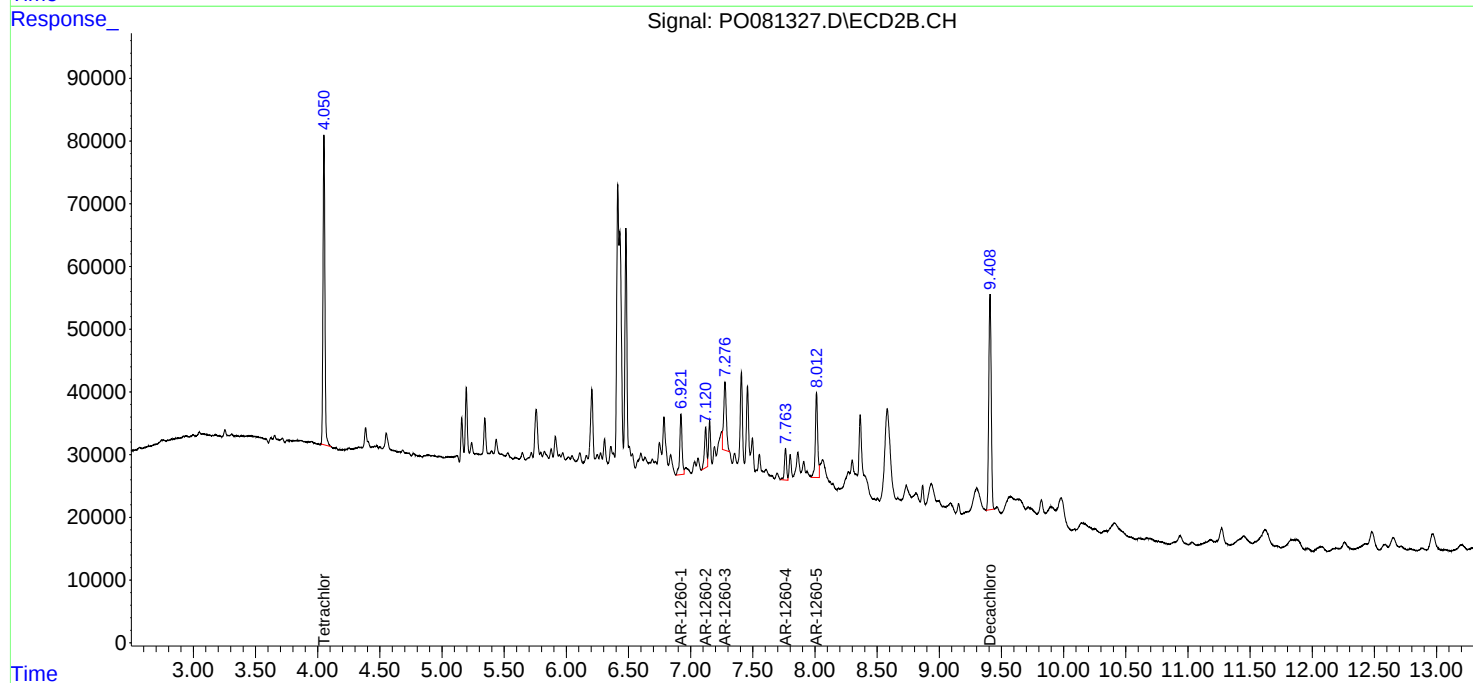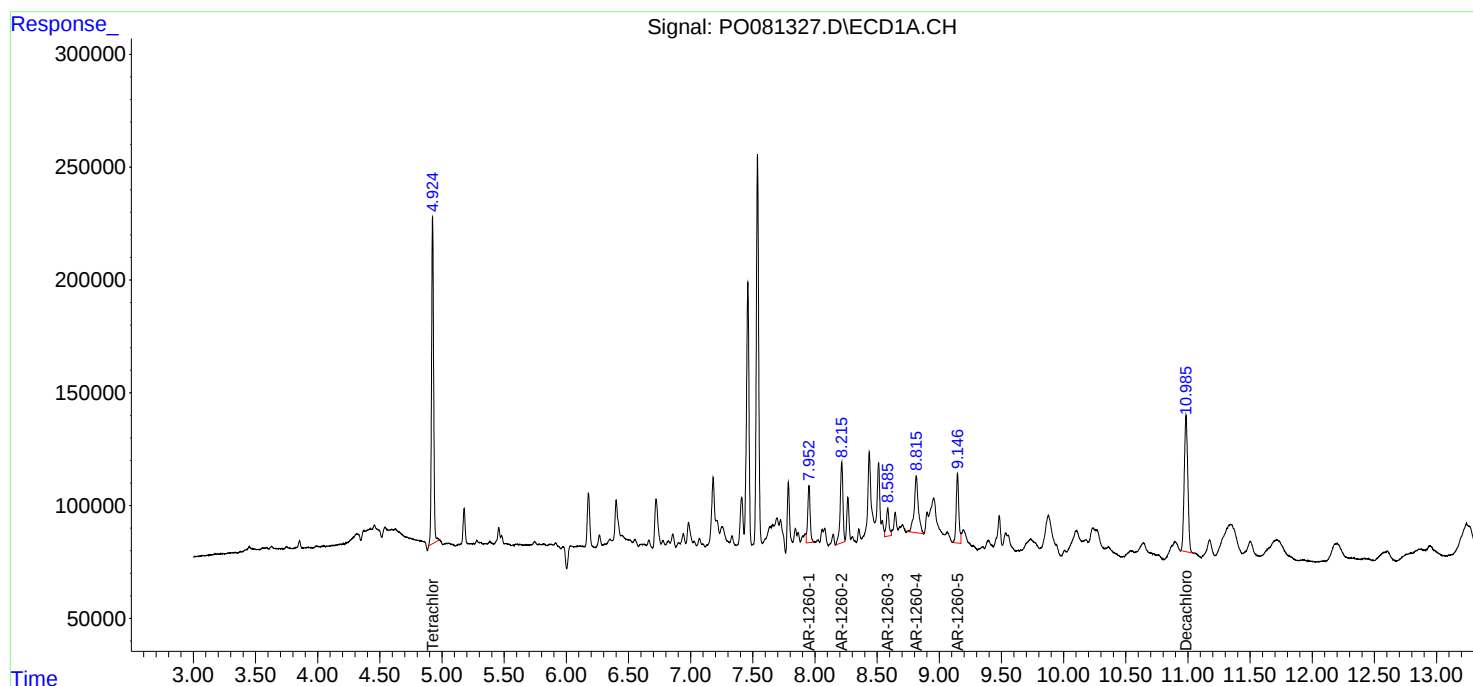

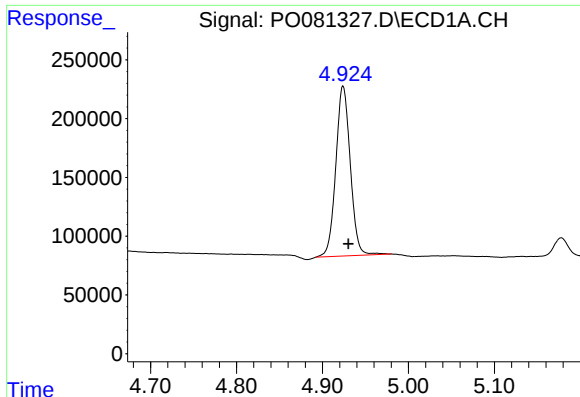


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: -0.006 min
Response: 1694223
Conc: 21.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-20-20210915-1-2-WC


Manual Integrations
APPROVED

mohammad
9/17/2021 2:55:03 PM

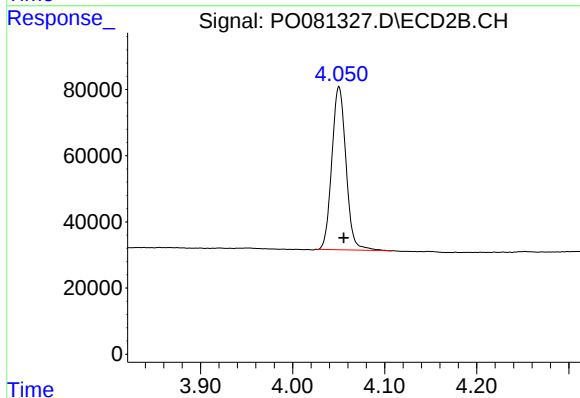


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.005 min
Response: 526221
Conc: 21.29 ng/ml

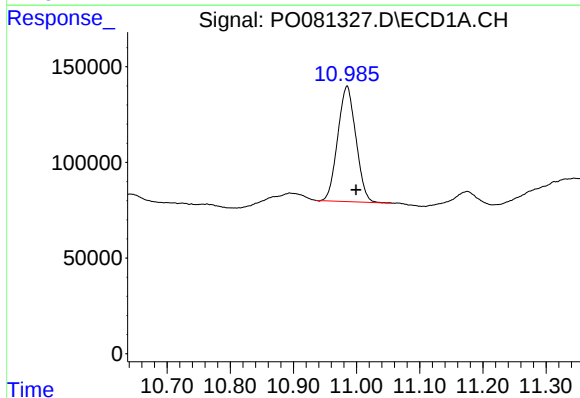


#2 Decachlorobiphenyl

R.T.: 10.985 min
Delta R.T.: -0.014 min
Response: 1201852
Conc: 20.24 ng/ml

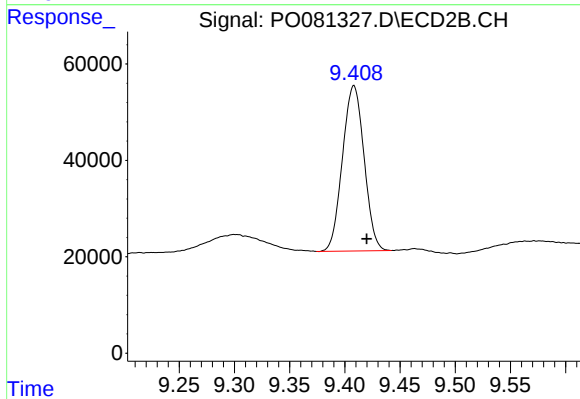

#2 Decachlorobiphenyl

R.T.: 9.408 min
Delta R.T.: -0.012 min
Response: 467221
Conc: 20.01 ng/ml

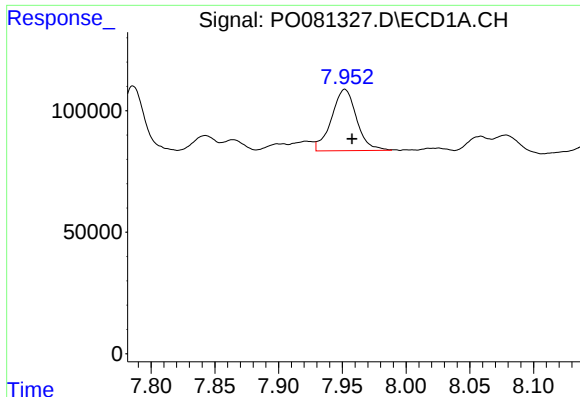


#31 AR-1260-1

R.T.: 7.952 min
Delta R.T.: -0.006 min
Response: 344244
Conc: 99.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MW-20-20210915-1-2-WC


Manual Integrations
APPROVED

mohammad
9/17/2021 2:55:03 PM

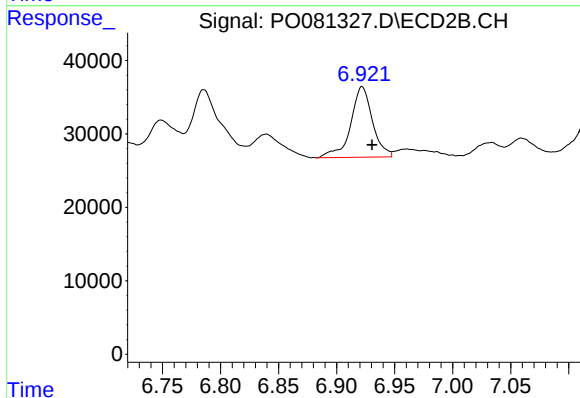


#31 AR-1260-1

R.T.: 6.922 min
Delta R.T.: -0.009 min
Response: 125805
Conc: 85.72 ng/ml

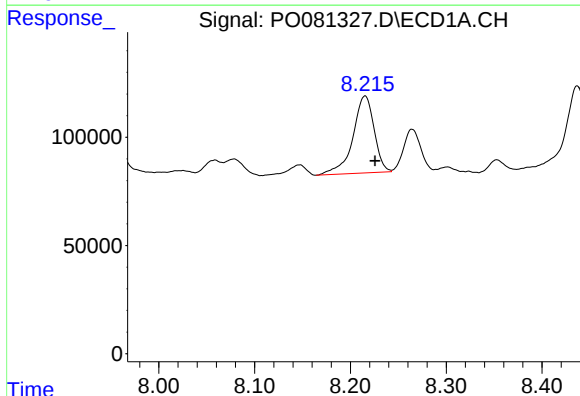


#32 AR-1260-2

R.T.: 8.215 min
Delta R.T.: -0.011 min
Response: 547370
Conc: 122.82 ng/ml

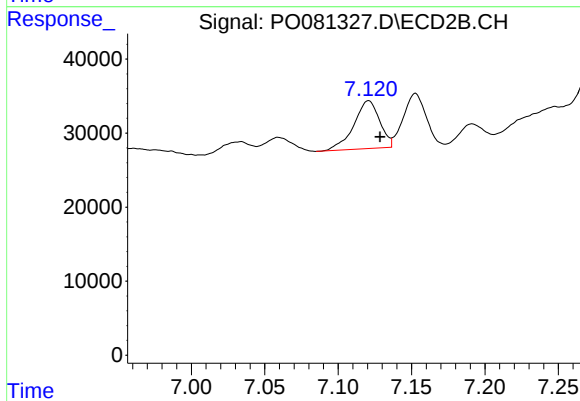

#32 AR-1260-2

R.T.: 7.121 min
Delta R.T.: -0.008 min
Response: 79228
Conc: 45.14 ng/ml

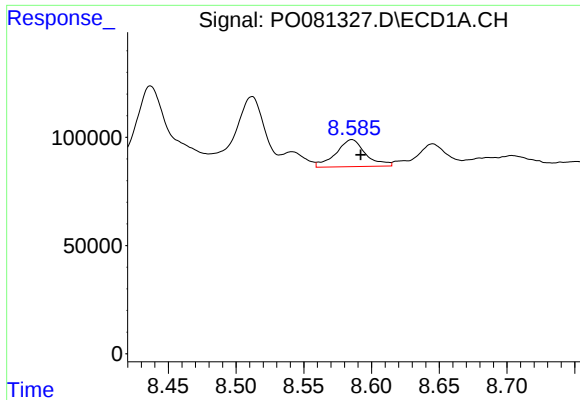


#33 AR-1260-3

R.T.: 8.586 min
Delta R.T.: -0.007 min
Response: 191272
Conc: 72.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-20-20210915-1-2-WC


Manual Integrations
APPROVED

mohammad
9/17/2021 2:55:03 PM

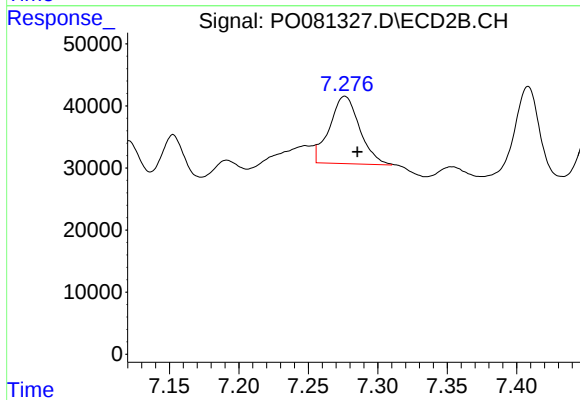


#33 AR-1260-3

R.T.: 7.276 min
Delta R.T.: -0.010 min
Response: 163388
Conc: 89.25 ng/ml m

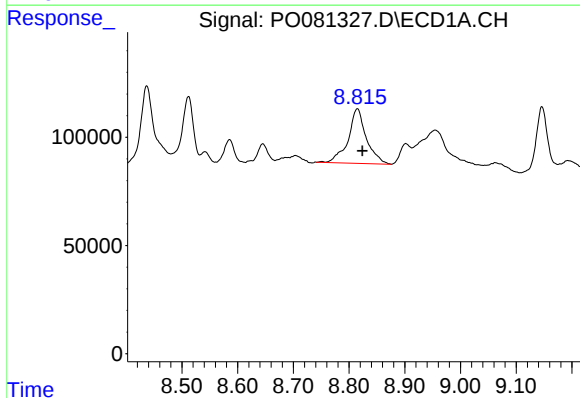


#34 AR-1260-4

R.T.: 8.815 min
Delta R.T.: -0.009 min
Response: 572992
Conc: 179.00 ng/ml

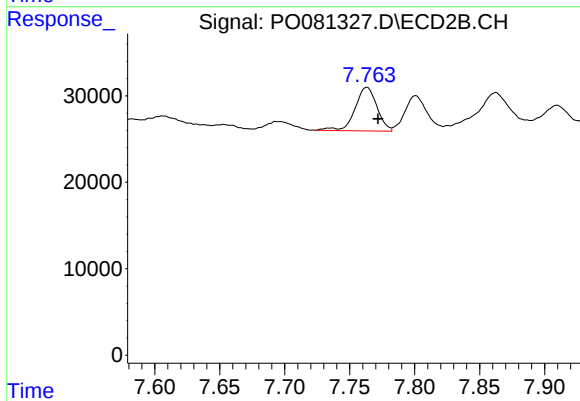

#34 AR-1260-4

R.T.: 7.763 min
Delta R.T.: -0.009 min
Response: 59312
Conc: 50.21 ng/ml

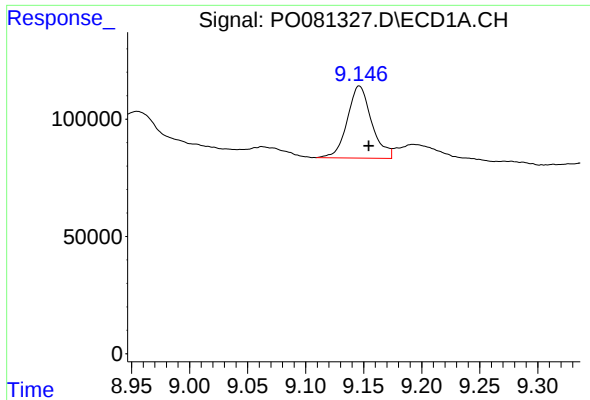


#35 AR-1260-5

R.T.: 9.146 min
Delta R.T.: -0.008 min
Response: 448821
Conc: 74.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-20-20210915-1-2-WC

Manual Integrations
APPROVED

mohammad
9/17/2021 2:55:03 PM

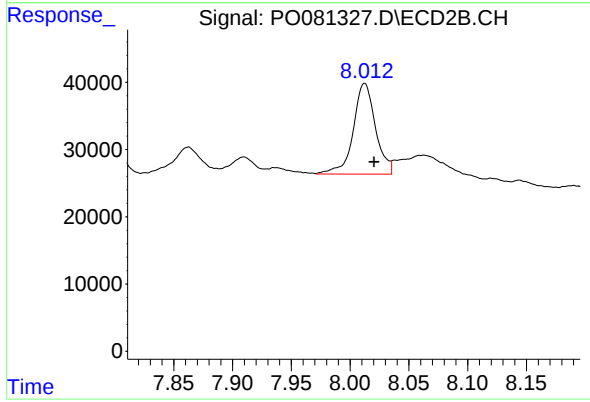

#35 AR-1260-5

R.T.: 8.012 min
Delta R.T.: -0.008 min
Response: 178421
Conc: 63.03 ng/ml m