

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091621\
 Data File : P0081334.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2021 00:55
 Operator : AJ\MA
 Sample : M3671-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FILTER-MEDIA-FILTERS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:50:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	4.050	1391428	407834	17.626	16.503
2) SA Decachlor...	10.989	9.410	3453354	647500	58.161m	27.737 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091621\
Data File : P0081334.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2021 00:55
Operator : AJ\MA
Sample : M3671-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FILTER-MEDIA-FILTERS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:50:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

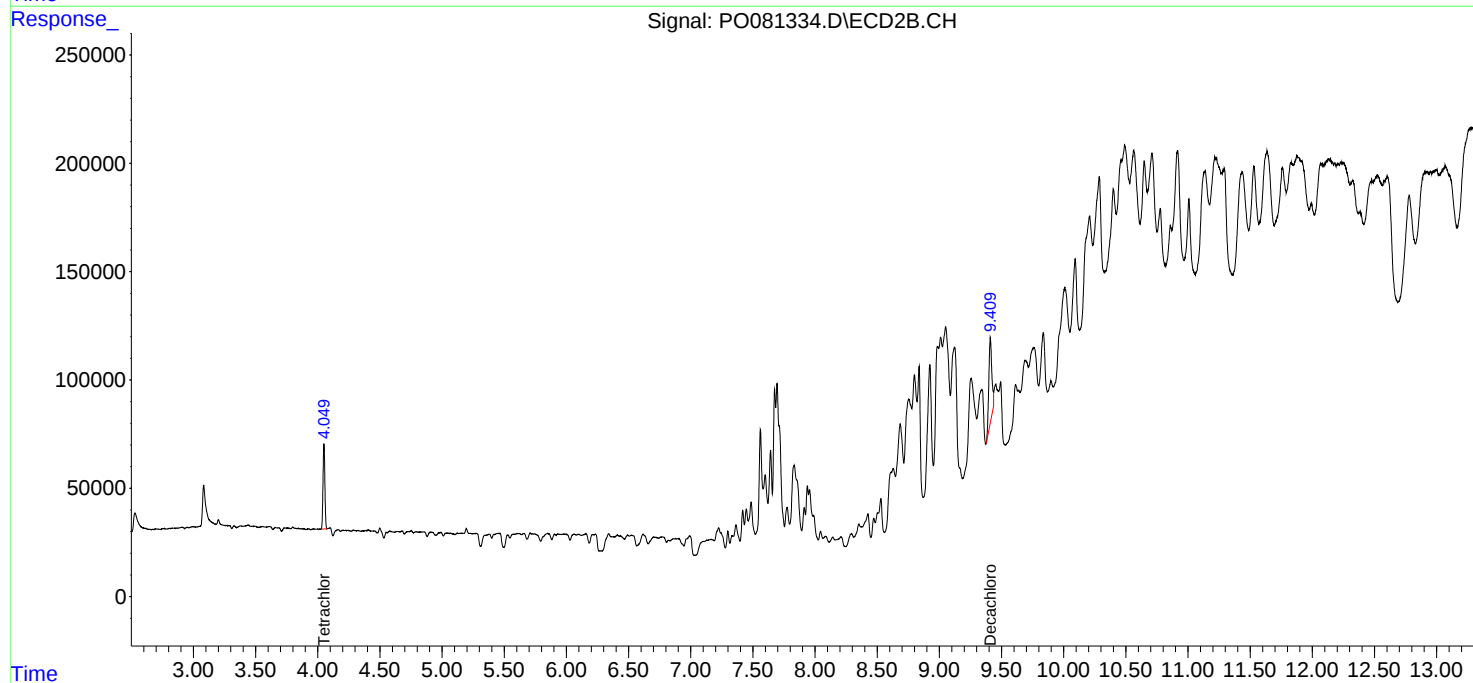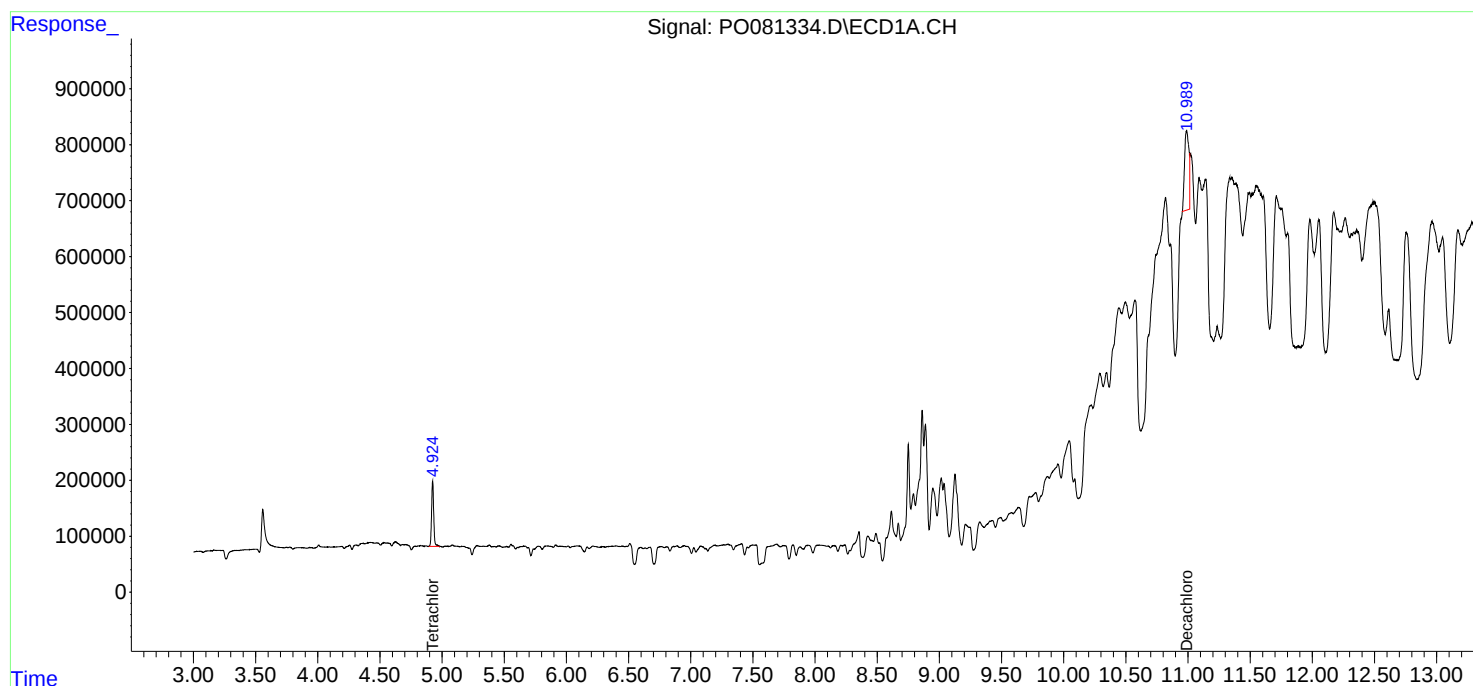


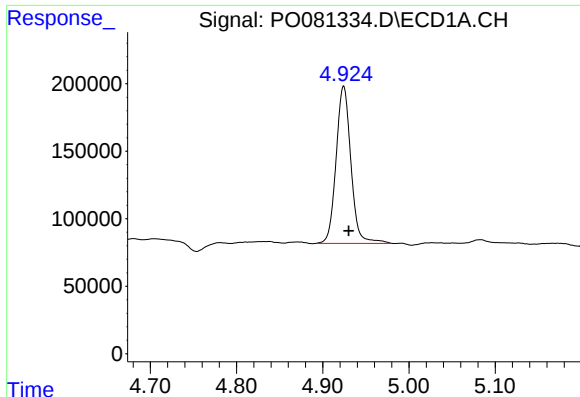

#1 Tetrachloro-m-xylene


R.T.: 4.924 min
Delta R.T.: -0.006 min
Response: 1391428
Conc: 17.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
FILTER-MEDIA-FILTERS

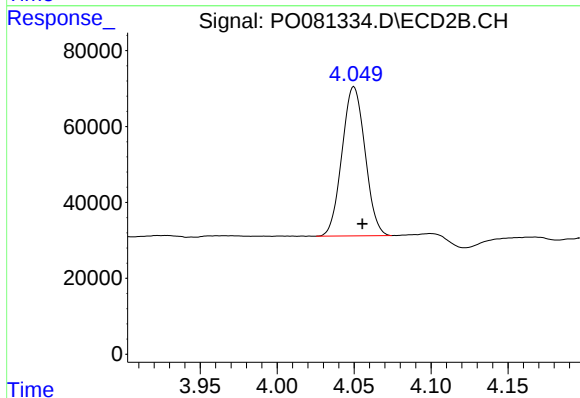


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.006 min
Response: 407834
Conc: 16.50 ng/ml

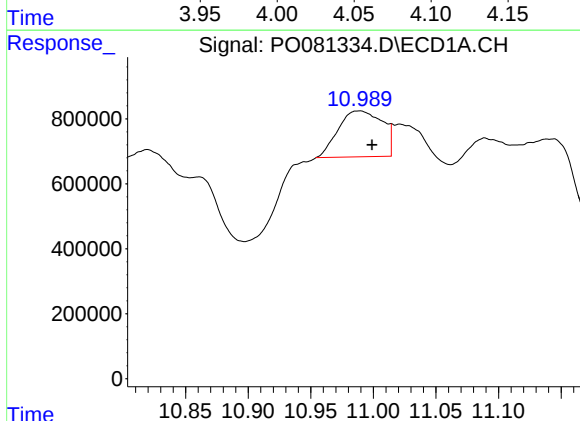

#2 Decachlorobiphenyl

R.T.: 10.989 min
Delta R.T.: -0.010 min
Response: 3453354
Conc: 58.16 ng/ml m

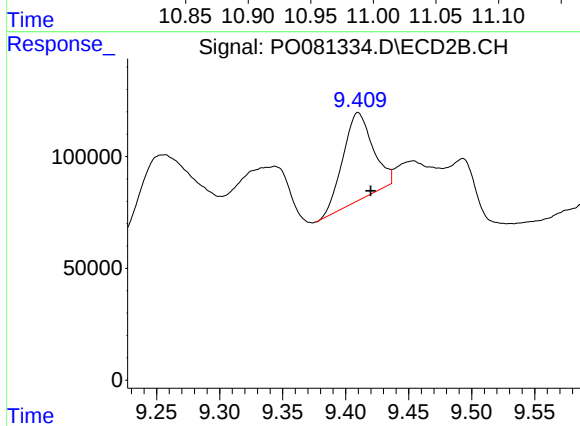

#2 Decachlorobiphenyl

R.T.: 9.410 min
Delta R.T.: -0.010 min
Response: 647500
Conc: 27.74 ng/ml