

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091621\
 Data File : P0081342.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2021 3:13
 Operator : AJ\MA
 Sample : M3761-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-20-20210915-5-5.5-WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 03:49:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.926	4.052	1778725	562510	22.532	22.763
2) SA Decachlor...	10.987	9.409	1148576	465131	19.344	19.925

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091621\
Data File : P0081342.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2021 3:13
Operator : AJ\MA
Sample : M3761-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MW-20-20210915-5-5.5-WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 03:49:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

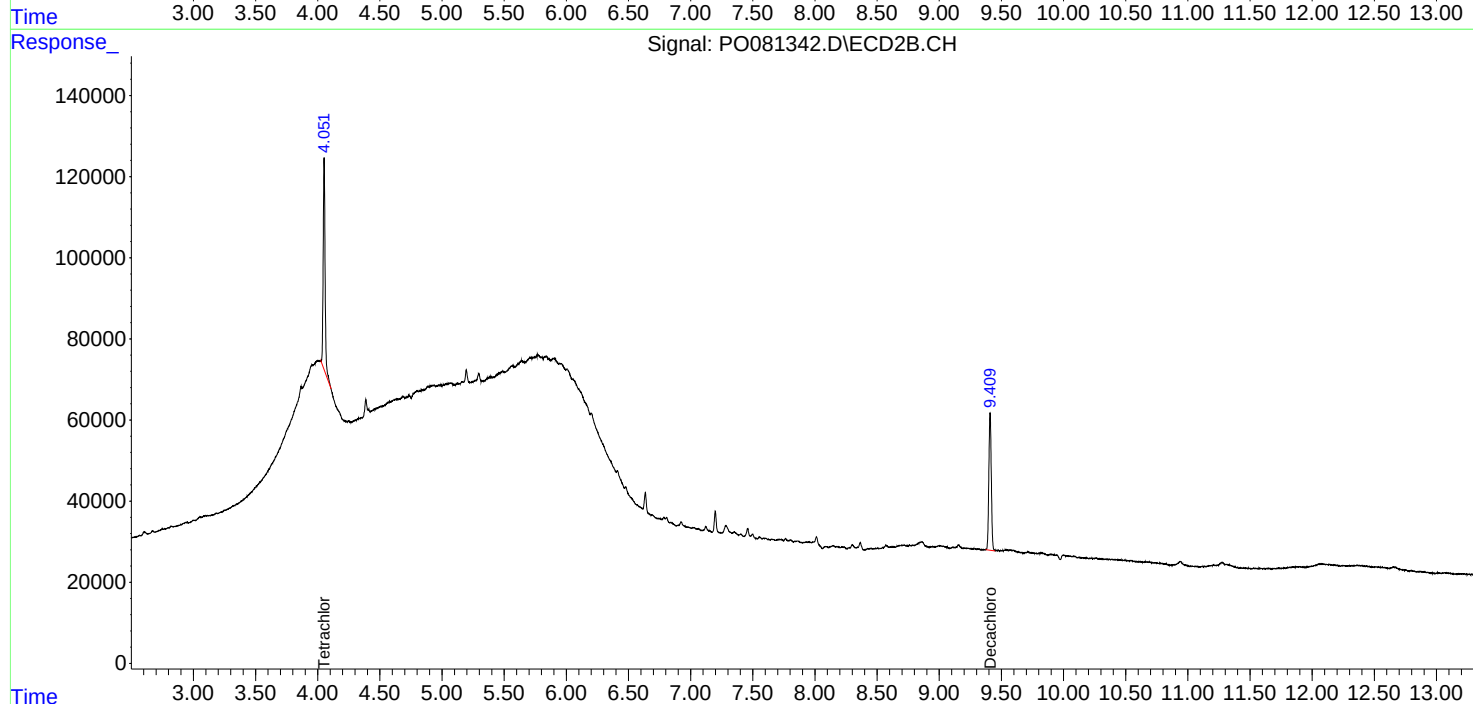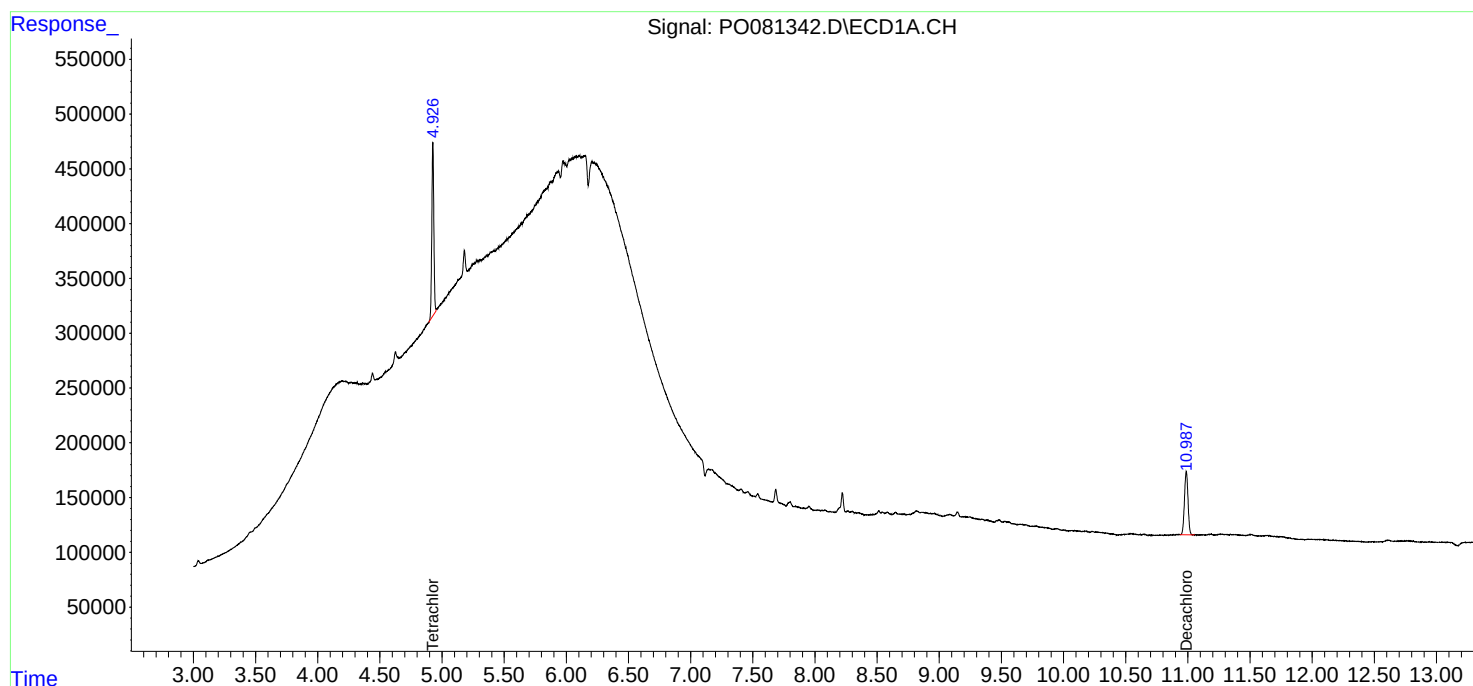


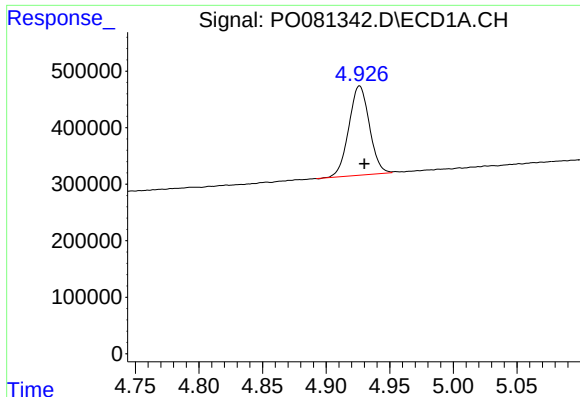

#1 Tetrachloro-m-xylene


R.T.: 4.926 min
Delta R.T.: -0.004 min
Response: 1778725
Conc: 22.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-20-20210915-5-5.5-WC

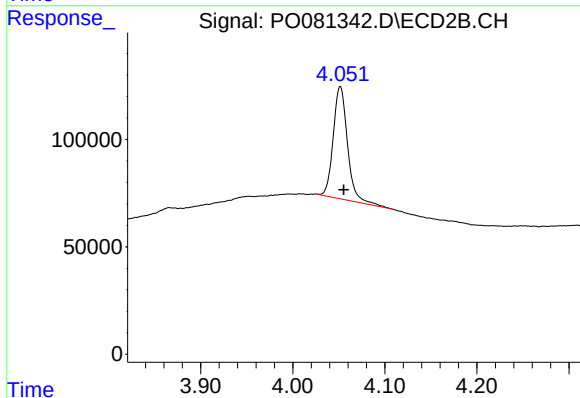


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: -0.004 min
Response: 562510
Conc: 22.76 ng/ml

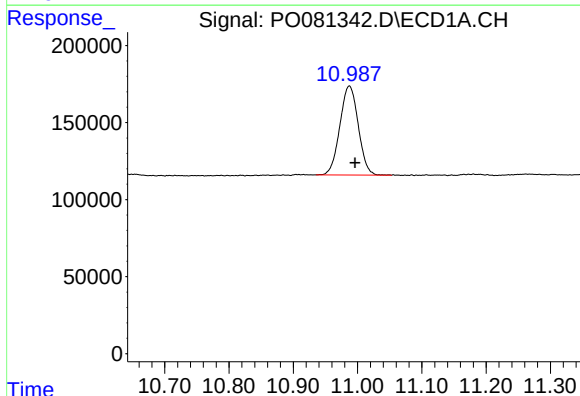

#2 Decachlorobiphenyl

R.T.: 10.987 min
Delta R.T.: -0.009 min
Response: 1148576
Conc: 19.34 ng/ml

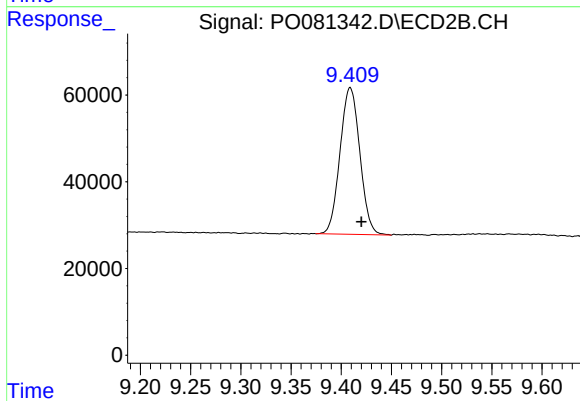

#2 Decachlorobiphenyl

R.T.: 9.409 min
Delta R.T.: -0.011 min
Response: 465131
Conc: 19.92 ng/ml