

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091622\
 Data File : P0089603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2022 21:07
 Operator : YP/AJ
 Sample : N4628-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HW-54

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/19/2022
 Supervised By :Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:02:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 16 08:48:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.475	3.662	70663655	28317048	18.258m	16.616m
2) SA Decachlor...	10.349	8.766	34765407	13527496	14.082	11.988

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091622\
Data File : PO089603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2022 21:07
Operator : YP/AJ
Sample : N4628-02
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HW-54


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2022
Supervised By :Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 04:02:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091522.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 16 08:48:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

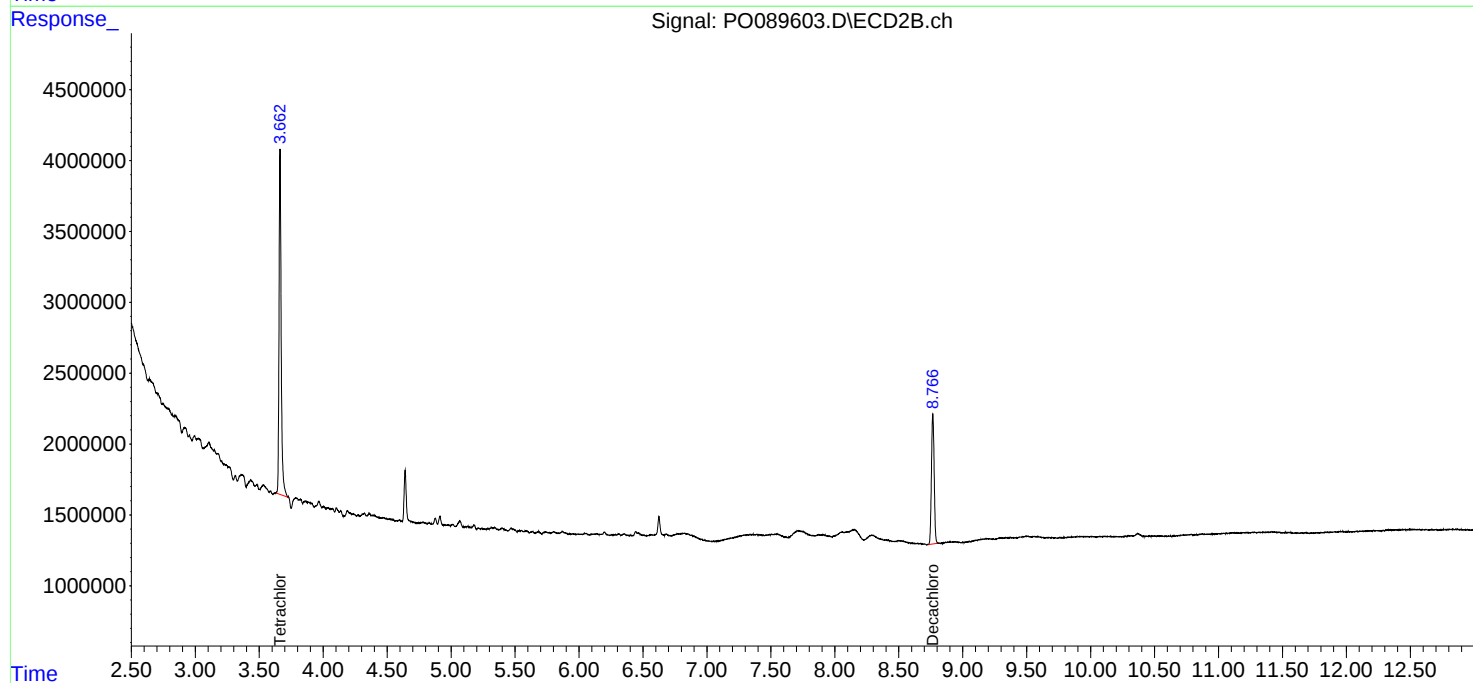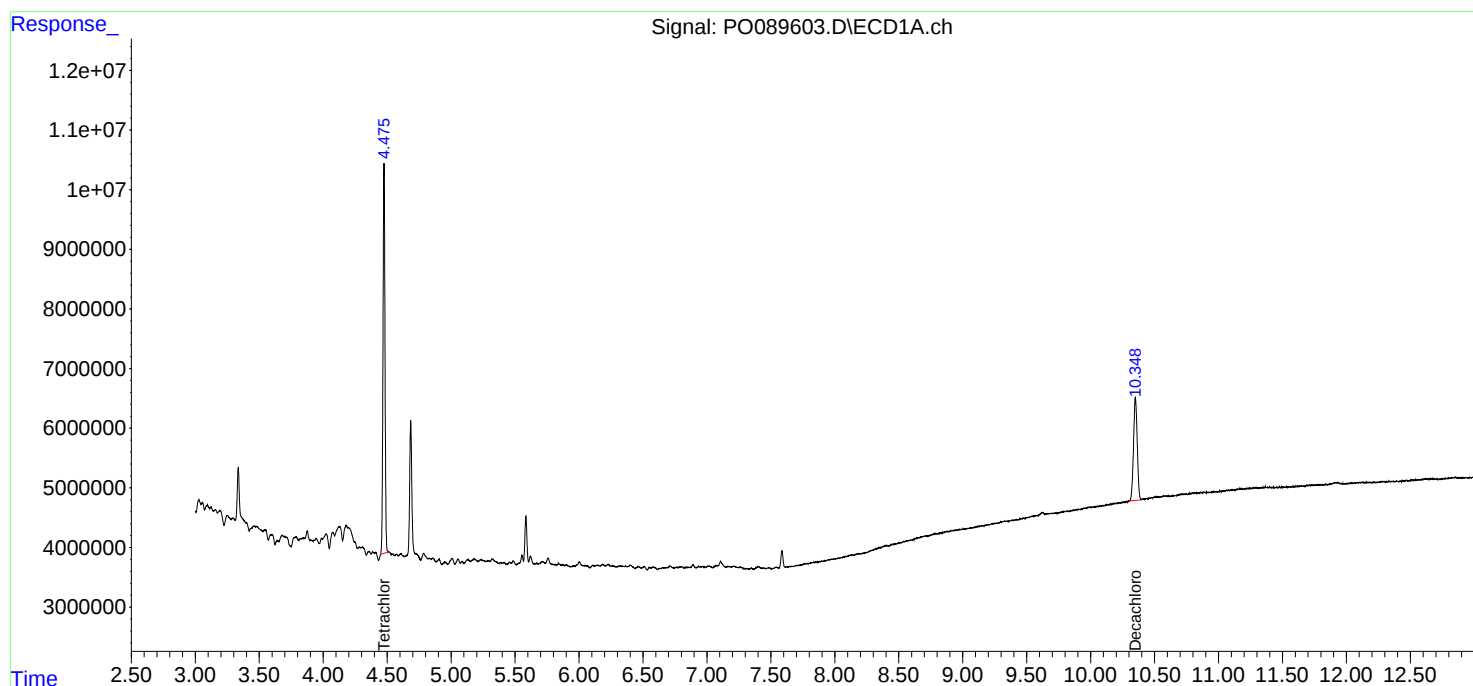

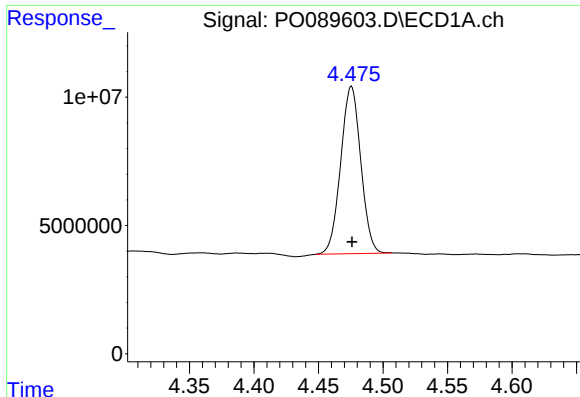


#1 Tetrachloro-m-xylene

R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 70663655
Conc: 18.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
HW-54


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2022
Supervised By :Ankita Jodhani 09/19/2022

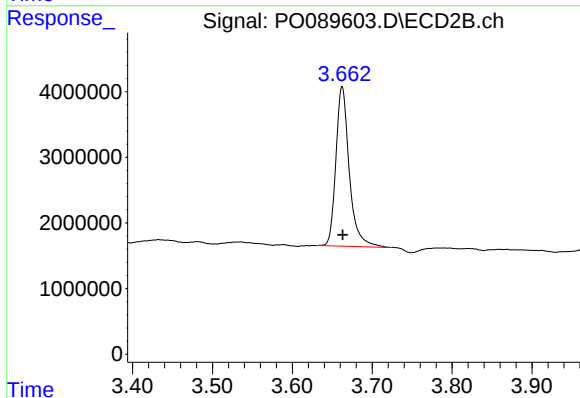


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.001 min
Response: 28317048
Conc: 16.62 ng/ml m

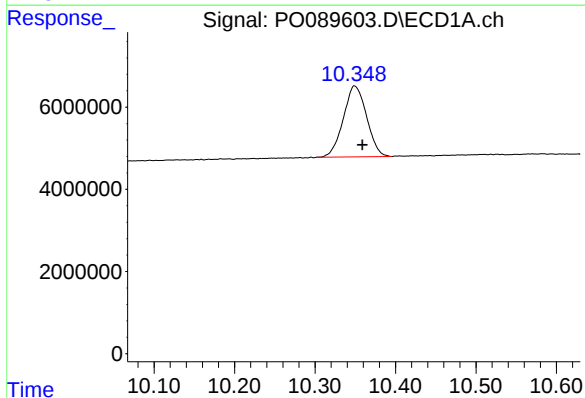

#2 Decachlorobiphenyl

R.T.: 10.349 min
Delta R.T.: -0.010 min
Response: 34765407
Conc: 14.08 ng/ml

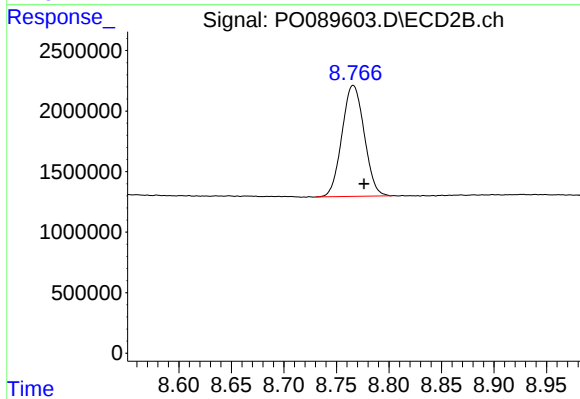

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.010 min
Response: 13527496
Conc: 11.99 ng/ml