

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091622\
 Data File : P0089606.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2022 21:58
 Operator : YP/AJ
 Sample : N4648-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 N48854-1040

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/19/2022
 Supervised By :Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:04:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 16 08:48:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.473	3.661	70084690	43763609	18.109m	25.680 #
2) SA Decachlor...	10.349	8.766	22049683	8502949	8.932	7.535

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091622\
Data File : PO089606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2022 21:58
Operator : YP/AJ
Sample : N4648-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
N48854-1040


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2022
Supervised By :Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 04:04:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091522.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 16 08:48:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

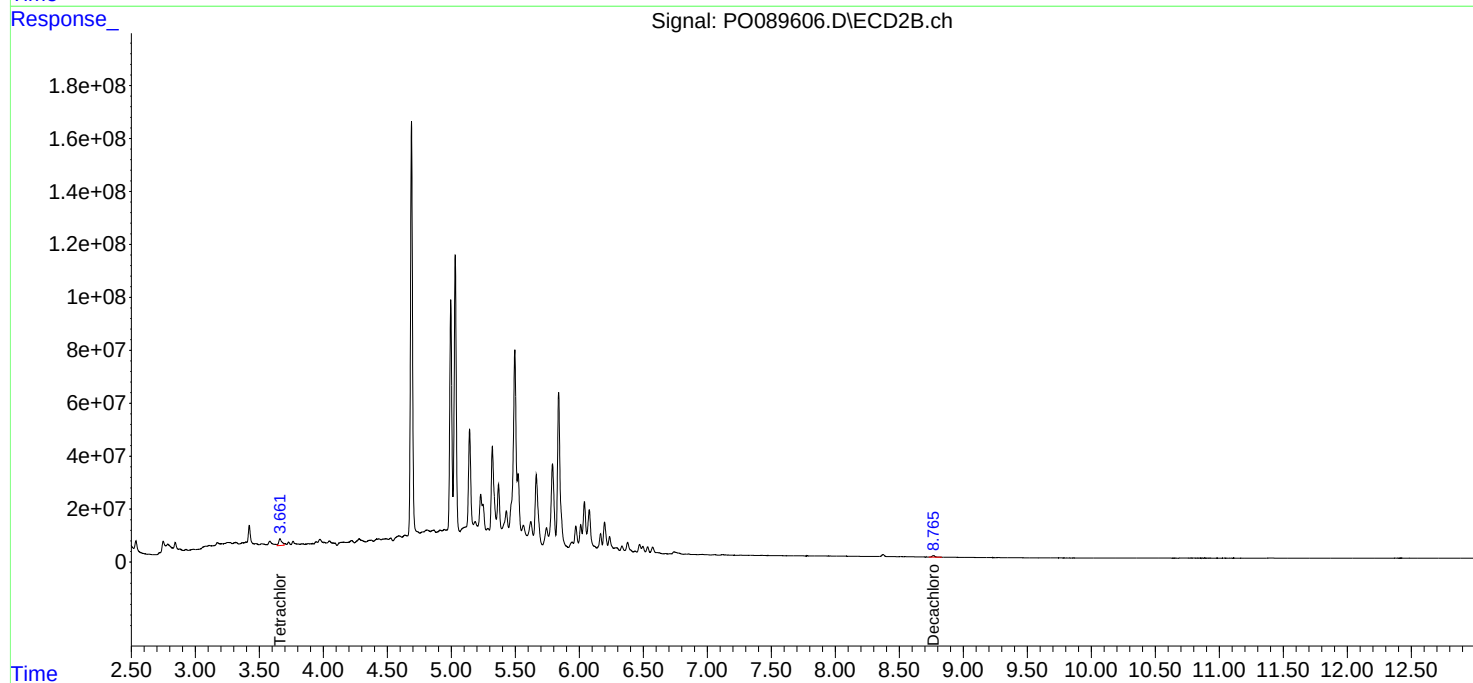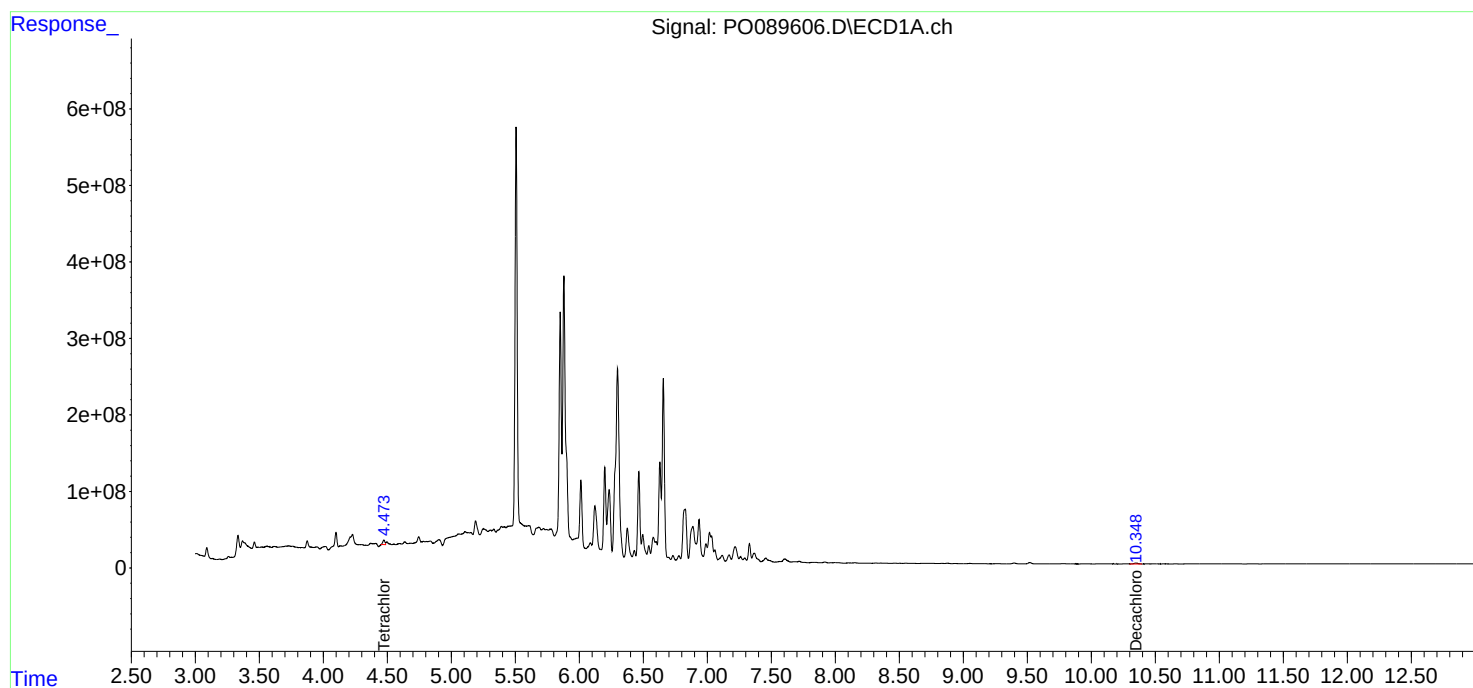

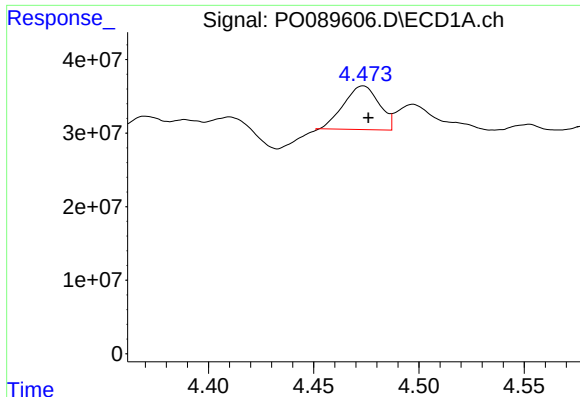


#1 Tetrachloro-m-xylene

R.T.: 4.473 min
Delta R.T.: -0.003 min
Response: 70084690
Conc: 18.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
N48854-1040


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2022
Supervised By :Ankita Jodhani 09/19/2022

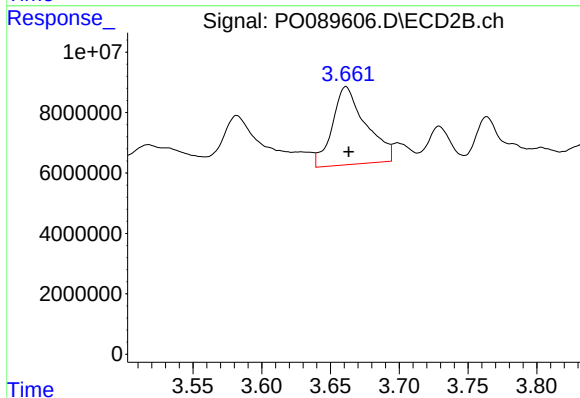


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: -0.002 min
Response: 43763609
Conc: 25.68 ng/ml

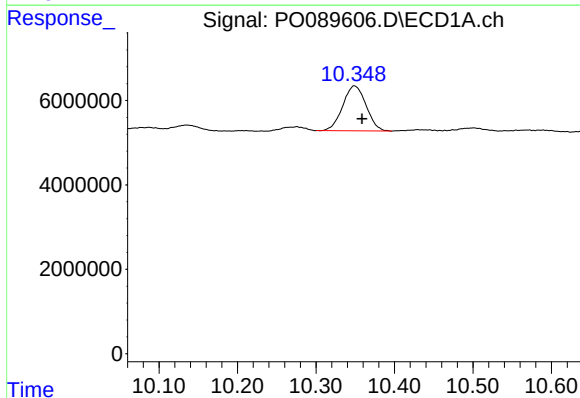

#2 Decachlorobiphenyl

R.T.: 10.349 min
Delta R.T.: -0.010 min
Response: 22049683
Conc: 8.93 ng/ml

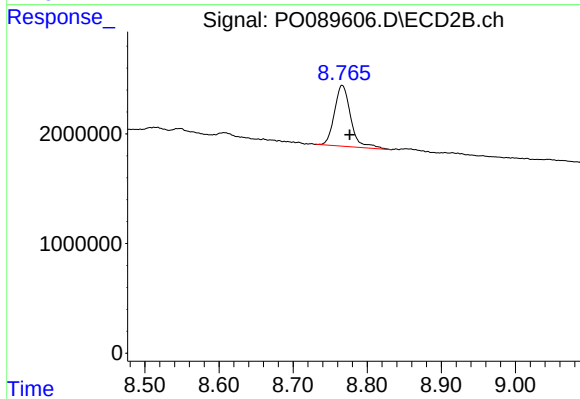

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.010 min
Response: 8502949
Conc: 7.54 ng/ml