

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091624\
 Data File : P0106595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2024 16:20
 Operator : YP/AJ
 Sample : P4009-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DN-B-34B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/17/2024
 Supervised By :Ankita Jodhani 09/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 02:08:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.713	164.7E6	56970724	21.963m	21.328
2) SA Decachlor...	10.192	8.736	75651382	31667047	15.305	15.832m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091624\
Data File : PO106595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2024 16:20
Operator : YP/AJ
Sample : P4009-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DN-B-34B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :Ankita Jodhani 09/17/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:08:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

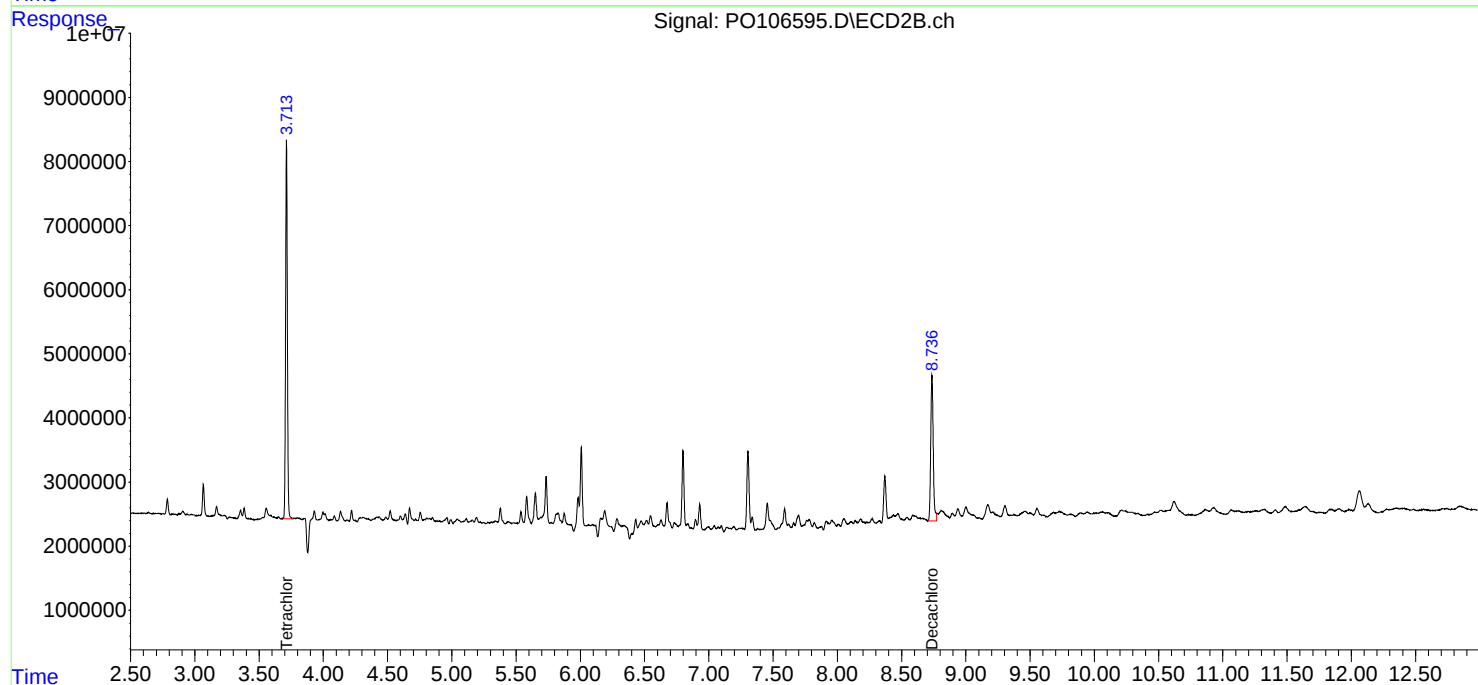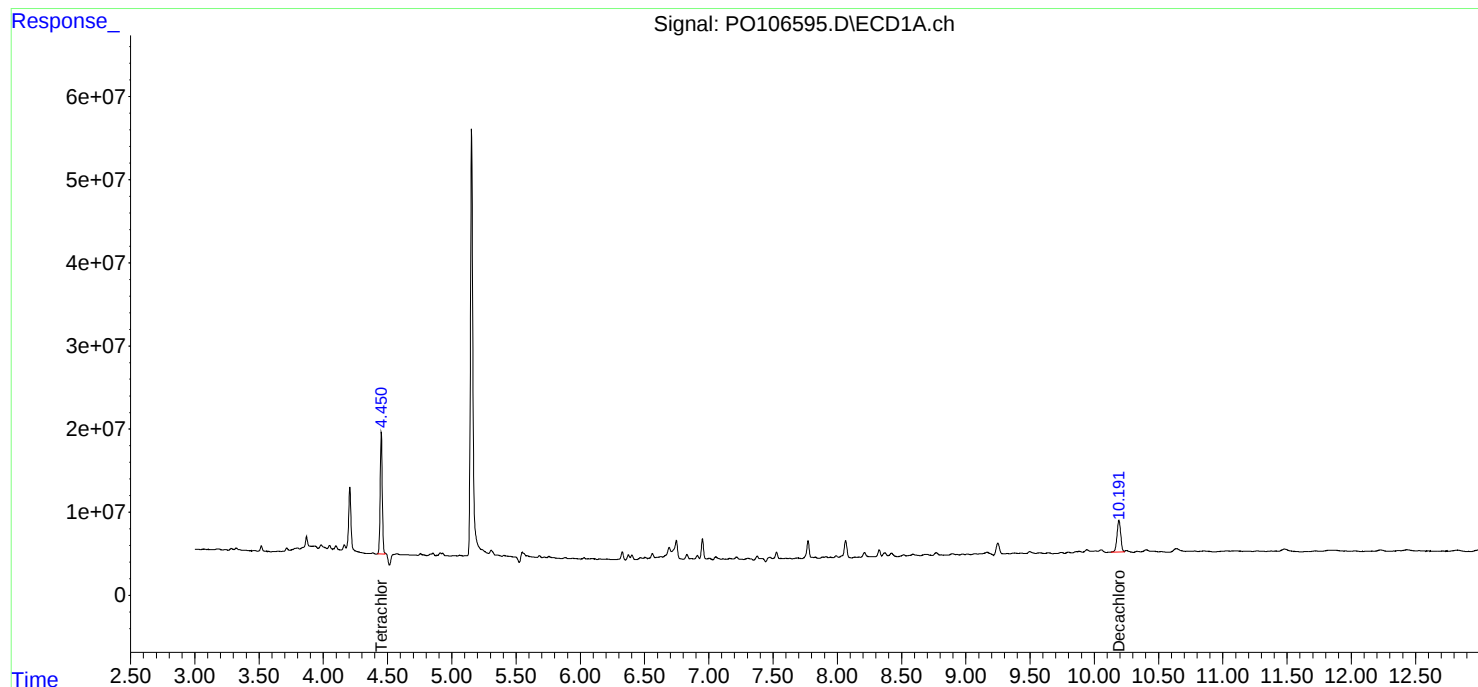

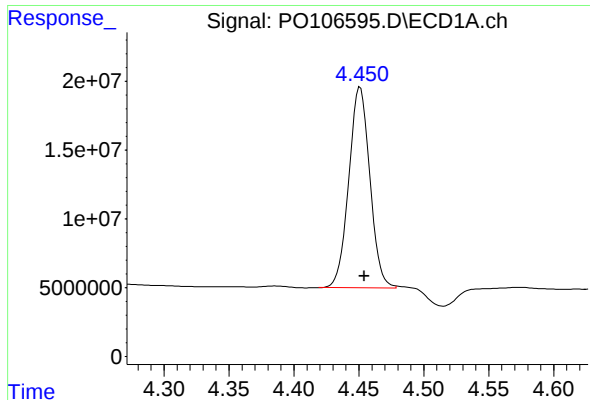


#1 Tetrachloro-m-xylene

R.T.: 4.450 min
Delta R.T.: -0.004 min
Response: 164749363
Conc: 21.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
DN-B-34B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :Ankita Jodhani 09/17/2024

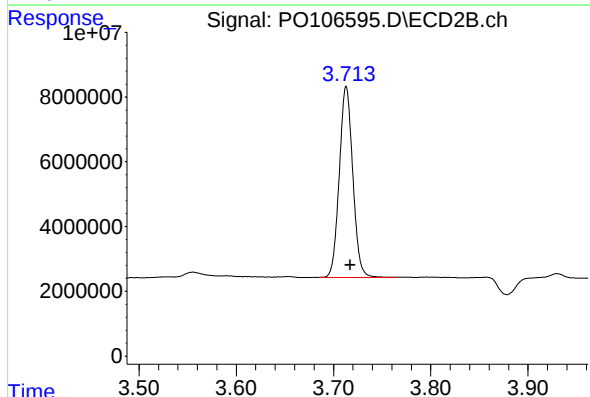


#1 Tetrachloro-m-xylene

R.T.: 3.713 min
Delta R.T.: -0.004 min
Response: 56970724
Conc: 21.33 ng/ml

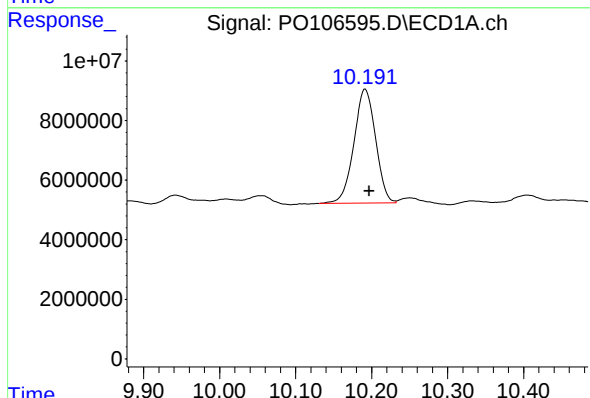

#2 Decachlorobiphenyl

R.T.: 10.192 min
Delta R.T.: -0.005 min
Response: 75651382
Conc: 15.31 ng/ml

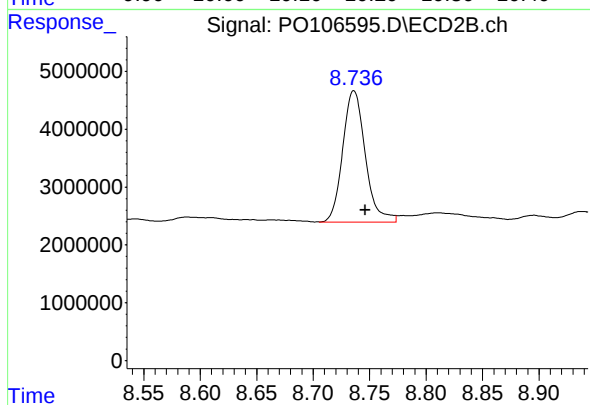

#2 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: -0.011 min
Response: 31667047
Conc: 15.83 ng/ml m