

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091624\
 Data File : P0106599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2024 17:33
 Operator : YP/AJ
 Sample : P3984-01RE
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-A-COMPRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/17/2024
 Supervised By :Ankita Jodhani 09/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 09:41:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.713	190.5E6	59956690	25.401m	22.445m
2) SA Decachlor...	10.192	8.735	260.1E6	116.6E6	52.620	58.309m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091624\
Data File : PO106599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2024 17:33
Operator : YP/AJ
Sample : P3984-01RE
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-A-COMPRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :Ankita Jodhani 09/17/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 09:41:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

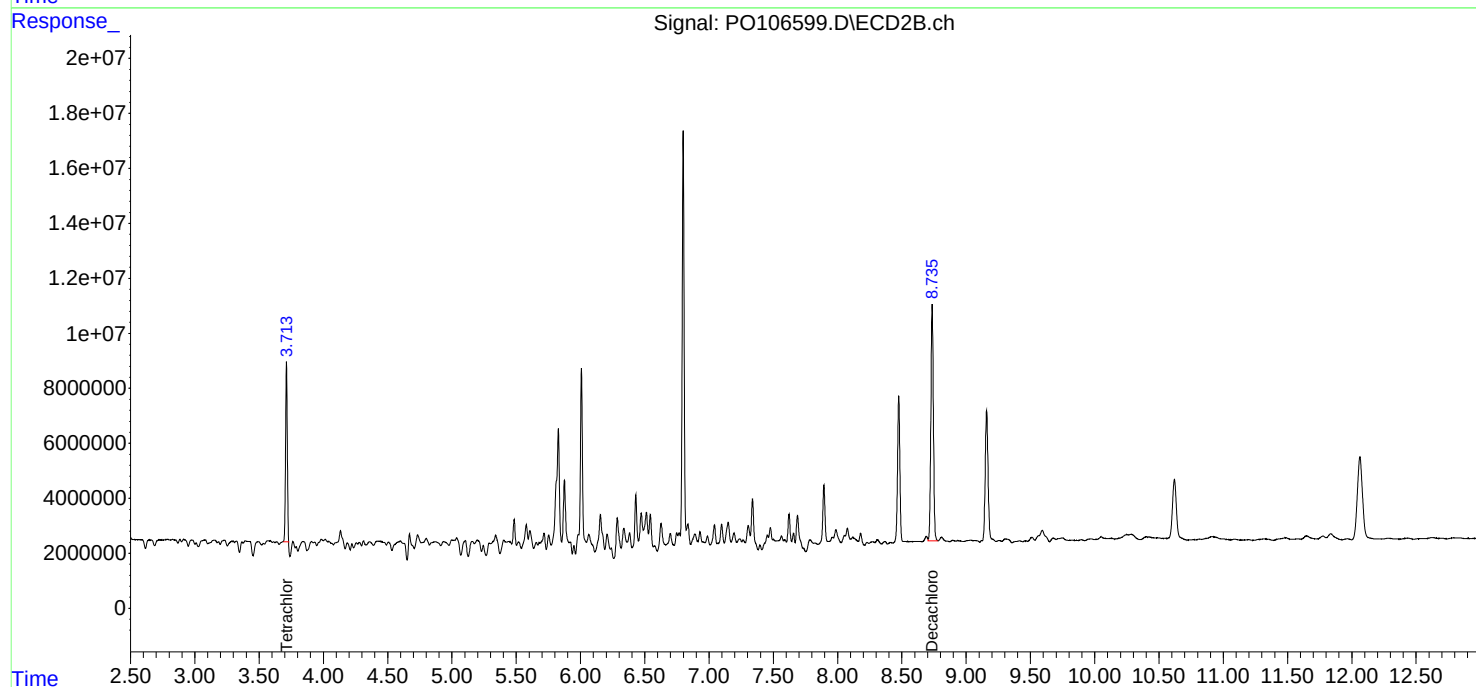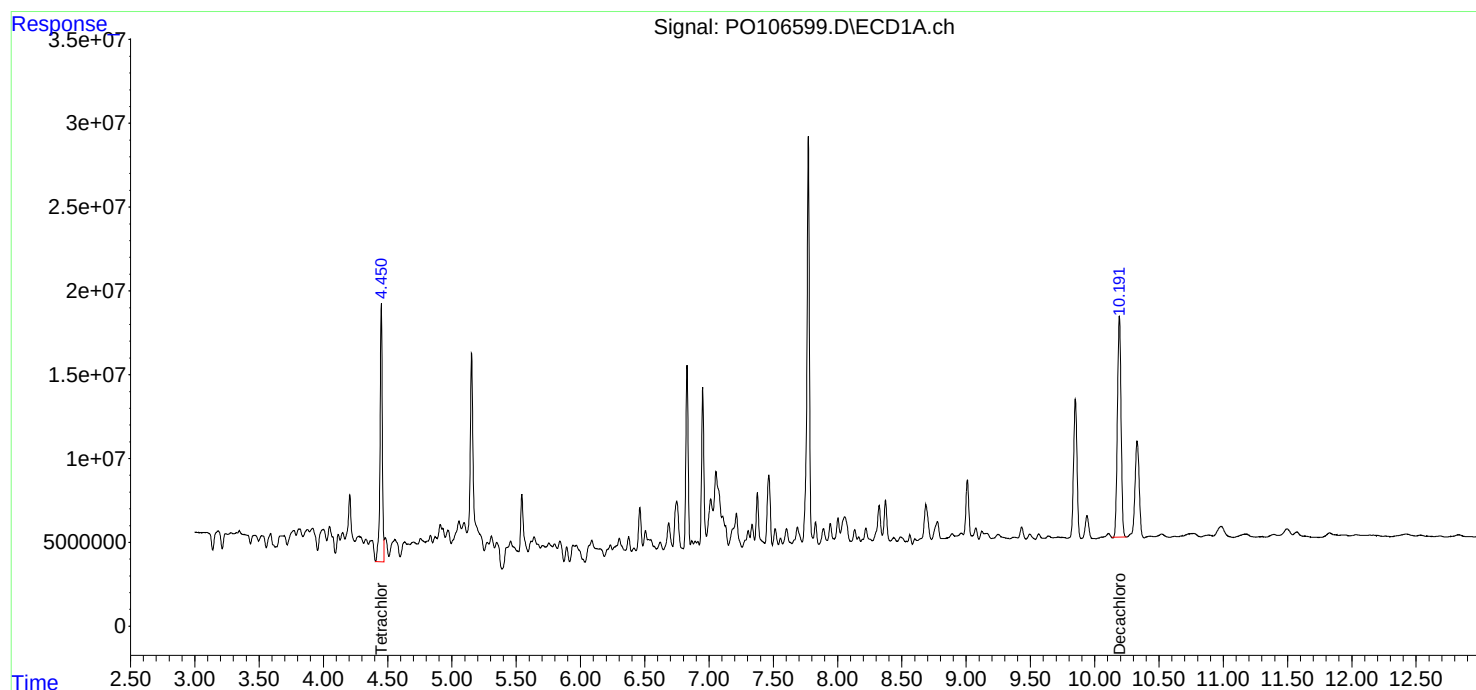

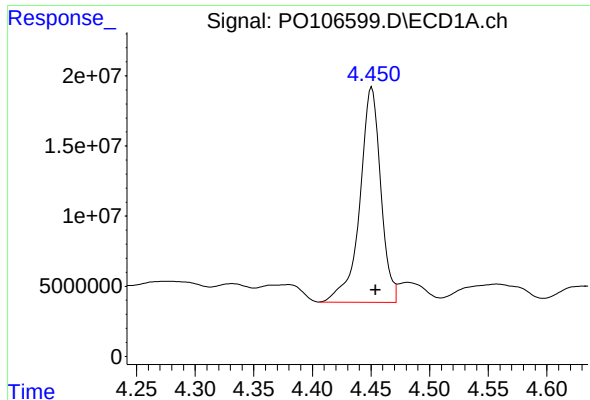


#1 Tetrachloro-m-xylene

R.T.: 4.450 min
Delta R.T.: -0.004 min
Response: 190539311
Conc: 25.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-A-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :Ankita Jodhani 09/17/2024

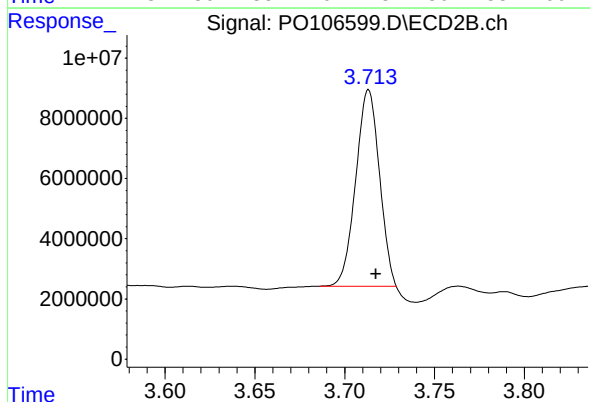


#1 Tetrachloro-m-xylene

R.T.: 3.713 min
Delta R.T.: -0.005 min
Response: 59956690
Conc: 22.45 ng/ml

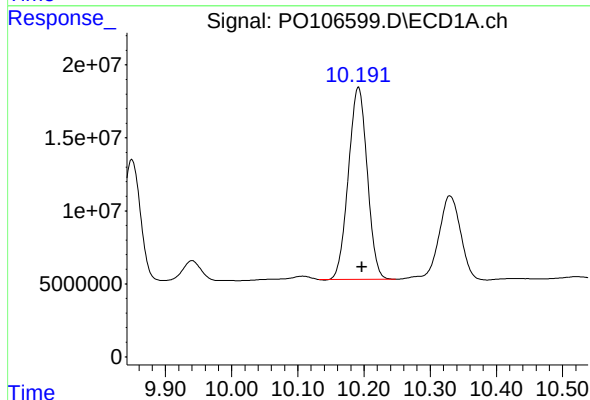

#2 Decachlorobiphenyl

R.T.: 10.192 min
Delta R.T.: -0.005 min
Response: 260092010
Conc: 52.62 ng/ml

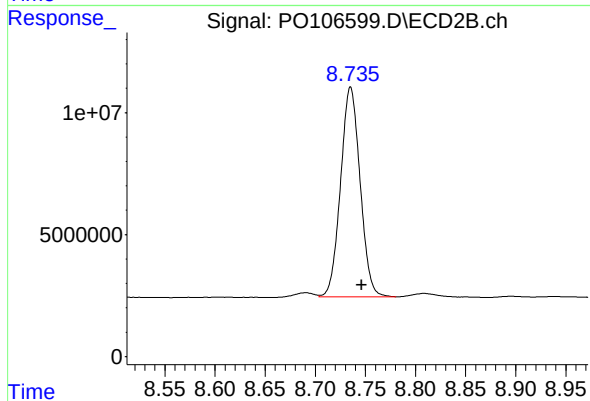

#2 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.012 min
Response: 116632819
Conc: 58.31 ng/ml