

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091718\
 Data File : P0049037.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2018 13:56
 Operator : SM/SJ
 Sample : PB112880BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 15:10:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 12 08:13:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.396	3.525	3451637	4473939	21.068	24.524
2)	SA Decachlor...	10.113	8.460	4575629	4182922	20.538	22.541
Target Compounds							
25)	L5 AR-1248-5	6.724	0.000	545310	0	104.051	N.D. #
29)	L6 AR-1254-4	7.335	0.000	764180	0	55.268	N.D. #
32)	L7 AR-1260-2	0.000	6.231	0	102027	N.D.	6.016 #
35)	L7 AR-1260-5	8.269	0.000	2957071	0	145.368	N.D. #
39)	L8 AR-1262-4	8.690	0.000	476024	0	44.046	N.D. #
40)	L8 AR-1262-5	9.405	0.000	539514	0	66.000	N.D. #
43)	L9 AR-1268-3	8.690	0.000	476024	0	18.159	N.D. #
45)	L9 AR-1268-5	9.790	0.000	370289	0	5.008	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091718\
Data File : PO049037.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2018 13:56
Operator : SM/SJ
Sample : PB112880BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 15:10:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 12 08:13:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

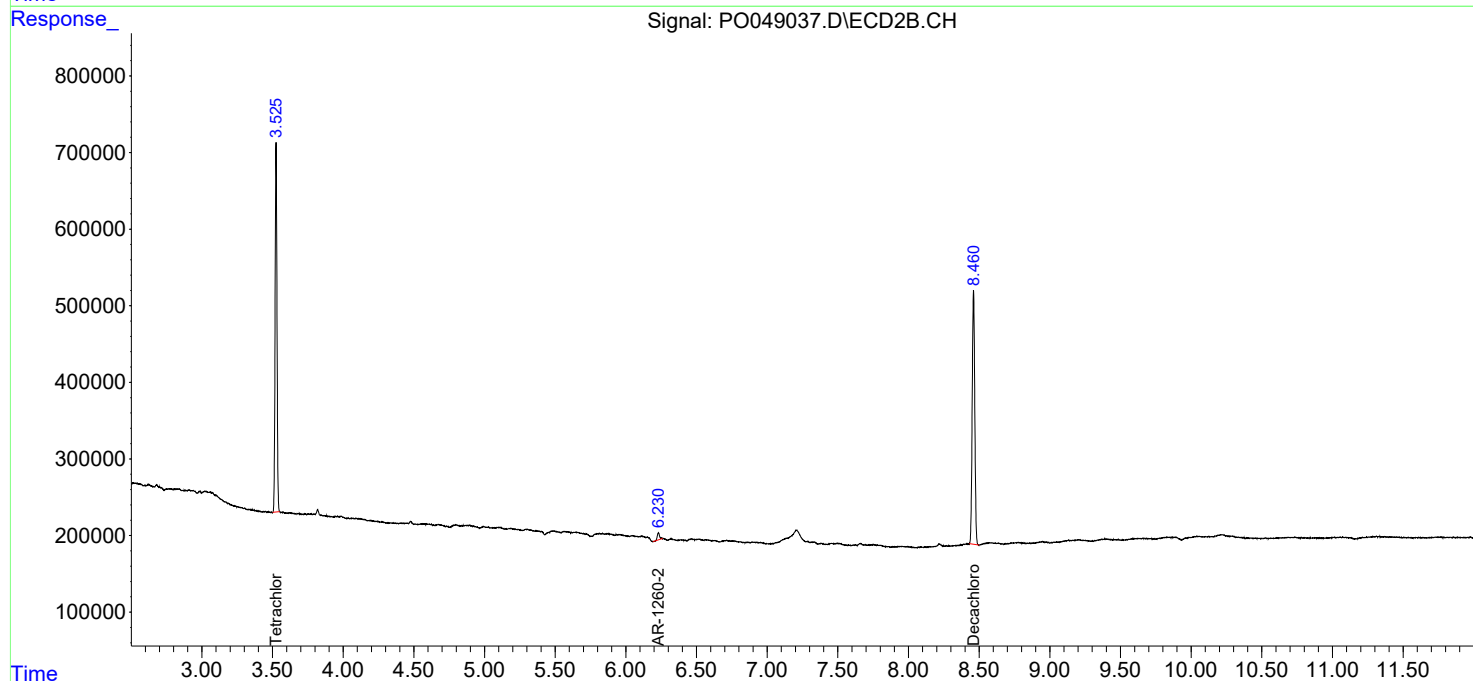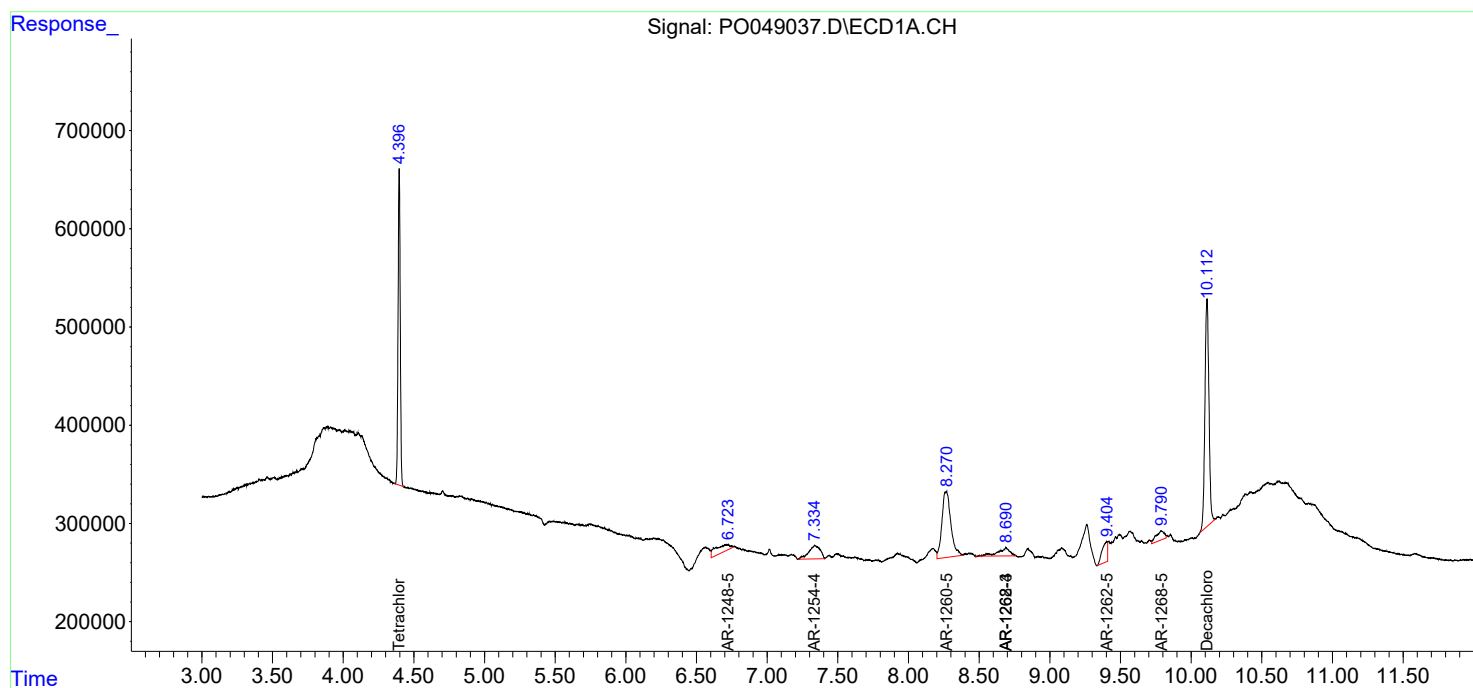


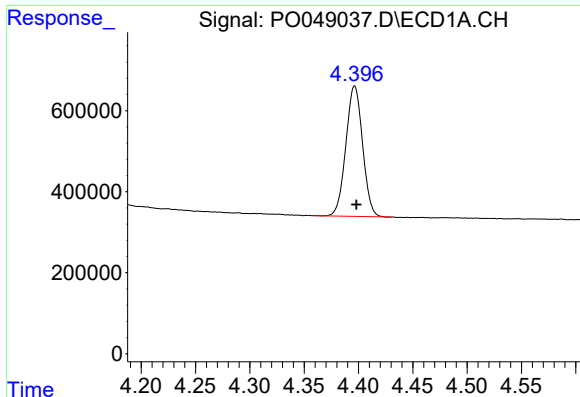

#1 Tetrachloro-m-xylene


R.T.: 4.396 min
Delta R.T.: -0.002 min
Response: 3451637
Conc: 21.07 ng/ml

Instrument :
ECD_O
ClientSampleId :

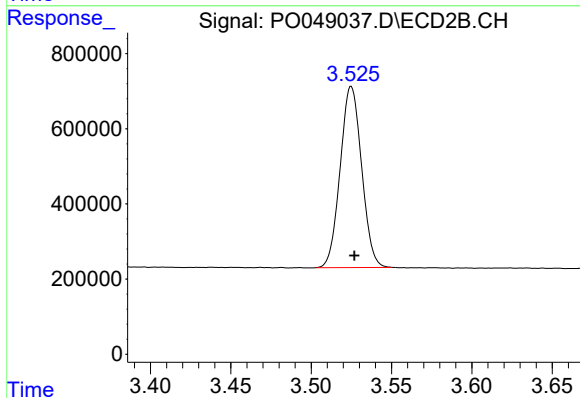


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.002 min
Response: 4473939
Conc: 24.52 ng/ml

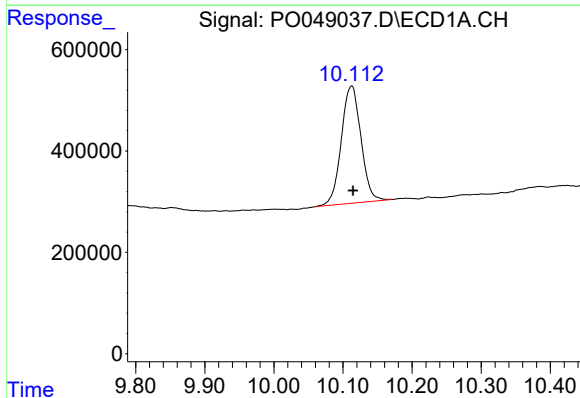


#2 Decachlorobiphenyl

R.T.: 10.113 min
Delta R.T.: -0.002 min
Response: 4575629
Conc: 20.54 ng/ml

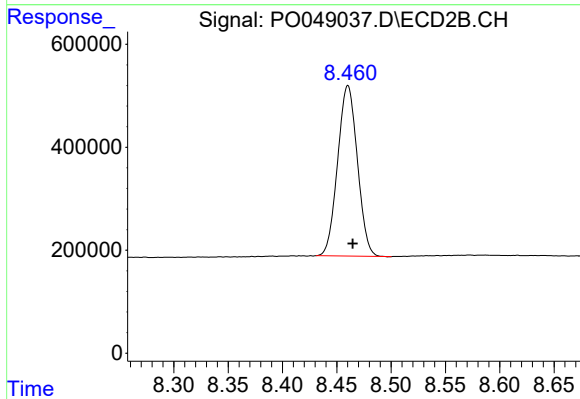

#2 Decachlorobiphenyl


R.T.: 8.460 min
Delta R.T.: -0.004 min
Response: 4182922
Conc: 22.54 ng/ml

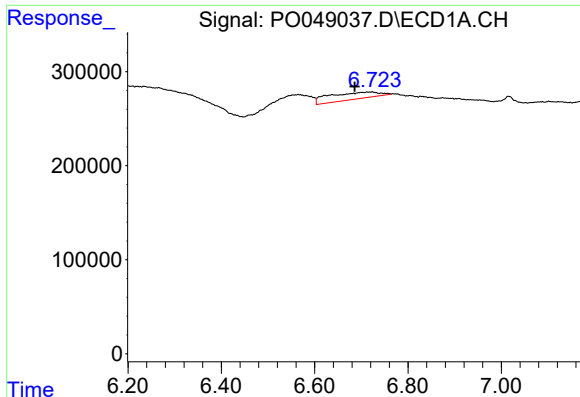

#25 AR-1248-5


R.T.: 6.724 min
Delta R.T.: 0.038 min
Response: 545310
Conc: 104.05 ng/ml

Instrument :
ECD_O
ClientSampleId :

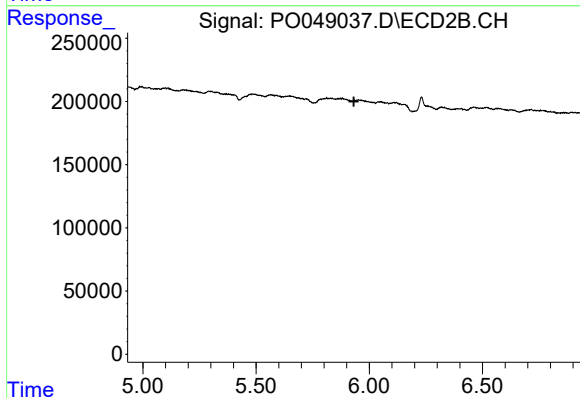


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.932 min
Response: 0
Conc: N.D.

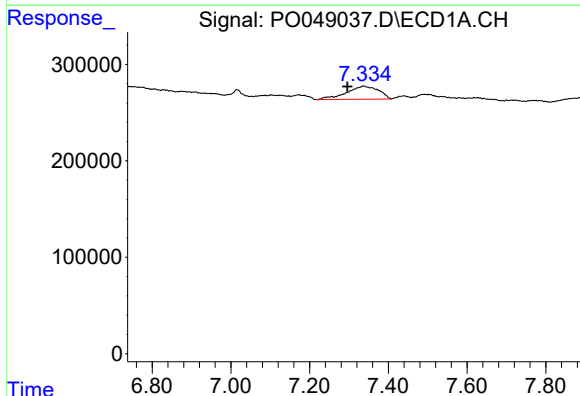


#29 AR-1254-4

R.T.: 7.335 min
Delta R.T.: 0.039 min
Response: 764180
Conc: 55.27 ng/ml

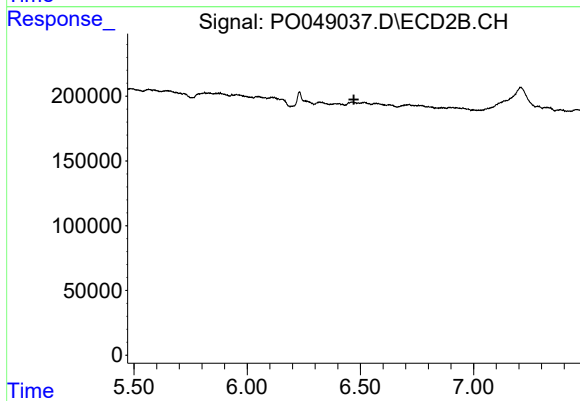

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.471 min
Response: 0
Conc: N.D.

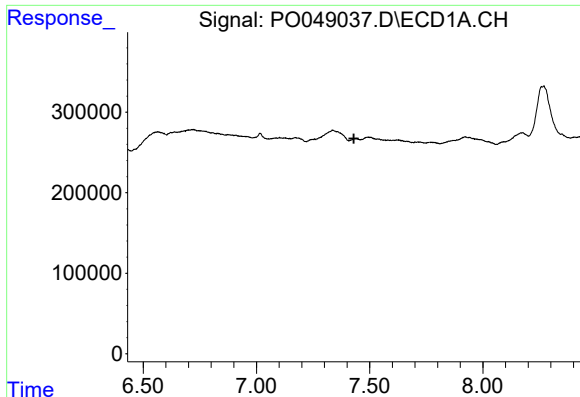

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

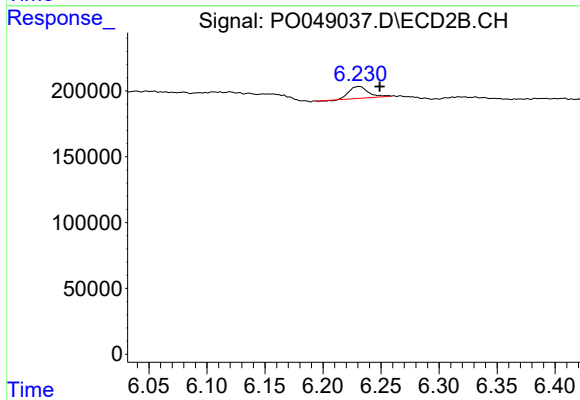


#32 AR-1260-2

R.T.: 6.231 min
Delta R.T.: -0.018 min
Response: 102027
Conc: 6.02 ng/ml

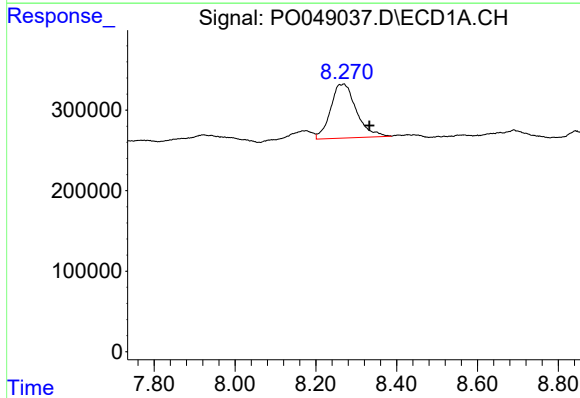


#35 AR-1260-5

R.T.: 8.269 min
Delta R.T.: -0.063 min
Response: 2957071
Conc: 145.37 ng/ml

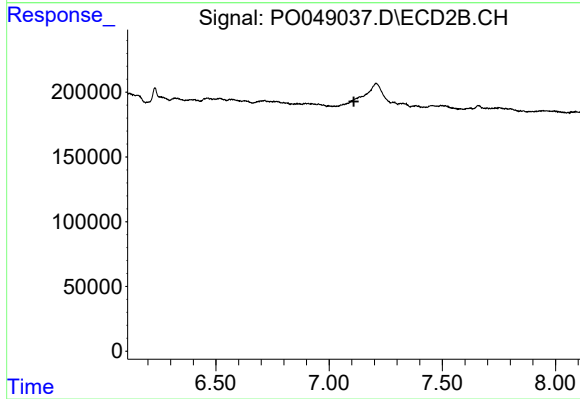

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.109 min
Response: 0
Conc: N.D.

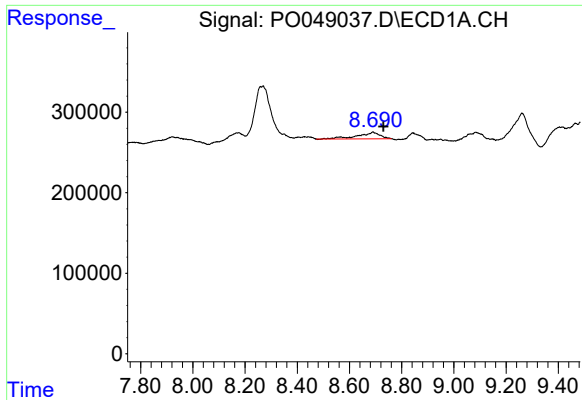

#39 AR-1262-4


R.T.: 8.690 min
Delta R.T.: -0.040 min
Response: 476024
Conc: 44.05 ng/ml

Instrument :
ECD_O
ClientSampleId :

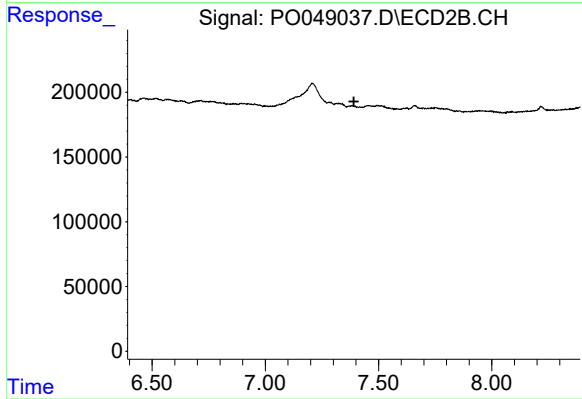


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.391 min
Response: 0
Conc: N.D.

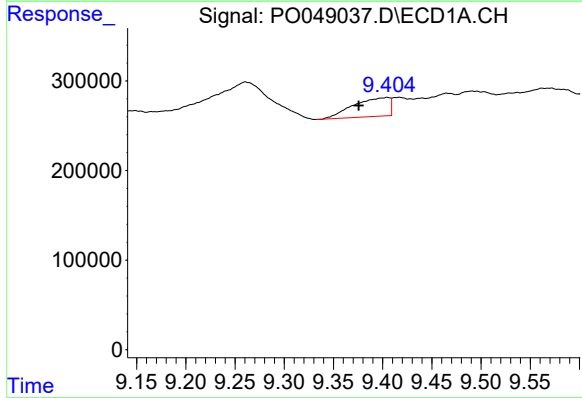


#40 AR-1262-5

R.T.: 9.405 min
Delta R.T.: 0.029 min
Response: 539514
Conc: 66.00 ng/ml

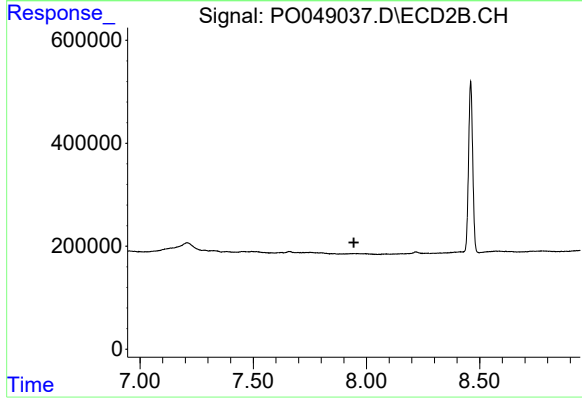

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 7.945 min
Response: 0
Conc: N.D.

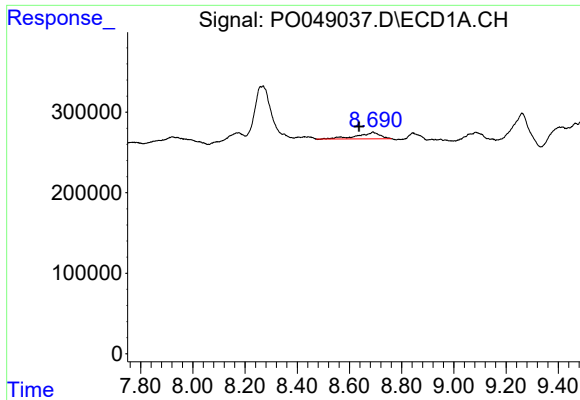

#43 AR-1268-3


R.T.: 8.690 min
Delta R.T.: 0.053 min
Response: 476024
Conc: 18.16 ng/ml

Instrument :
ECD_O
ClientSampleId :

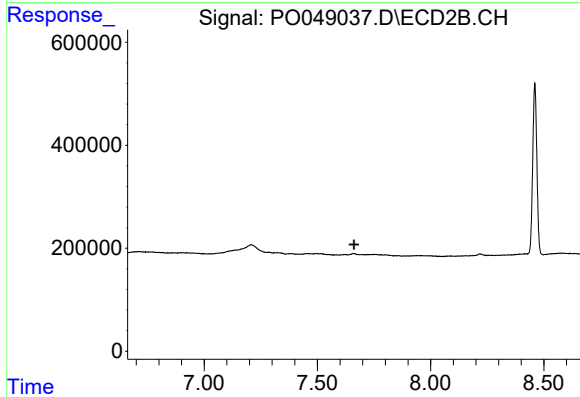


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.662 min
Response: 0
Conc: N.D.

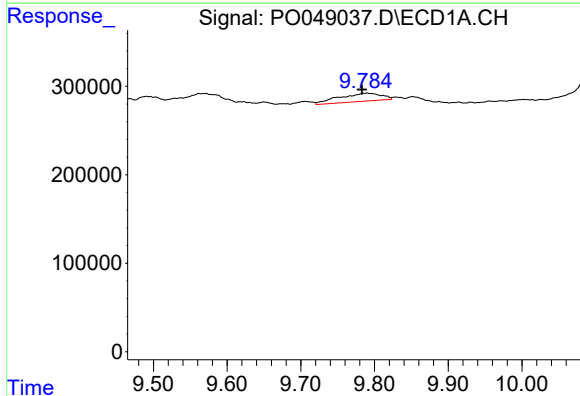

#45 AR-1268-5

R.T.: 9.790 min
Delta R.T.: 0.006 min
Response: 370289
Conc: 5.01 ng/ml

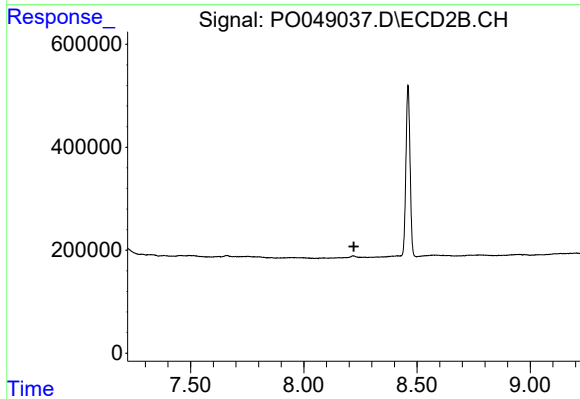

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.221 min
Response: 0
Conc: N.D.