

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091718\
 Data File : P0049055.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2018 19:50
 Operator : SM/SJ
 Sample : J4919-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ROLLOFF-03_COMP_FILL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 00:53:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 12 08:13:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.528	2833533	3997025	17.296	21.910m#
2) SA Decachlor...	10.114	8.463	2806144	2163823	12.595	11.661

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091718\
Data File : P0049055.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2018 19:50
Operator : SM/SJ
Sample : J4919-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ROLLOFF-03_COMP_FILL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 00:53:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 12 08:13:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

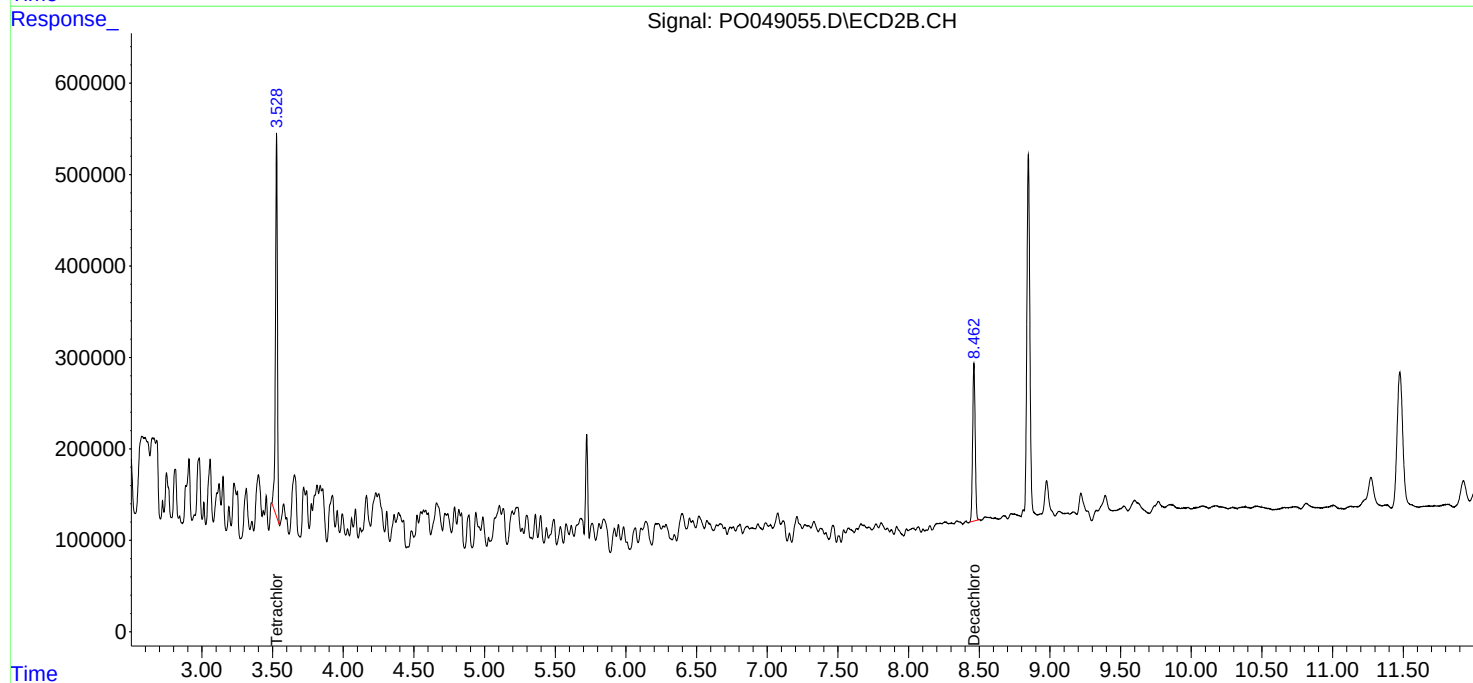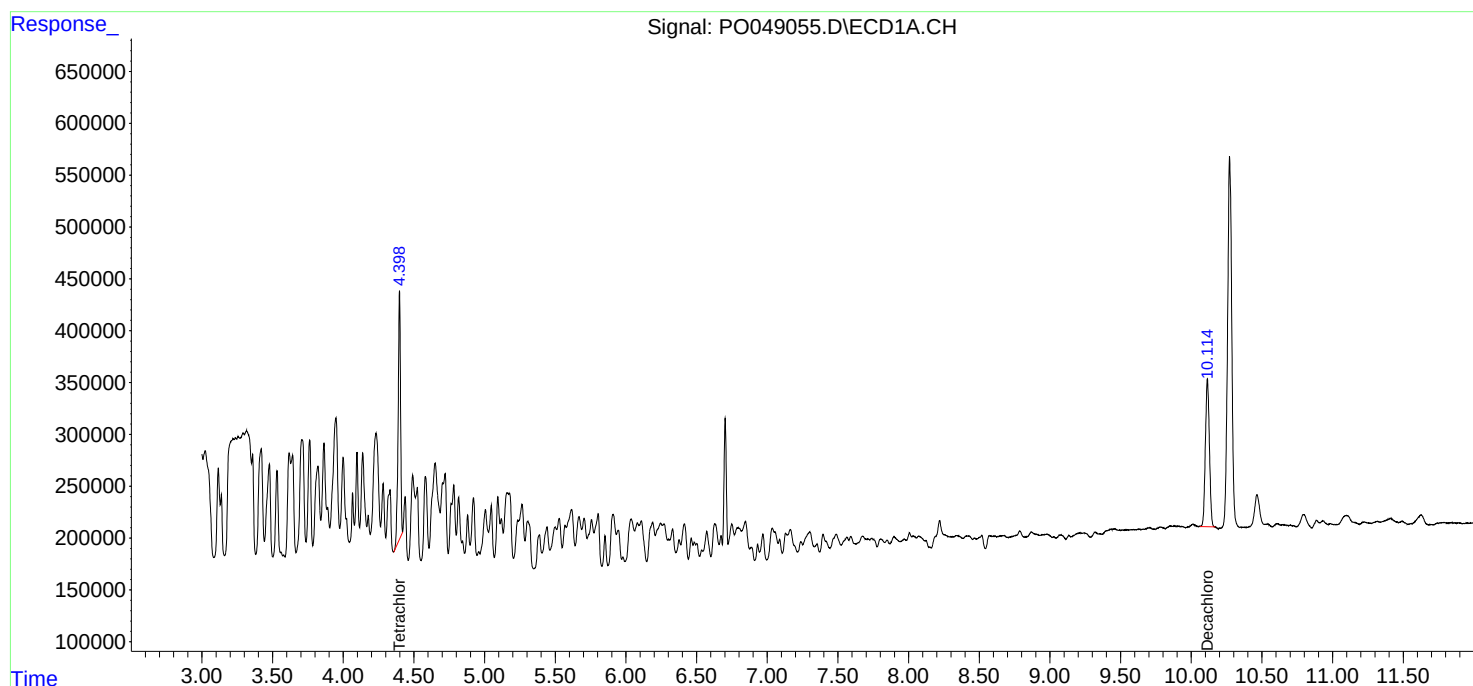


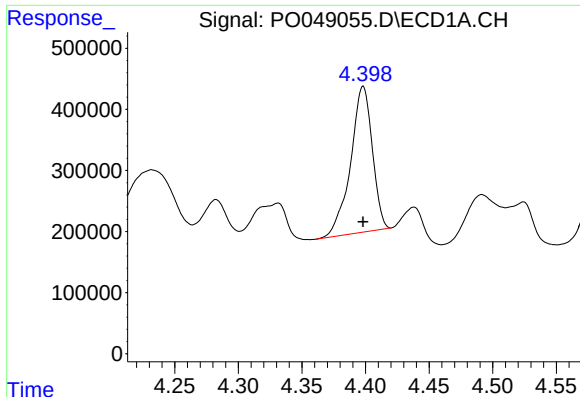

#1 Tetrachloro-m-xylene


R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 2833533
Conc: 17.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
ROLLOFF-03_COMP_FILL

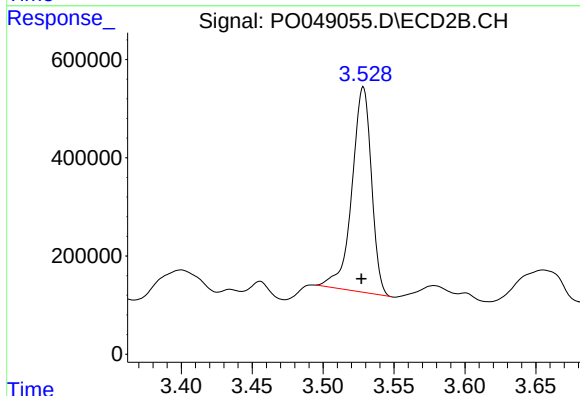


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: 0.001 min
Response: 3997025
Conc: 21.91 ng/ml m

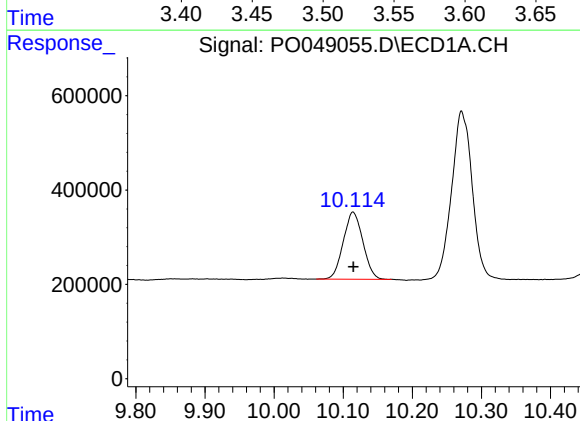

#2 Decachlorobiphenyl

R.T.: 10.114 min
Delta R.T.: 0.000 min
Response: 2806144
Conc: 12.60 ng/ml

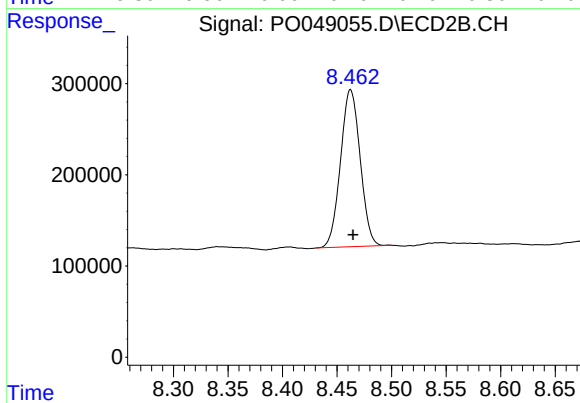

#2 Decachlorobiphenyl

R.T.: 8.463 min
Delta R.T.: -0.002 min
Response: 2163823
Conc: 11.66 ng/ml