

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
 Data File : P0061030.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 23:53
 Operator : SM/AJ
 Sample : K4923-04
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-40-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:22:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.371	3.532	1141181	883146	31.018	31.629
2)	SA Decachlor...	10.033	8.410	786506	571668	17.118	16.309
Target Compounds							
3)	L1 AR-1016-1	0.000	4.585	0	3769	N.D.	3.049 #
4)	L1 AR-1016-2	0.000	4.605	0	4296	N.D.	2.525 #
5)	L1 AR-1016-3	0.000	4.775	0	4383	N.D.	4.521 #
6)	L1 AR-1016-4	0.000	4.815	0	6443	N.D.	7.872 #
7)	L1 AR-1016-5	0.000	5.023	0	2695	N.D.	2.574 #
9)	L2 AR-1221-2	0.000	3.820	0	9538	N.D.	33.937 #
10)	L2 AR-1221-3	0.000	3.935	0	179	N.D.	0.216 #
11)	L3 AR-1232-1	0.000	3.935	0	179	N.D.	0.196 #
12)	L3 AR-1232-2	0.000	4.605	0	4296	N.D.	4.255 #
13)	L3 AR-1232-3	0.000	4.775	0	4383	N.D.	7.810 #
14)	L3 AR-1232-4	0.000	4.815	0	6443	N.D.	12.338 #
15)	L3 AR-1232-5	0.000	5.023	0	2695	N.D.	4.763 #
16)	L4 AR-1242-1	0.000	4.585	0	3769	N.D.	4.140 #
17)	L4 AR-1242-2	0.000	4.605	0	4296	N.D.	3.432 #
18)	L4 AR-1242-3	0.000	4.775	0	4383	N.D.	6.134 #
19)	L4 AR-1242-4	0.000	4.815	0	6443	N.D.	8.848 #
20)	L4 AR-1242-5	6.382	5.365	21156	34743	18.878	35.097 #
21)	L5 AR-1248-1	0.000	4.585	0	3769	N.D.	5.314 #
22)	L5 AR-1248-2	0.000	4.815	0	6443	N.D.	6.669 #
23)	L5 AR-1248-3	0.000	4.815	0	6443	N.D.	6.398 #
24)	L5 AR-1248-4	6.382	5.023	21156	2695	11.612	2.244 #
25)	L5 AR-1248-5	6.382	5.404	21156	11149	12.092	8.819 #
26)	L6 AR-1254-1	6.382	5.365	21156	34743	10.981	16.858 #
27)	L6 AR-1254-2	6.601	5.509	84689	33925	26.912	17.978 #
28)	L6 AR-1254-3	6.967	5.904	70696	84298	20.073	26.513 #
29)	L6 AR-1254-4	7.251	6.128	39318	31461	14.524	15.111
30)	L6 AR-1254-5	7.668	6.538	135687	107068	46.014	33.830 #
31)	L7 AR-1260-1	7.128	6.032	41394	55641	17.002	26.453 #
32)	L7 AR-1260-2	7.381	6.217	127844	50886	42.286	19.727 #
33)	L7 AR-1260-3	7.742	6.366	35168	49412	14.736	20.519 #
34)	L7 AR-1260-4	7.961	6.832	70558	27745	25.220	12.963 #
35)	L7 AR-1260-5	8.281	7.070	38287	53145	7.031	10.997 #
36)	L8 AR-1262-1	7.742	6.575	35168	41010	9.956	13.730 #
37)	L8 AR-1262-2	8.281	7.070	38287	53145	6.141	10.221 #
38)	L8 AR-1262-3	8.599	7.351	27895	14465	6.547	6.815
39)	L8 AR-1262-4	0.000	7.411	0	44783	N.D.	11.725 #
40)	L8 AR-1262-5	0.000	7.902	0	17729	N.D.	10.592 #
41)	L9 AR-1268-1	8.599	7.351	27895	14465	3.780	2.468 #
42)	L9 AR-1268-2	0.000	7.411	0	44783	N.D.	8.402 #
43)	L9 AR-1268-3	0.000	7.617	0	1920	N.D.	0.433 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
 Data File : P0061030.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 23:53
 Operator : SM/AJ
 Sample : K4923-04
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-40-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:22:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	0.000	7.902	0	17729	N.D.	9.278 #
45) L9	AR-1268-5	0.000	8.174	0	18452	N.D.	1.533 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091719\
Data File : PO061030.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2019 23:53
Operator : SM/AJ
Sample : K4923-04
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:22:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

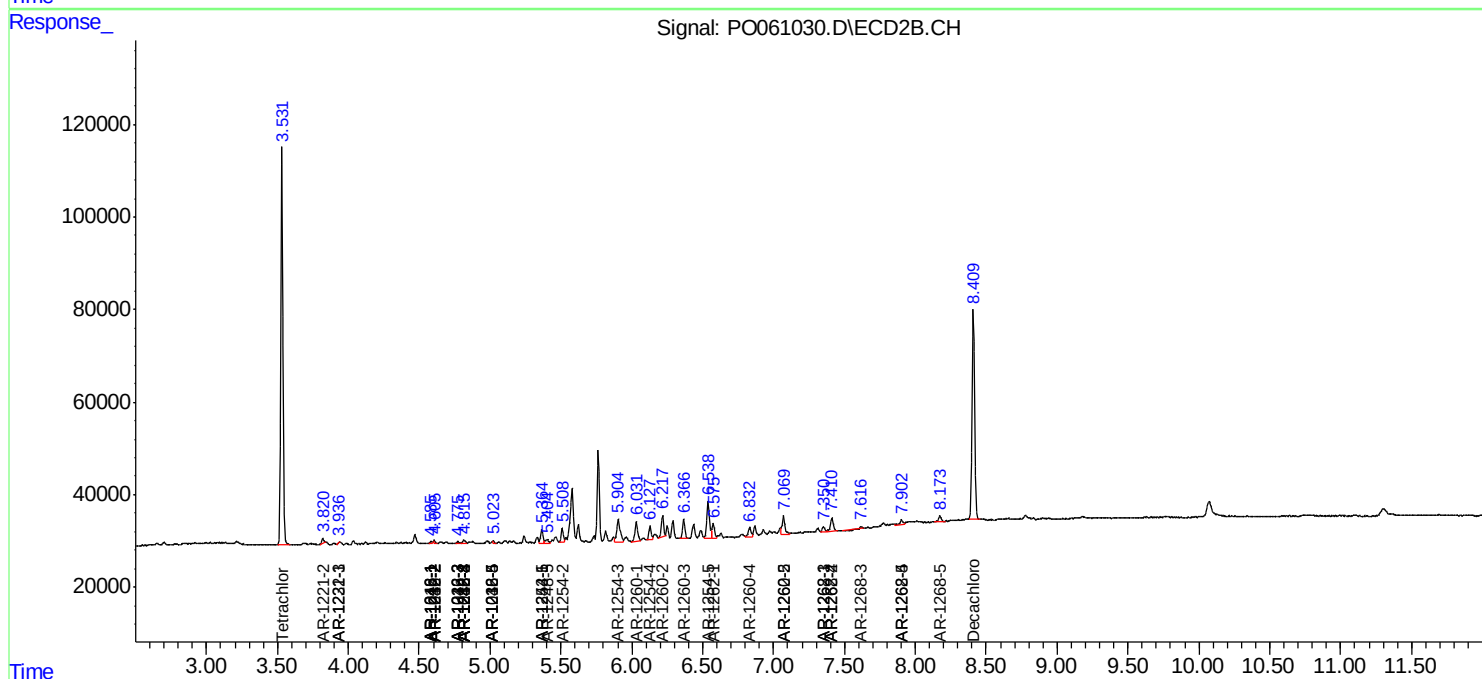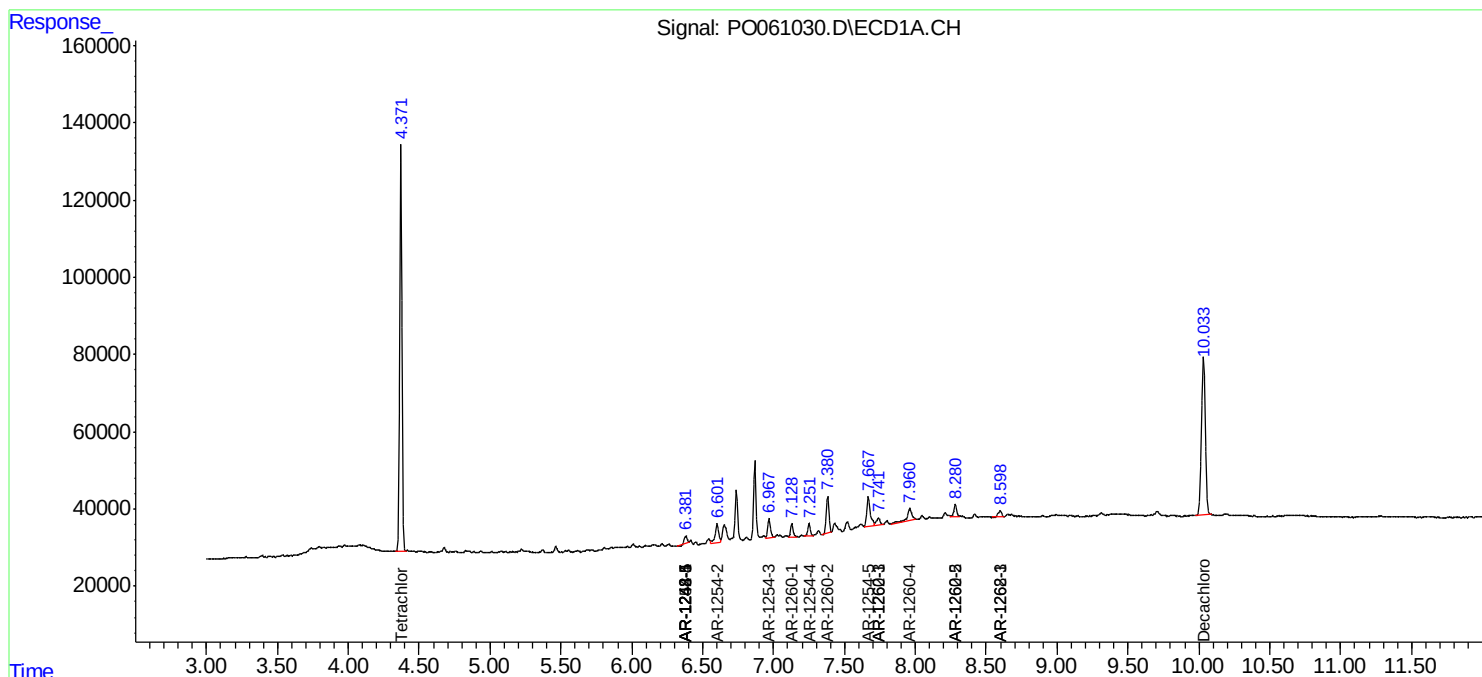




#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 1141181
Conc: 31.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

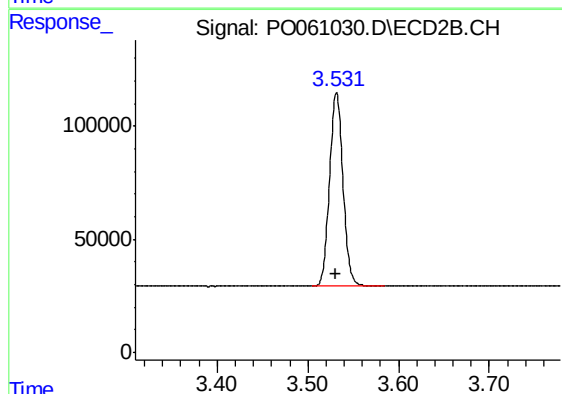


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 883146
Conc: 31.63 ng/ml

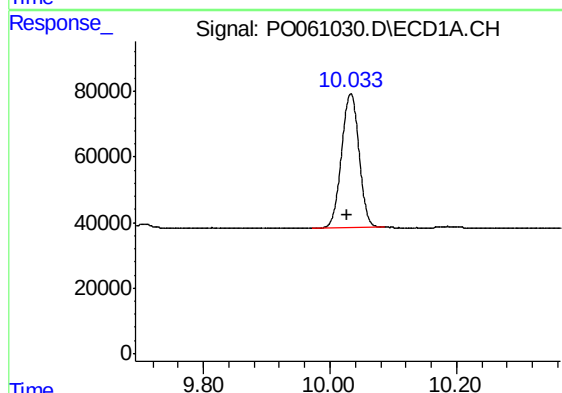


#2 Decachlorobiphenyl

R.T.: 10.033 min
Delta R.T.: 0.005 min
Response: 786506
Conc: 17.12 ng/ml

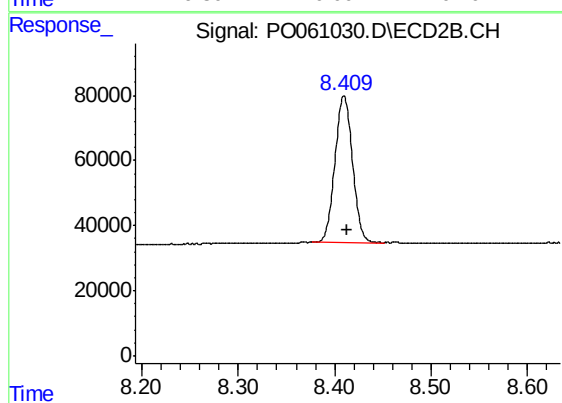

#2 Decachlorobiphenyl


R.T.: 8.410 min
Delta R.T.: -0.003 min
Response: 571668
Conc: 16.31 ng/ml

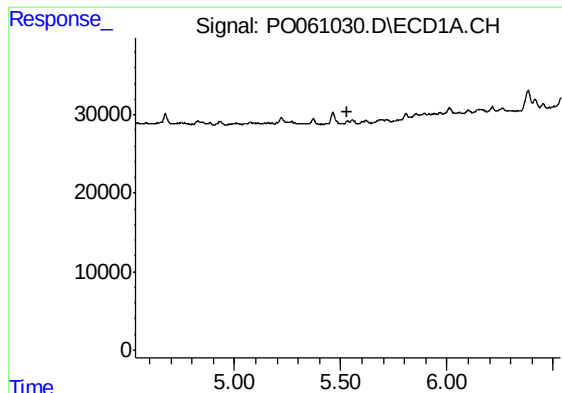

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T. : 5.533 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

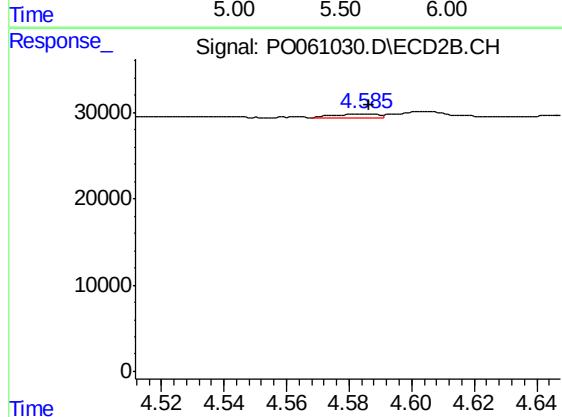


#3 AR-1016-1

R.T.: 4.585 min
Delta R.T.: -0.001 min
Response: 3769
Conc: 3.05 ng/ml

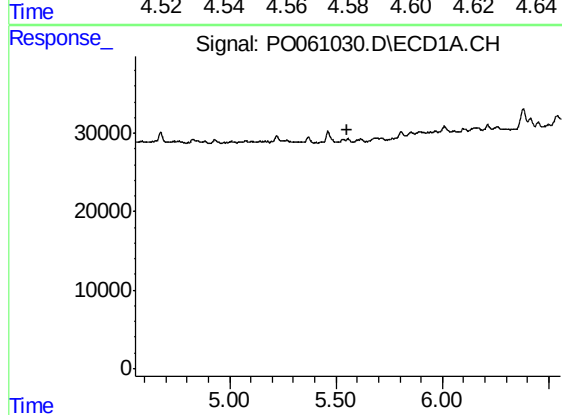


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.556 min
Response: 0
Conc: N.D.

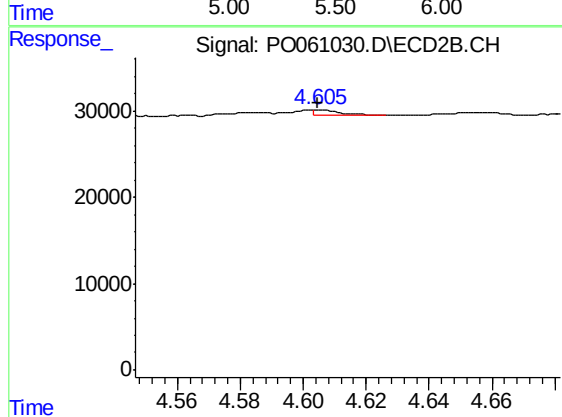

#4 AR-1016-2


R.T.: 4.605 min
Delta R.T.: 0.000 min
Response: 4296
Conc: 2.53 ng/ml

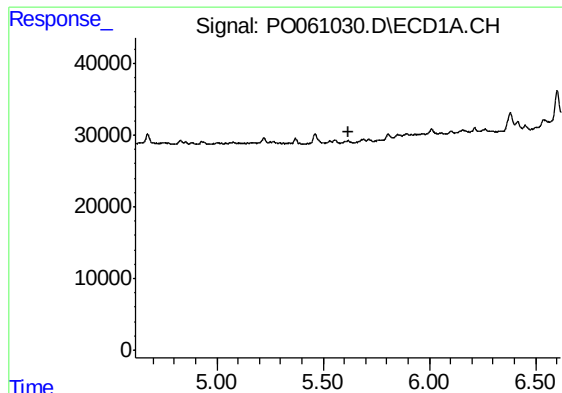

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T. : 5.617 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

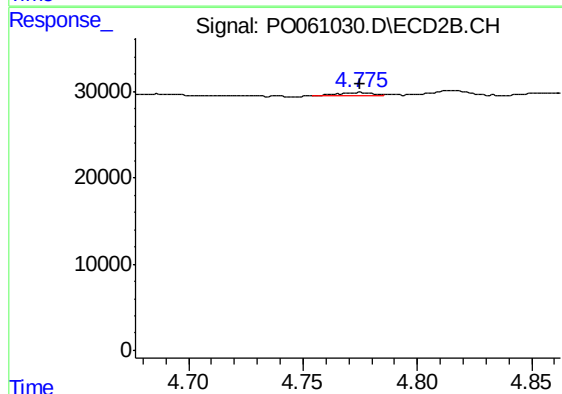


#5 AR-1016-3

R.T.: 4.775 min
Delta R.T.: 0.000 min
Response: 4383
Conc: 4.52 ng/ml

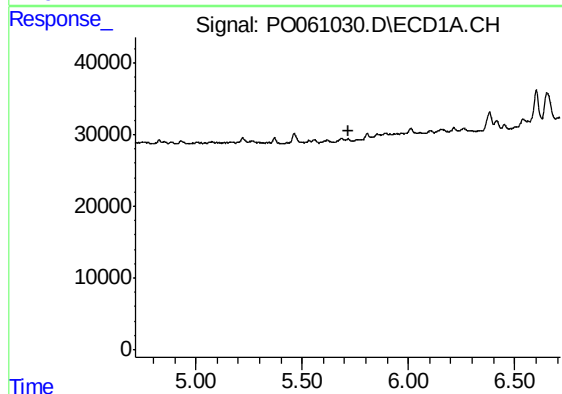


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.716 min
Response: 0
Conc: N.D.

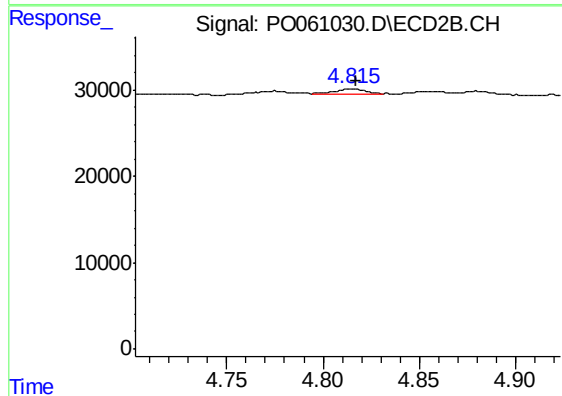

#6 AR-1016-4


R.T.: 4.815 min
Delta R.T.: -0.002 min
Response: 6443
Conc: 7.87 ng/ml



#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP




#7 AR-1016-5

R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 2695
Conc: 2.57 ng/ml




#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.664 min
Response: 0
Conc: N.D.

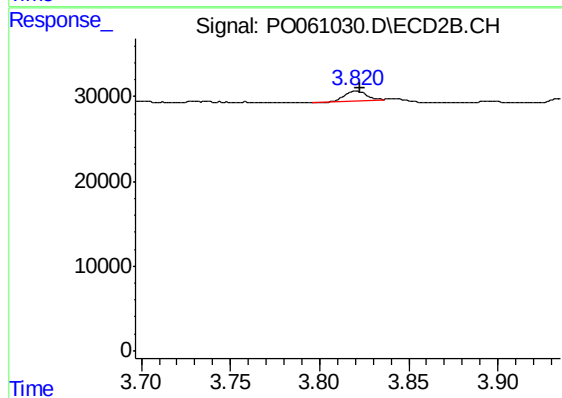

#9 AR-1221-2


R.T.: 3.820 min
Delta R.T.: -0.003 min
Response: 9538
Conc: 33.94 ng/ml



#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.741 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

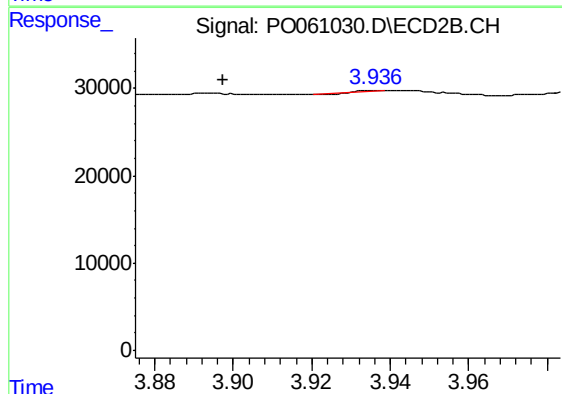


#10 AR-1221-3

R.T.: 3.935 min
Delta R.T.: 0.038 min
Response: 179
Conc: 0.22 ng/ml




#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.741 min
Response: 0
Conc: N.D.

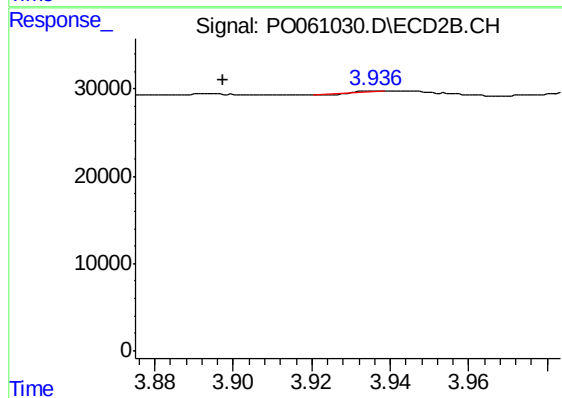

#11 AR-1232-1


R.T.: 3.935 min
Delta R.T.: 0.038 min
Response: 179
Conc: 0.20 ng/ml

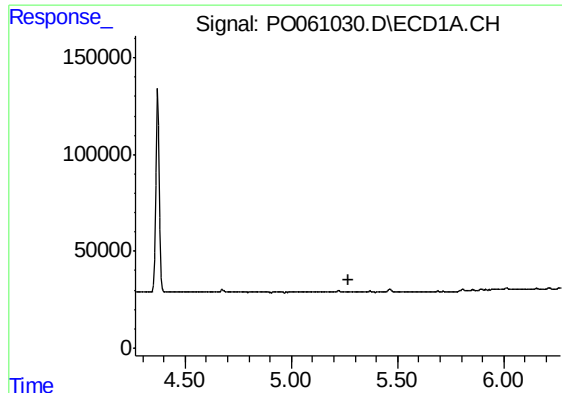

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

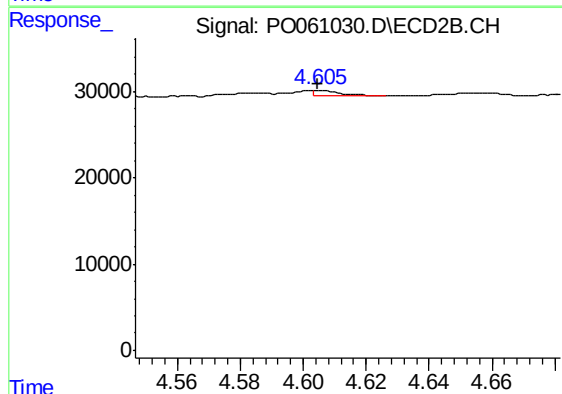


#12 AR-1232-2

R.T.: 4.605 min
Delta R.T.: 0.000 min
Response: 4296
Conc: 4.26 ng/ml

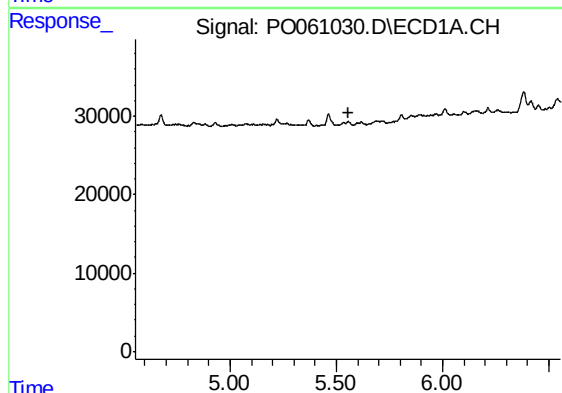


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 5.555 min
Response: 0
Conc: N.D.

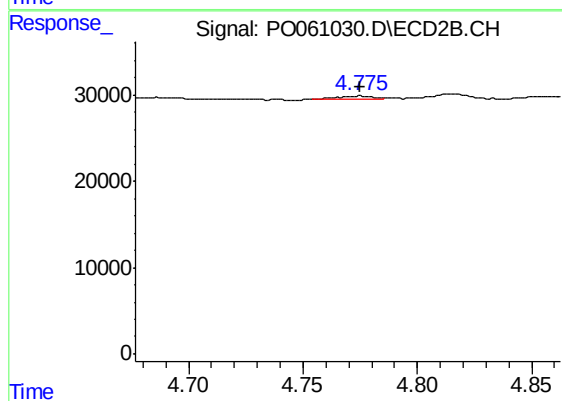

#13 AR-1232-3


R.T.: 4.775 min
Delta R.T.: 0.000 min
Response: 4383
Conc: 7.81 ng/ml

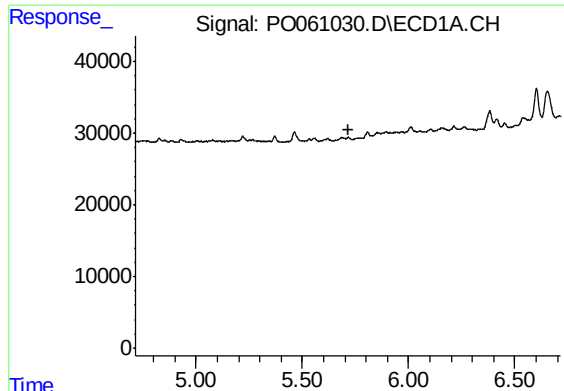

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 5.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

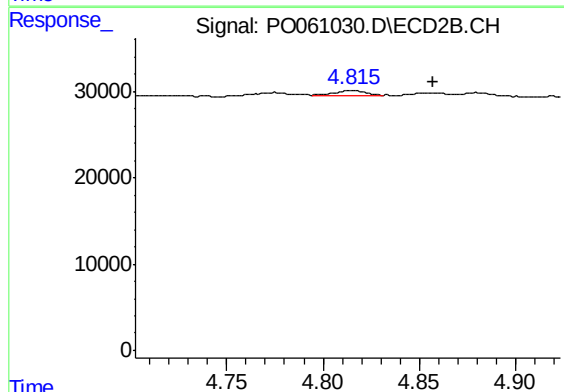


#14 AR-1232-4

R.T.: 4.815 min
Delta R.T.: -0.042 min
Response: 6443
Conc: 12.34 ng/ml

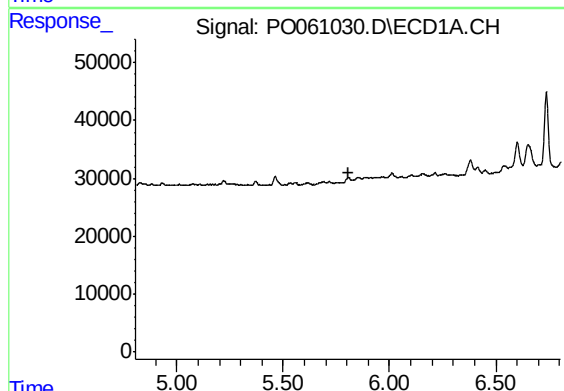


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.805 min
Response: 0
Conc: N.D.

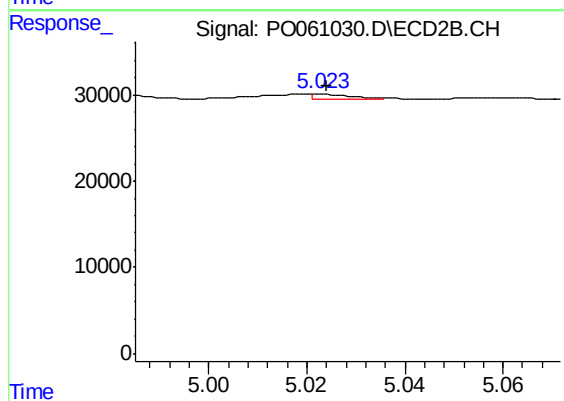

#15 AR-1232-5


R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 2695
Conc: 4.76 ng/ml



#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 5.533 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

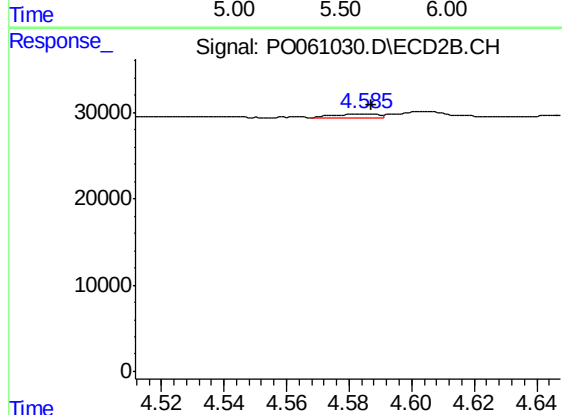


#16 AR-1242-1

R.T.: 4.585 min
Delta R.T.: -0.002 min
Response: 3769
Conc: 4.14 ng/ml

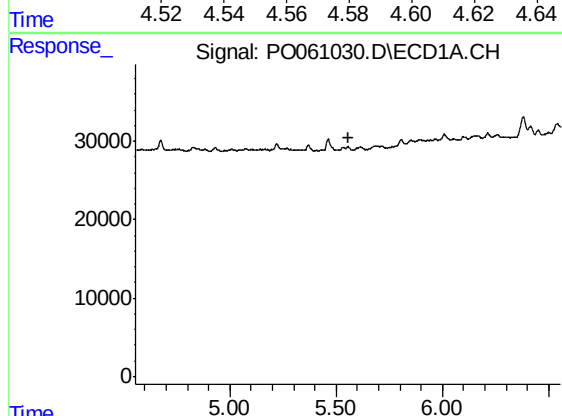


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 5.556 min
Response: 0
Conc: N.D.

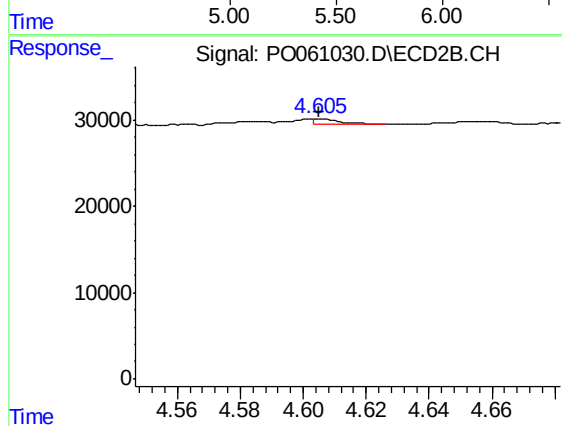

#17 AR-1242-2


R.T.: 4.605 min
Delta R.T.: 0.000 min
Response: 4296
Conc: 3.43 ng/ml



#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.617 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP




#18 AR-1242-3

R.T.: 4.775 min
Delta R.T.: 0.000 min
Response: 4383
Conc: 6.13 ng/ml




#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.715 min
Response: 0
Conc: N.D.

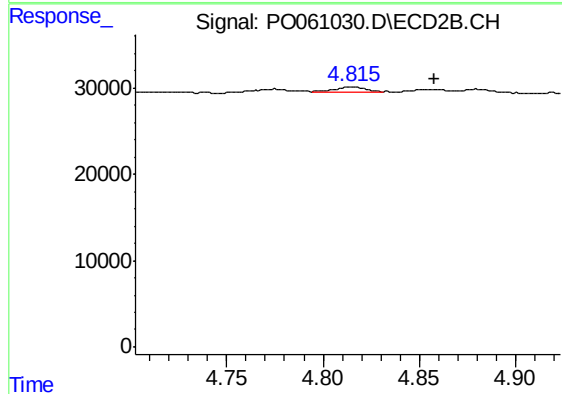

#19 AR-1242-4


R.T.: 4.815 min
Delta R.T.: -0.043 min
Response: 6443
Conc: 8.85 ng/ml

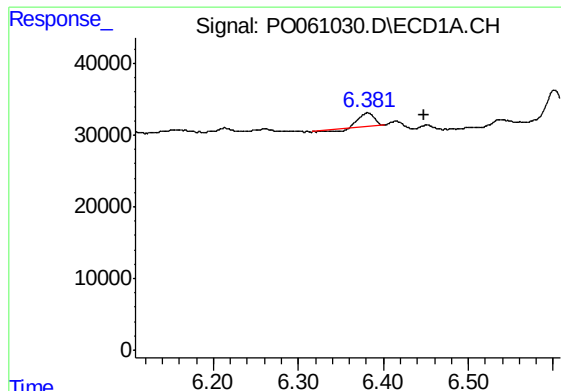

#20 AR-1242-5


R.T.: 6.382 min
Delta R.T.: -0.067 min
Response: 21156
Conc: 18.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

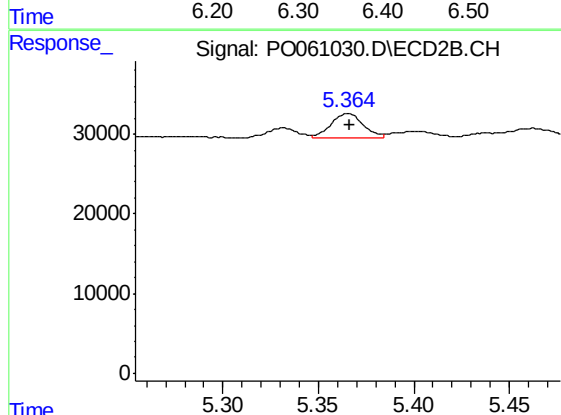


#20 AR-1242-5

R.T.: 5.365 min
Delta R.T.: -0.002 min
Response: 34743
Conc: 35.10 ng/ml

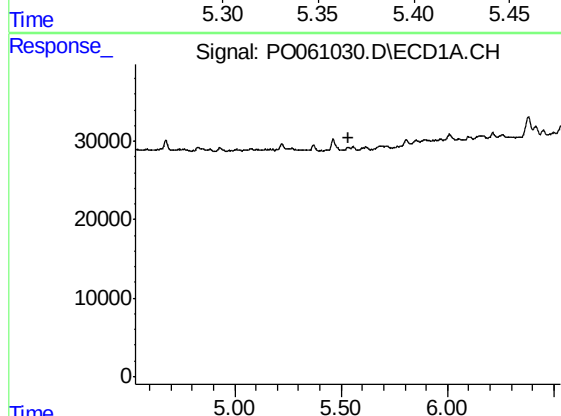


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.532 min
Response: 0
Conc: N.D.

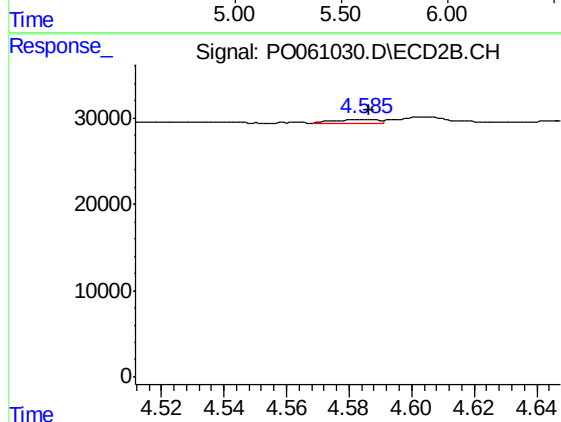

#21 AR-1248-1


R.T.: 4.585 min
Delta R.T.: -0.001 min
Response: 3769
Conc: 5.31 ng/ml

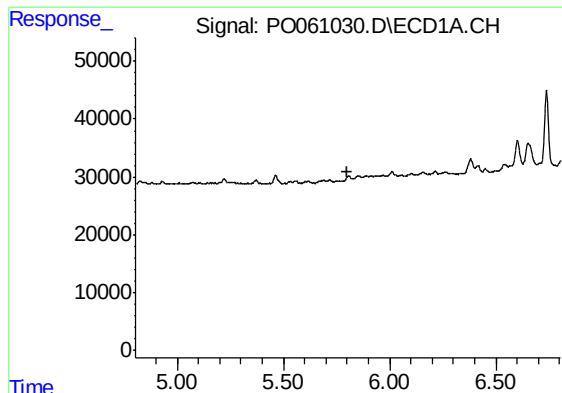

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 5.804 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP




#22 AR-1248-2

R.T.: 4.815 min
Delta R.T.: -0.002 min
Response: 6443
Conc: 6.67 ng/ml




#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 6.007 min
Response: 0
Conc: N.D.

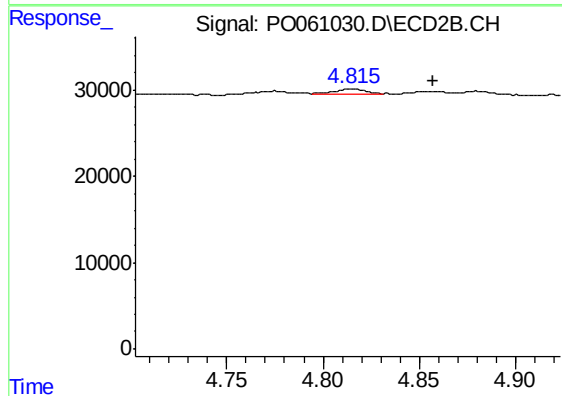

#23 AR-1248-3


R.T.: 4.815 min
Delta R.T.: -0.042 min
Response: 6443
Conc: 6.40 ng/ml



#24 AR-1248-4


R.T.: 6.382 min
Delta R.T.: -0.028 min
Response: 21156
Conc: 11.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP




#24 AR-1248-4

R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 2695
Conc: 2.24 ng/ml




#25 AR-1248-5

R.T.: 6.382 min
Delta R.T.: -0.066 min
Response: 21156
Conc: 12.09 ng/ml

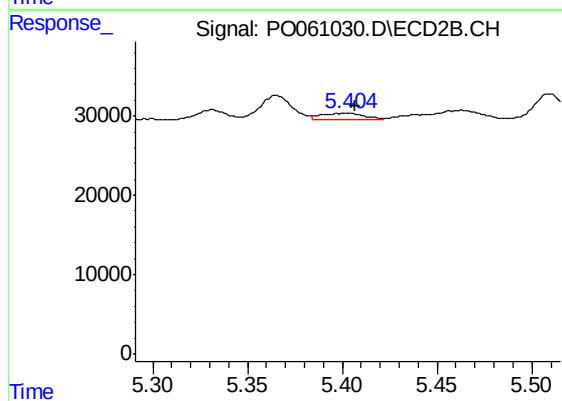

#25 AR-1248-5


R.T.: 5.404 min
Delta R.T.: -0.003 min
Response: 11149
Conc: 8.82 ng/ml



#26 AR-1254-1


R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 21156
Conc: 10.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

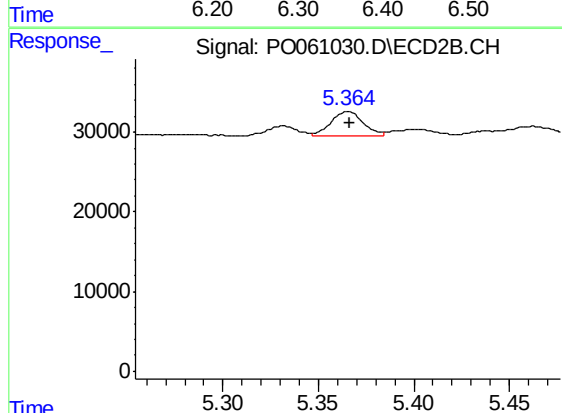


#26 AR-1254-1

R.T.: 5.365 min
Delta R.T.: -0.001 min
Response: 34743
Conc: 16.86 ng/ml

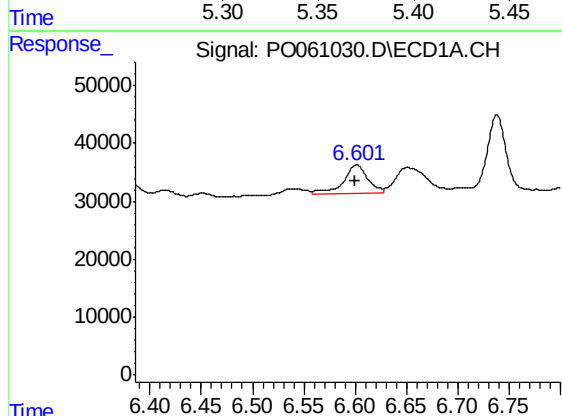


#27 AR-1254-2

R.T.: 6.601 min
Delta R.T.: 0.002 min
Response: 84689
Conc: 26.91 ng/ml

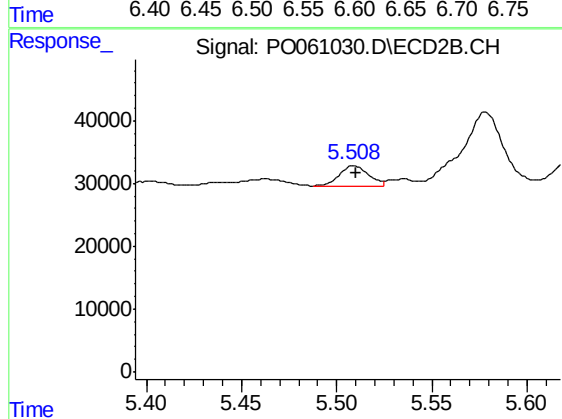

#27 AR-1254-2


R.T.: 5.509 min
Delta R.T.: -0.002 min
Response: 33925
Conc: 17.98 ng/ml



#28 AR-1254-3


R.T.: 6.967 min
Delta R.T.: 0.002 min
Response: 70696
Conc: 20.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP




#28 AR-1254-3

R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 84298
Conc: 26.51 ng/ml




#29 AR-1254-4

R.T.: 7.251 min
Delta R.T.: 0.001 min
Response: 39318
Conc: 14.52 ng/ml

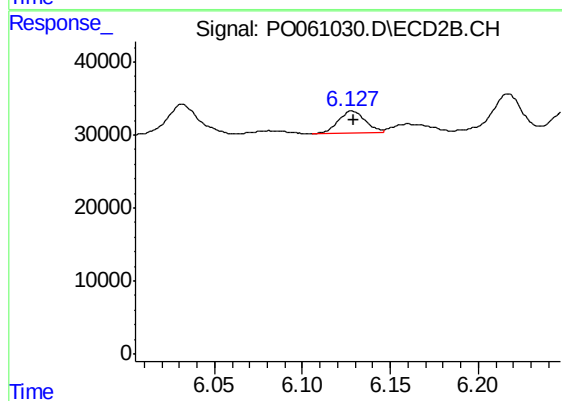

#29 AR-1254-4


R.T.: 6.128 min
Delta R.T.: -0.001 min
Response: 31461
Conc: 15.11 ng/ml



#30 AR-1254-5


R.T.: 7.668 min
Delta R.T.: 0.001 min
Response: 135687
Conc: 46.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

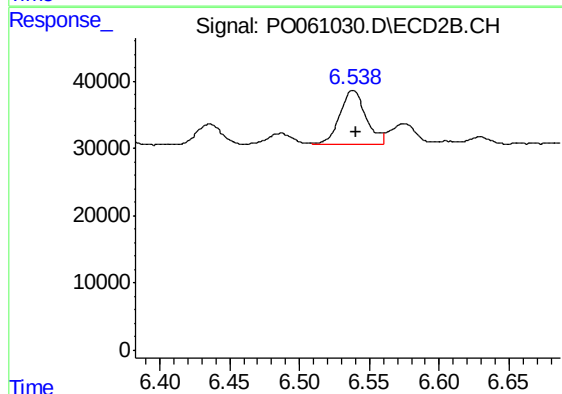


#30 AR-1254-5

R.T.: 6.538 min
Delta R.T.: -0.002 min
Response: 107068
Conc: 33.83 ng/ml




#31 AR-1260-1

R.T.: 7.128 min
Delta R.T.: 0.000 min
Response: 41394
Conc: 17.00 ng/ml

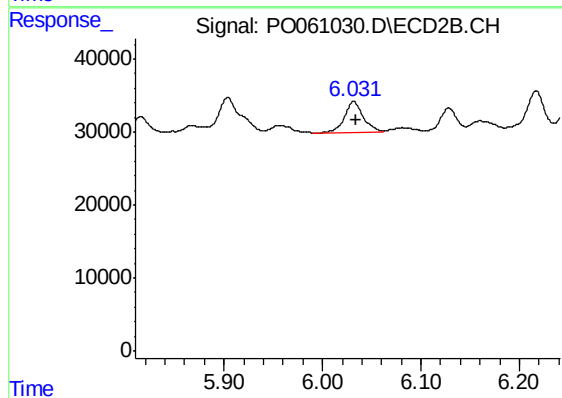

#31 AR-1260-1


R.T.: 6.032 min
Delta R.T.: -0.003 min
Response: 55641
Conc: 26.45 ng/ml



#32 AR-1260-2


R.T.: 7.381 min
Delta R.T.: -0.004 min
Response: 127844
Conc: 42.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP




#32 AR-1260-2

R.T.: 6.217 min
Delta R.T.: -0.002 min
Response: 50886
Conc: 19.73 ng/ml




#33 AR-1260-3

R.T.: 7.742 min
Delta R.T.: 0.000 min
Response: 35168
Conc: 14.74 ng/ml

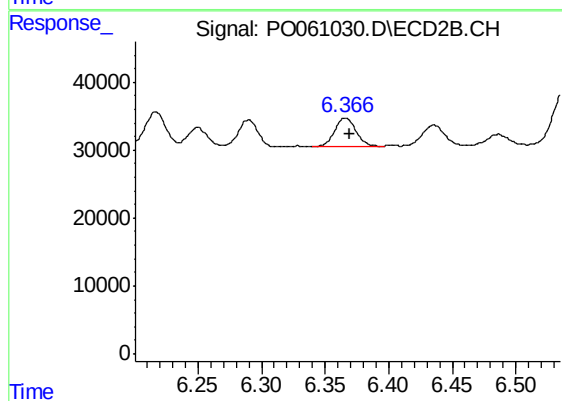

#33 AR-1260-3


R.T.: 6.366 min
Delta R.T.: -0.004 min
Response: 49412
Conc: 20.52 ng/ml

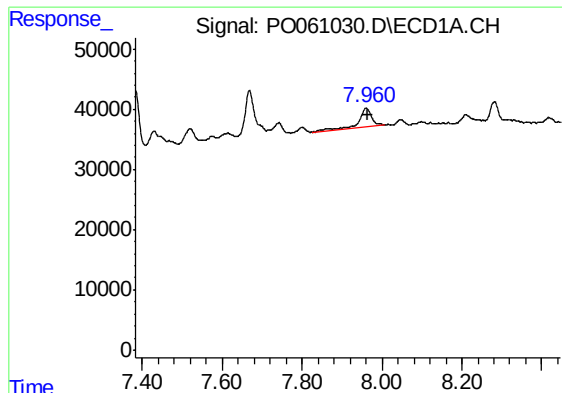

#34 AR-1260-4


R.T.: 7.961 min
Delta R.T.: -0.005 min
Response: 70558
Conc: 25.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

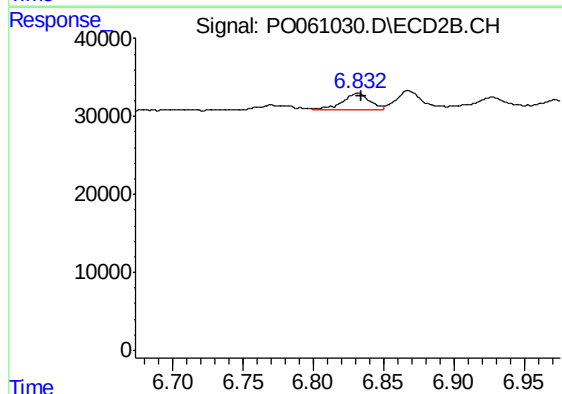


#34 AR-1260-4

R.T.: 6.832 min
Delta R.T.: -0.003 min
Response: 27745
Conc: 12.96 ng/ml




#35 AR-1260-5

R.T.: 8.281 min
Delta R.T.: 0.002 min
Response: 38287
Conc: 7.03 ng/ml

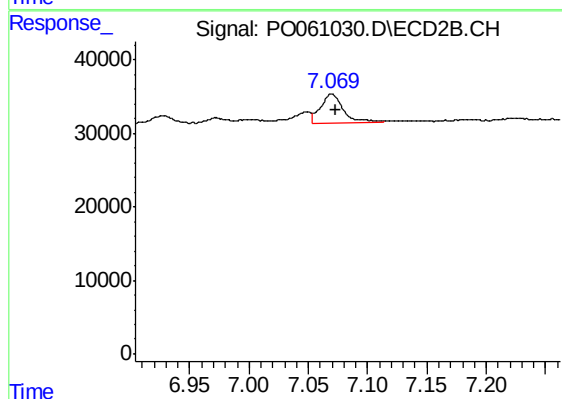

#35 AR-1260-5


R.T.: 7.070 min
Delta R.T.: -0.004 min
Response: 53145
Conc: 11.00 ng/ml



#36 AR-1262-1


R.T.: 7.742 min
Delta R.T.: -0.003 min
Response: 35168
Conc: 9.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP




#36 AR-1262-1

R.T.: 6.575 min
Delta R.T.: -0.006 min
Response: 41010
Conc: 13.73 ng/ml




#37 AR-1262-2

R.T.: 8.281 min
Delta R.T.: -0.003 min
Response: 38287
Conc: 6.14 ng/ml

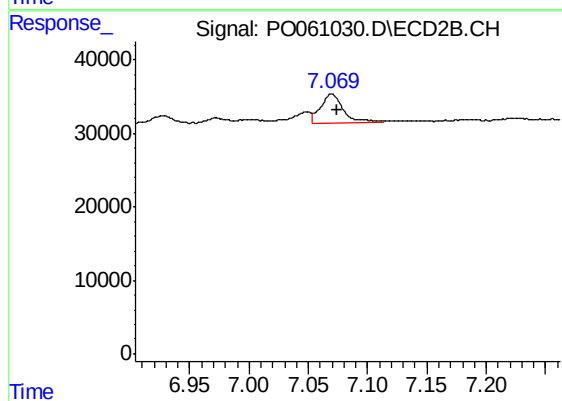

#37 AR-1262-2


R.T.: 7.070 min
Delta R.T.: -0.005 min
Response: 53145
Conc: 10.22 ng/ml

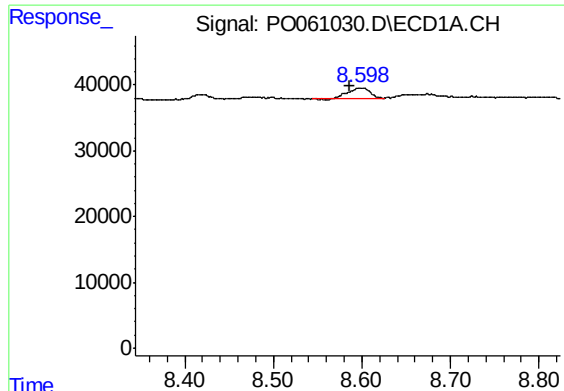

#38 AR-1262-3


R.T.: 8.599 min
Delta R.T.: 0.012 min
Response: 27895
Conc: 6.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

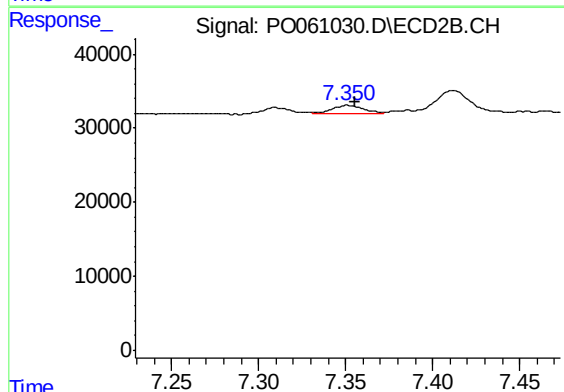


#38 AR-1262-3

R.T.: 7.351 min
Delta R.T.: -0.004 min
Response: 14465
Conc: 6.82 ng/ml

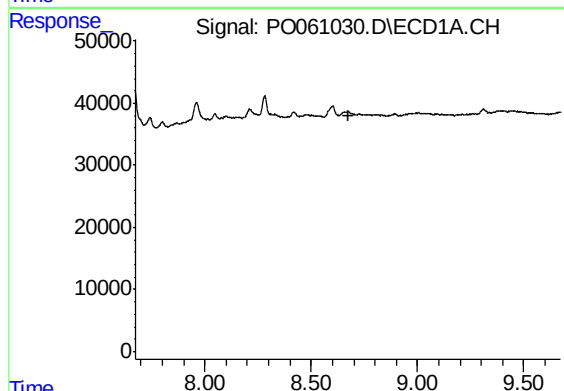


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.673 min
Response: 0
Conc: N.D.

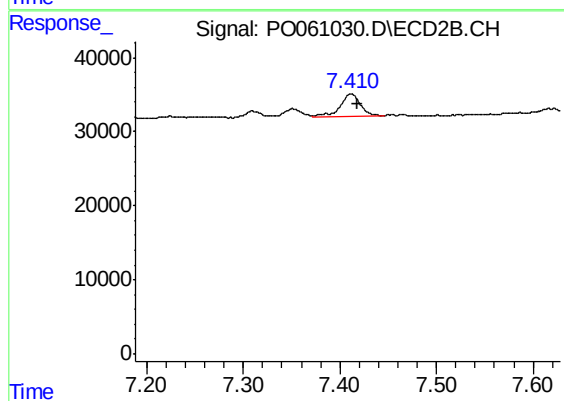

#39 AR-1262-4


R.T.: 7.411 min
Delta R.T.: -0.006 min
Response: 44783
Conc: 11.72 ng/ml



#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.311 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

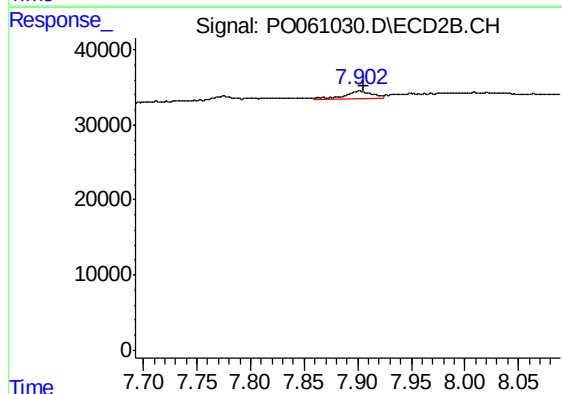


#40 AR-1262-5

R.T.: 7.902 min
Delta R.T.: -0.003 min
Response: 17729
Conc: 10.59 ng/ml




#41 AR-1268-1

R.T.: 8.599 min
Delta R.T.: 0.019 min
Response: 27895
Conc: 3.78 ng/ml

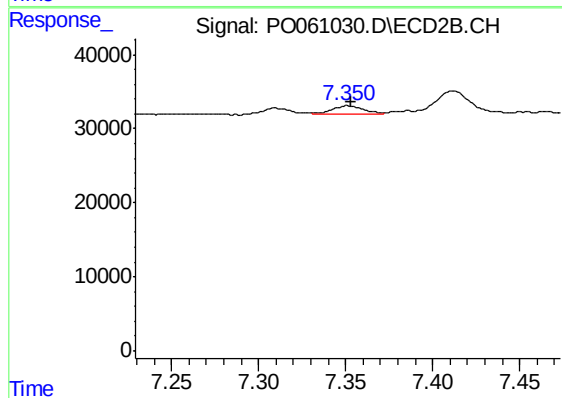

#41 AR-1268-1


R.T.: 7.351 min
Delta R.T.: -0.002 min
Response: 14465
Conc: 2.47 ng/ml



#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP




#42 AR-1268-2

R.T.: 7.411 min
Delta R.T.: -0.005 min
Response: 44783
Conc: 8.40 ng/ml




#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.893 min
Response: 0
Conc: N.D.

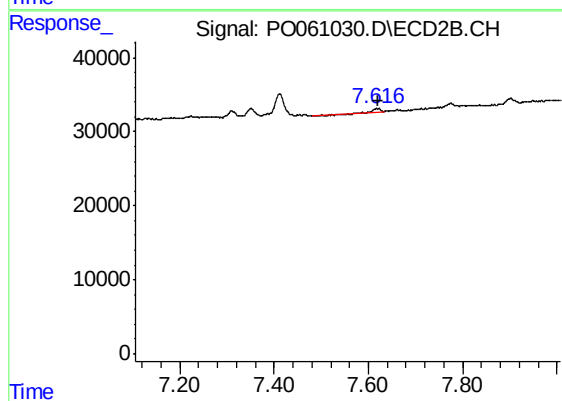

#43 AR-1268-3


R.T.: 7.617 min
Delta R.T.: -0.005 min
Response: 1920
Conc: 0.43 ng/ml



#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP




#44 AR-1268-4

R.T.: 7.902 min
Delta R.T.: -0.001 min
Response: 17729
Conc: 9.28 ng/ml



#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.704 min
Response: 0
Conc: N.D.

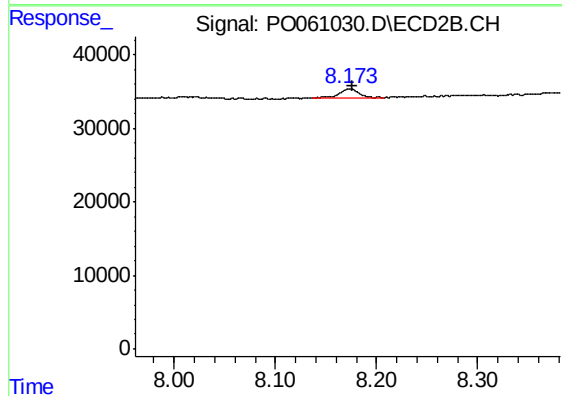

#45 AR-1268-5

R.T.: 8.174 min
Delta R.T.: -0.003 min
Response: 18452
Conc: 1.53 ng/ml