

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
 Data File : P0060989.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 10:59
 Operator : SM/AJ
 Sample : K4886-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-13-S(1.5-4)

Manual Integrations
 APPROVED

Ankita
 9/19/2019 9:01:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 15:37:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.534	977805	837826	26.577	30.006
2) SA Decachlor...	10.034	8.412	621556	429514	13.528	12.254

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
Data File : P0060989.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2019 10:59
Operator : SM/AJ
Sample : K4886-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-13-S(1.5-4)


Manual Integrations
APPROVED

Ankita
9/19/2019 9:01:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 15:37:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

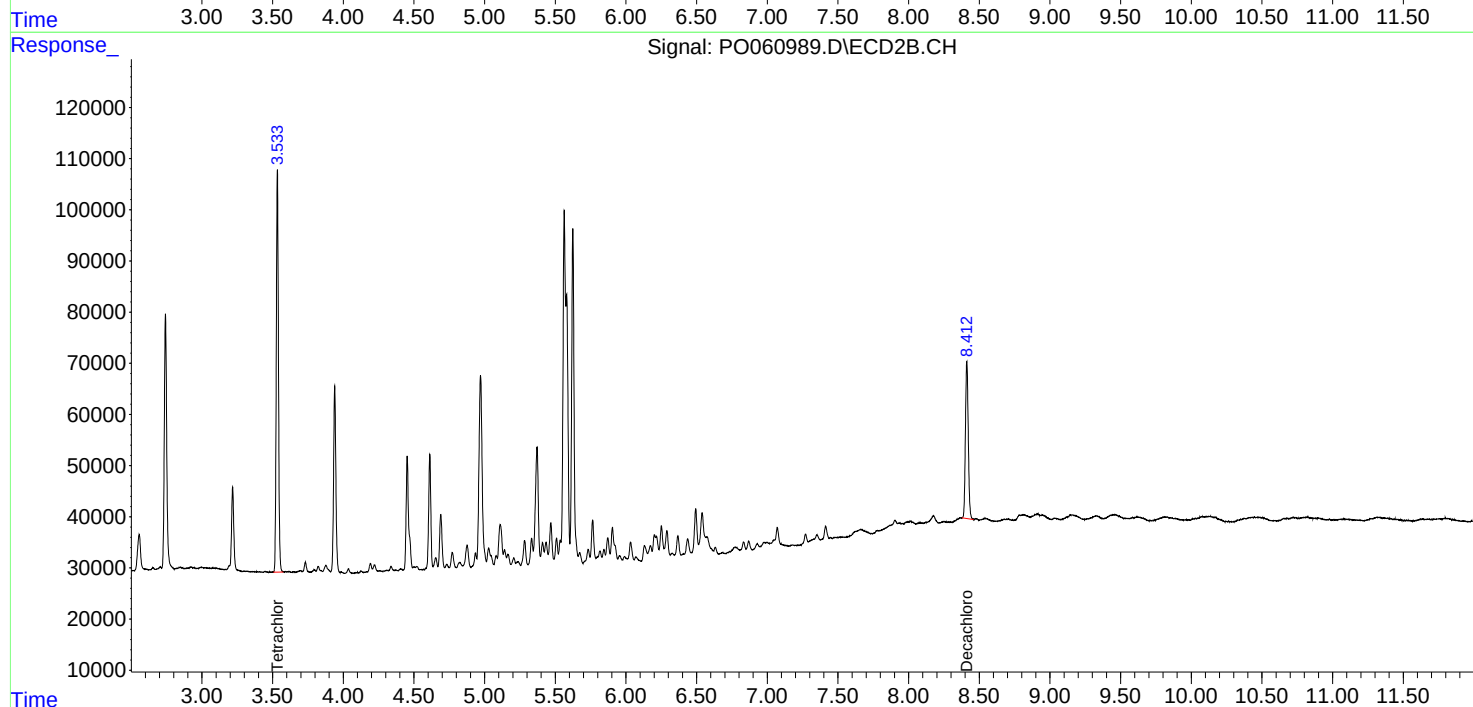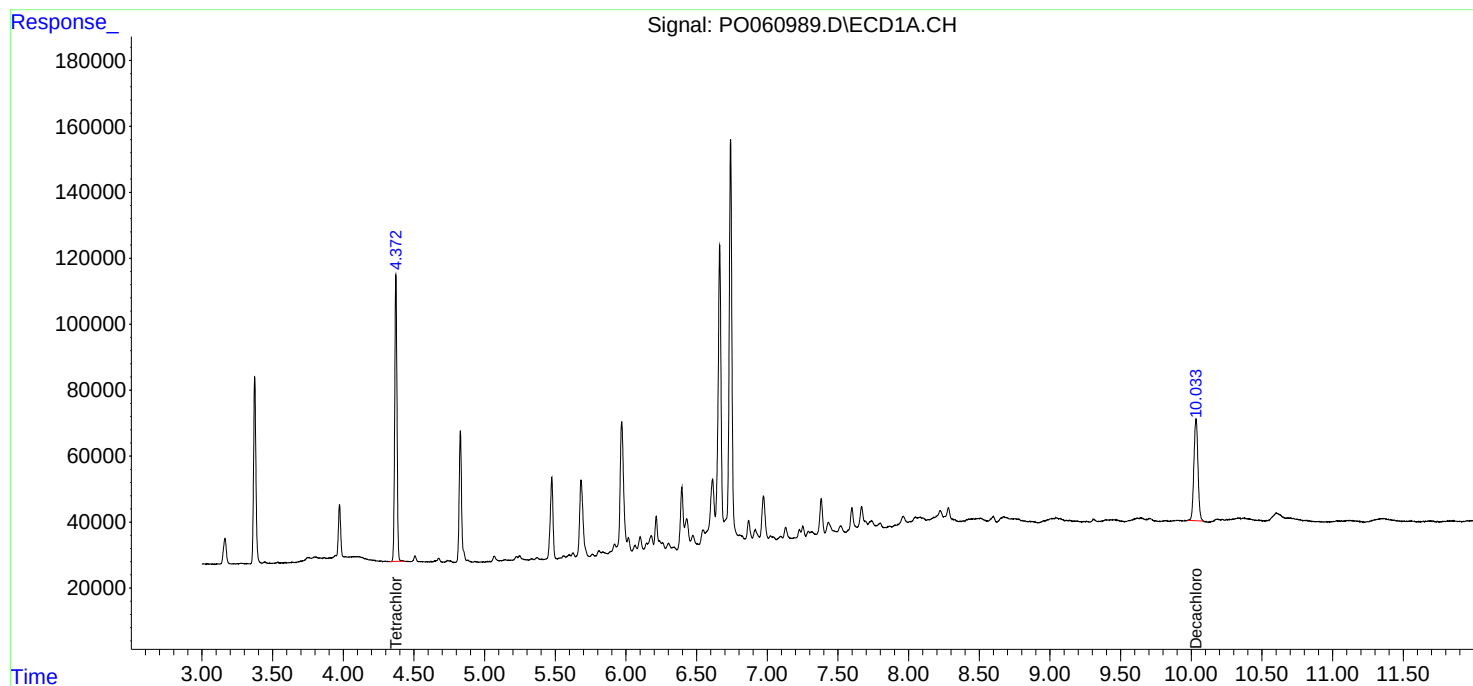

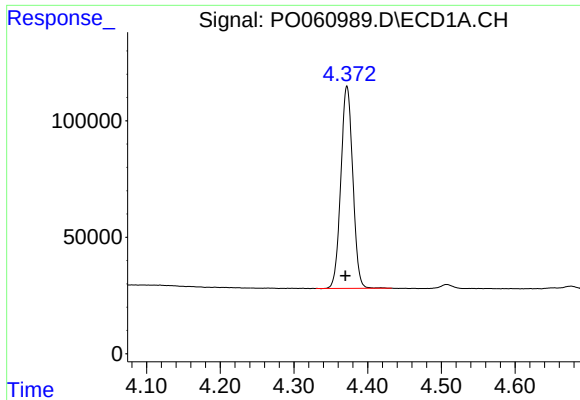


#1 Tetrachloro-m-xylene

R.T.: 4.372 min
Delta R.T.: 0.002 min
Response: 977805
Conc: 26.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-13-S(1.5-4)


Manual Integrations
APPROVED

Ankita
9/19/2019 9:01:56 AM

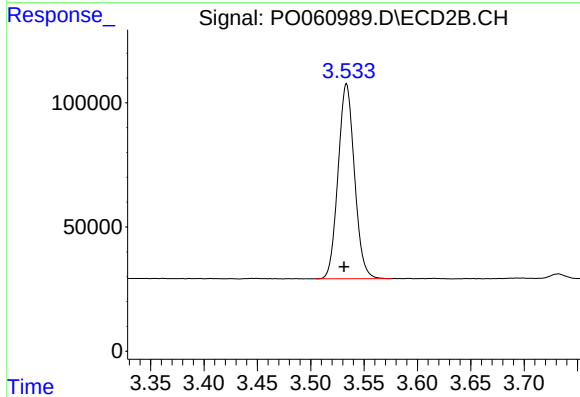


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: 0.002 min
Response: 837826
Conc: 30.01 ng/ml

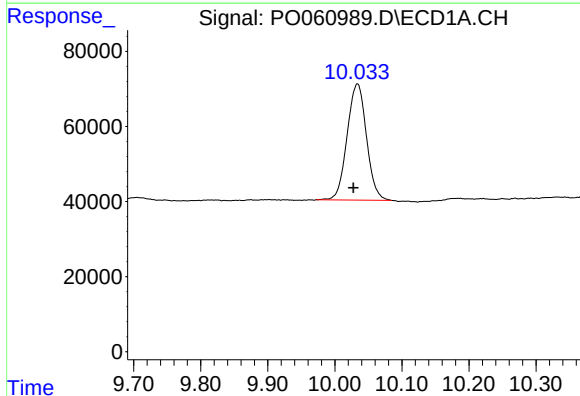

#2 Decachlorobiphenyl

R.T.: 10.034 min
Delta R.T.: 0.006 min
Response: 621556
Conc: 13.53 ng/ml

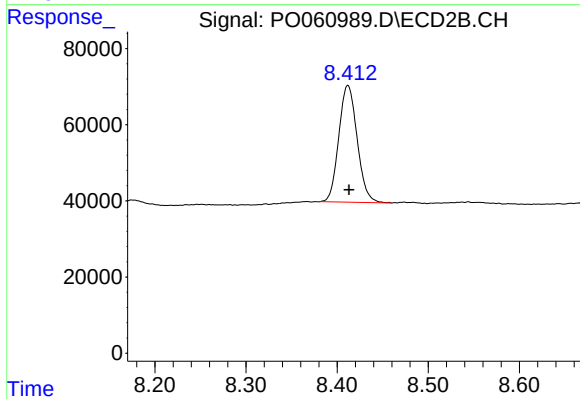

#2 Decachlorobiphenyl

R.T.: 8.412 min
Delta R.T.: -0.001 min
Response: 429514
Conc: 12.25 ng/ml