

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
 Data File : P0061017.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 20:02
 Operator : SM/AJ
 Sample : K4847-12
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-35-COMP

Manual Integrations
 APPROVED

Ankita
 9/19/2019 9:02:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:15:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.368	3.529	620477	495031	16.865	17.729
2) SA Decachlor...	10.028	8.407	887974	686609	19.326	19.588m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
Data File : P0061017.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2019 20:02
Operator : SM/AJ
Sample : K4847-12
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-35-COMP


Manual Integrations
APPROVED

Ankita
9/19/2019 9:02:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:15:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

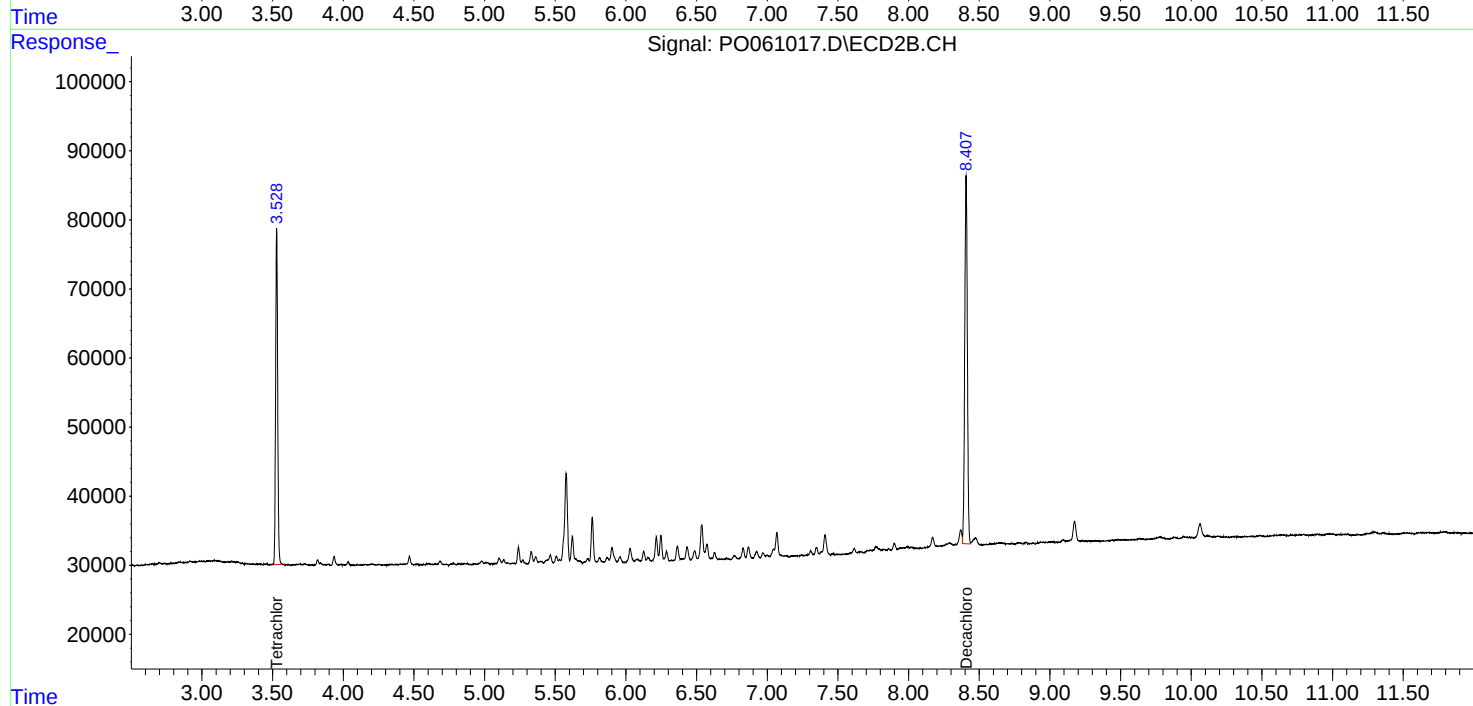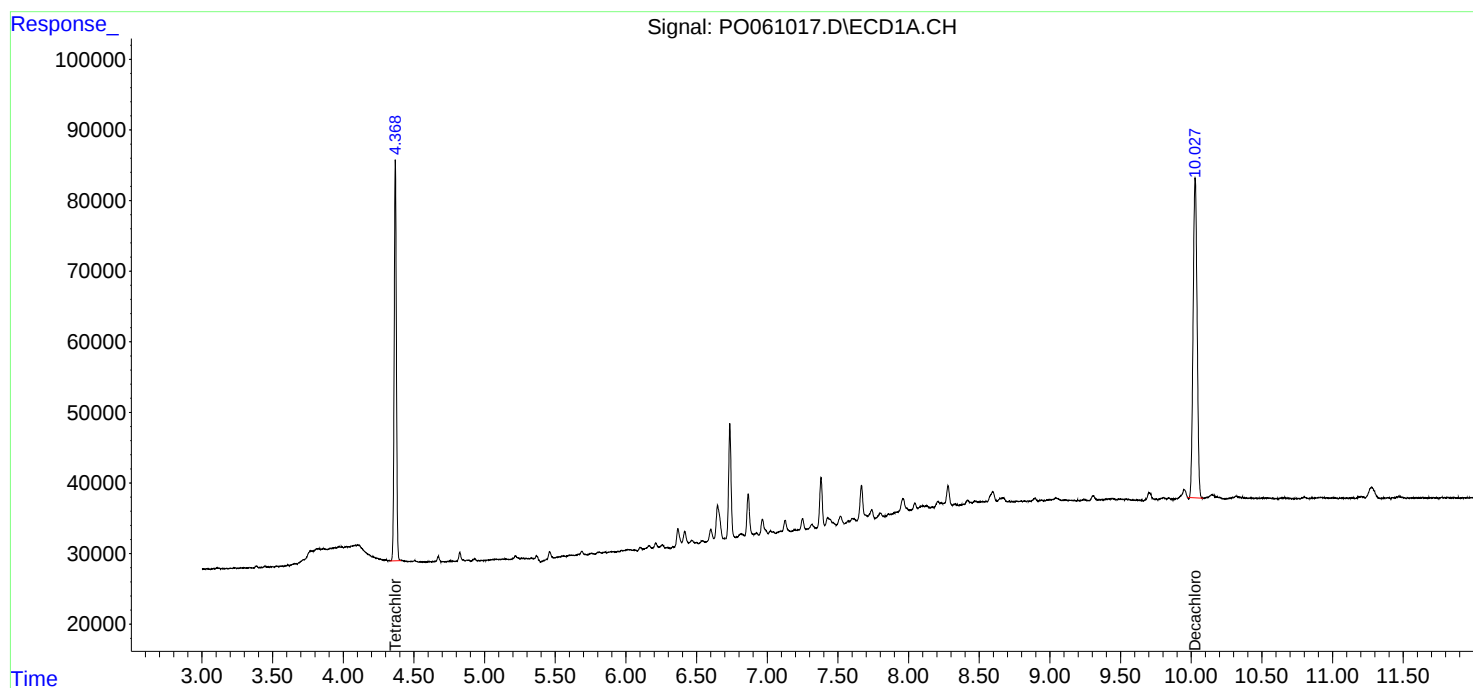

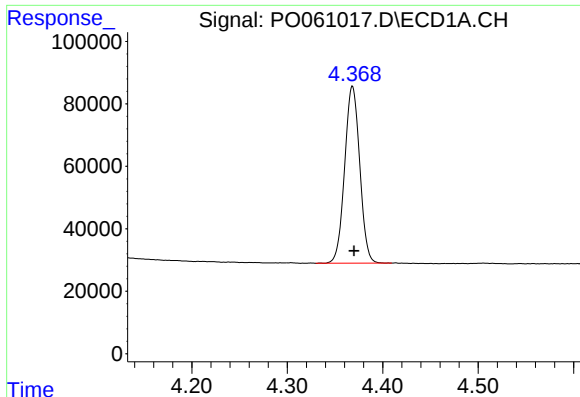


#1 Tetrachloro-m-xylene

R.T.: 4.368 min
Delta R.T.: -0.002 min
Response: 620477
Conc: 16.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-35-COMP


Manual Integrations
APPROVED

Ankita
9/19/2019 9:02:26 AM

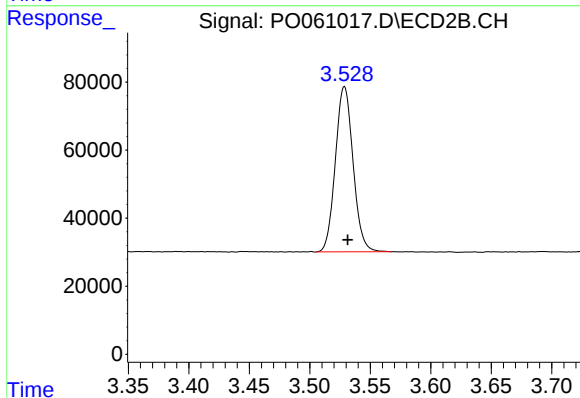


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.003 min
Response: 495031
Conc: 17.73 ng/ml

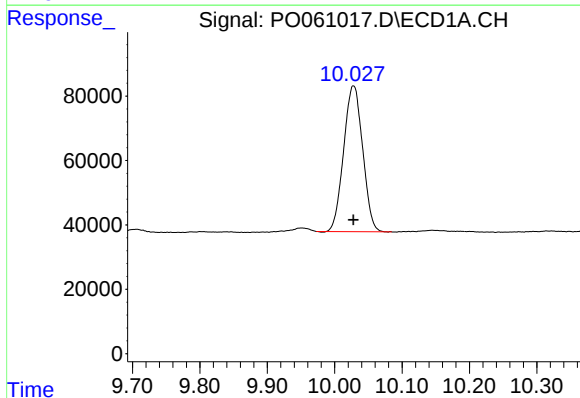

#2 Decachlorobiphenyl

R.T.: 10.028 min
Delta R.T.: 0.000 min
Response: 887974
Conc: 19.33 ng/ml

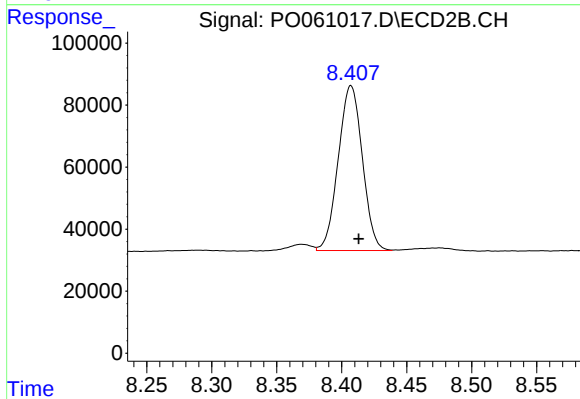

#2 Decachlorobiphenyl

R.T.: 8.407 min
Delta R.T.: -0.006 min
Response: 686609
Conc: 19.59 ng/ml m