

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
 Data File : P0061021.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 21:10
 Operator : SM/AJ
 Sample : K4861-11
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1-S(1.5-4)

Manual Integrations
 APPROVED

Ankita
 9/19/2019 9:02:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:17:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.369	3.530	640338	515148	17.405	18.449
2) SA Decachlor...	10.029	8.409	750064	574146	16.325	16.380

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
Data File : P0061021.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2019 21:10
Operator : SM/AJ
Sample : K4861-11
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-1-S(1.5-4)


Manual Integrations
APPROVED

Ankita
9/19/2019 9:02:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:17:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

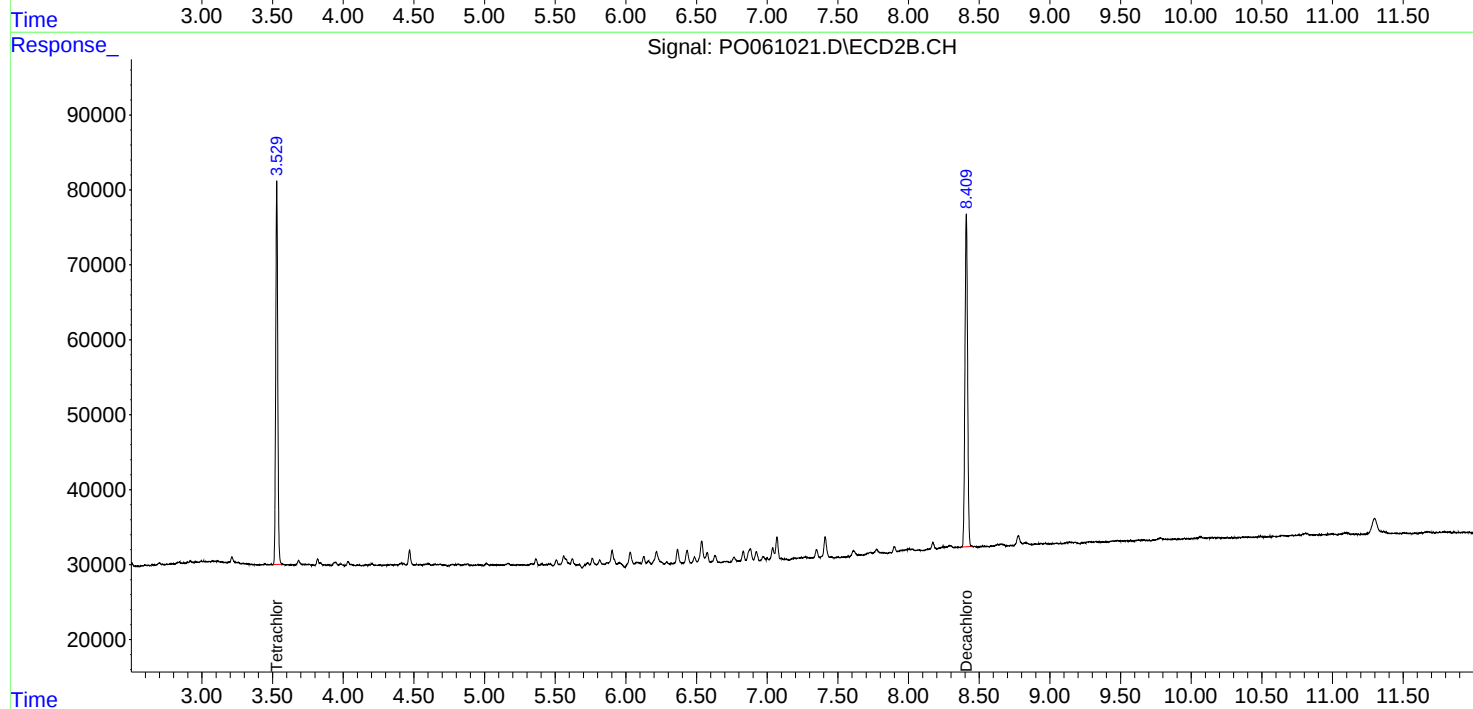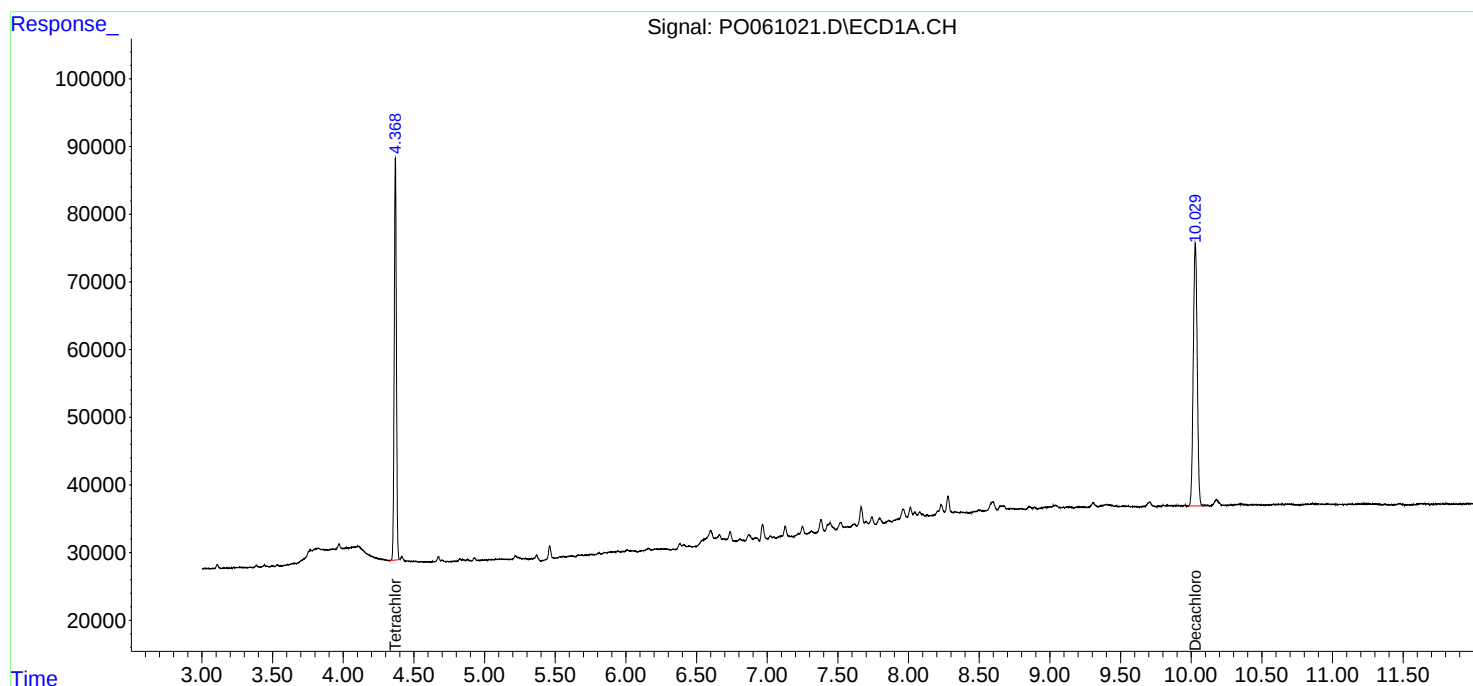

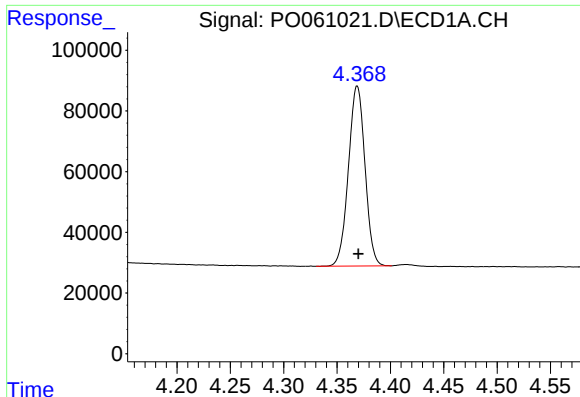


#1 Tetrachloro-m-xylene

R.T.: 4.369 min
Delta R.T.: -0.001 min
Response: 640338
Conc: 17.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-S(1.5-4)


Manual Integrations
APPROVED

Ankita
9/19/2019 9:02:30 AM

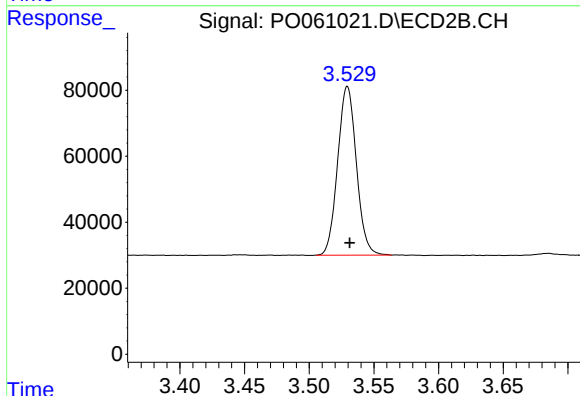


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.002 min
Response: 515148
Conc: 18.45 ng/ml

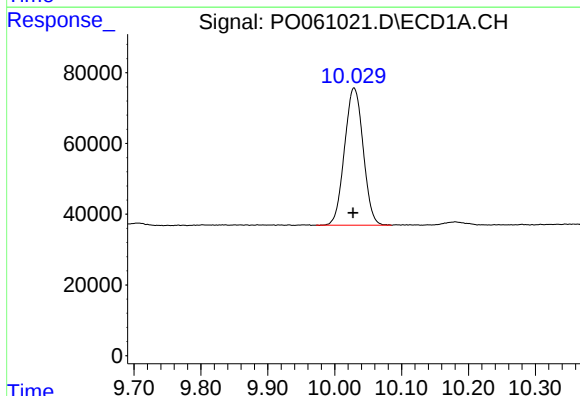

#2 Decachlorobiphenyl

R.T.: 10.029 min
Delta R.T.: 0.001 min
Response: 750064
Conc: 16.32 ng/ml

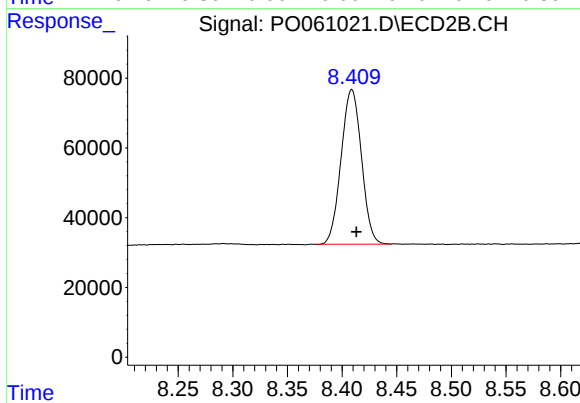

#2 Decachlorobiphenyl

R.T.: 8.409 min
Delta R.T.: -0.004 min
Response: 574146
Conc: 16.38 ng/ml