

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
 Data File : P0061030.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 23:53
 Operator : SM/AJ
 Sample : K4923-04
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-40-COMP

Manual Integrations
 APPROVED

Ankita
 9/19/2019 9:02:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:22:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.532	1141181	883146	31.018	31.629
2) SA Decachlor...	10.033	8.410	786506	571668	17.118	16.309
Target Compounds						
26) L6 AR-1254-1	6.381	5.365	43816	34743	22.742m	16.858 #
27) L6 AR-1254-2	6.601	5.509	84689	33925	26.912	17.978 #
28) L6 AR-1254-3	6.967	5.904	70696	84298	20.073	26.513 #
29) L6 AR-1254-4	7.251	6.128	39318	31461	14.524	15.111
30) L6 AR-1254-5	7.668	6.538	135687	107068	46.014	33.830 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
Data File : P0061030.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2019 23:53
Operator : SM/AJ
Sample : K4923-04
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-40-COMP


Manual Integrations
APPROVED

Ankita
9/19/2019 9:02:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:22:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

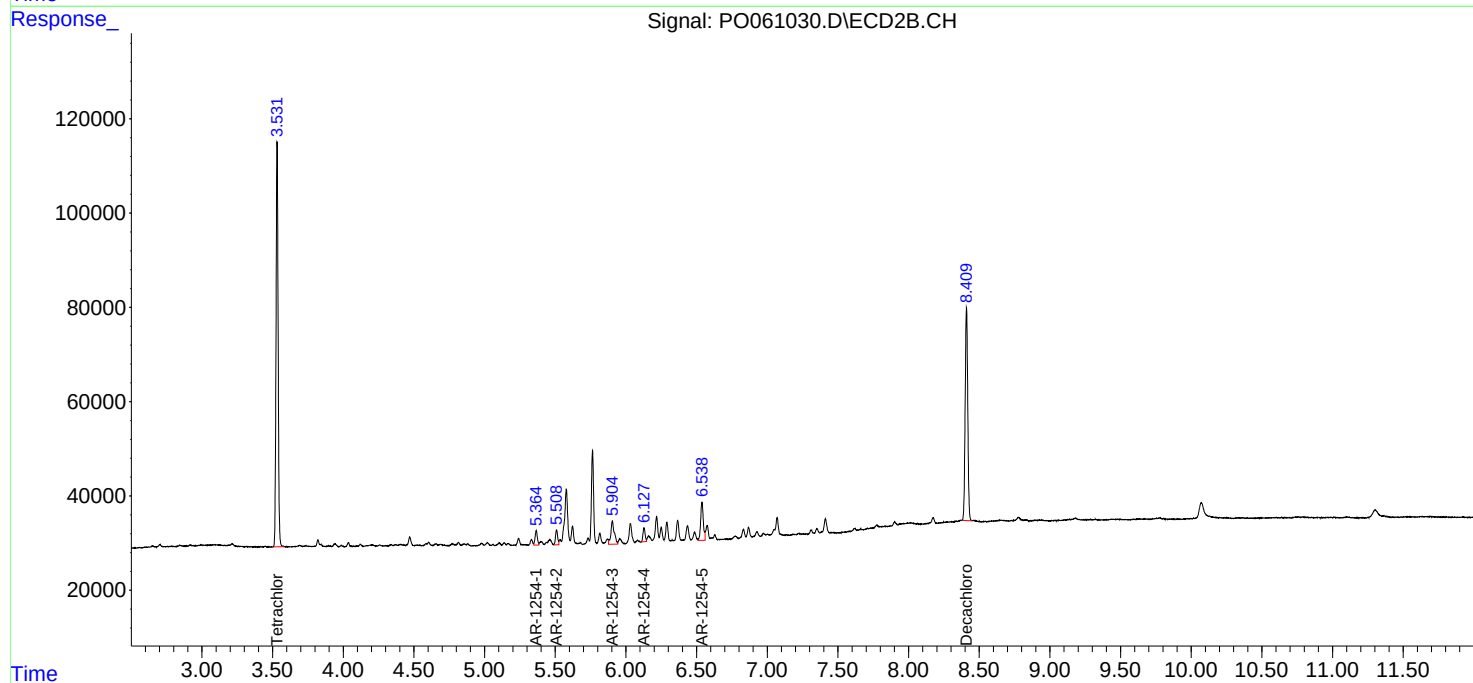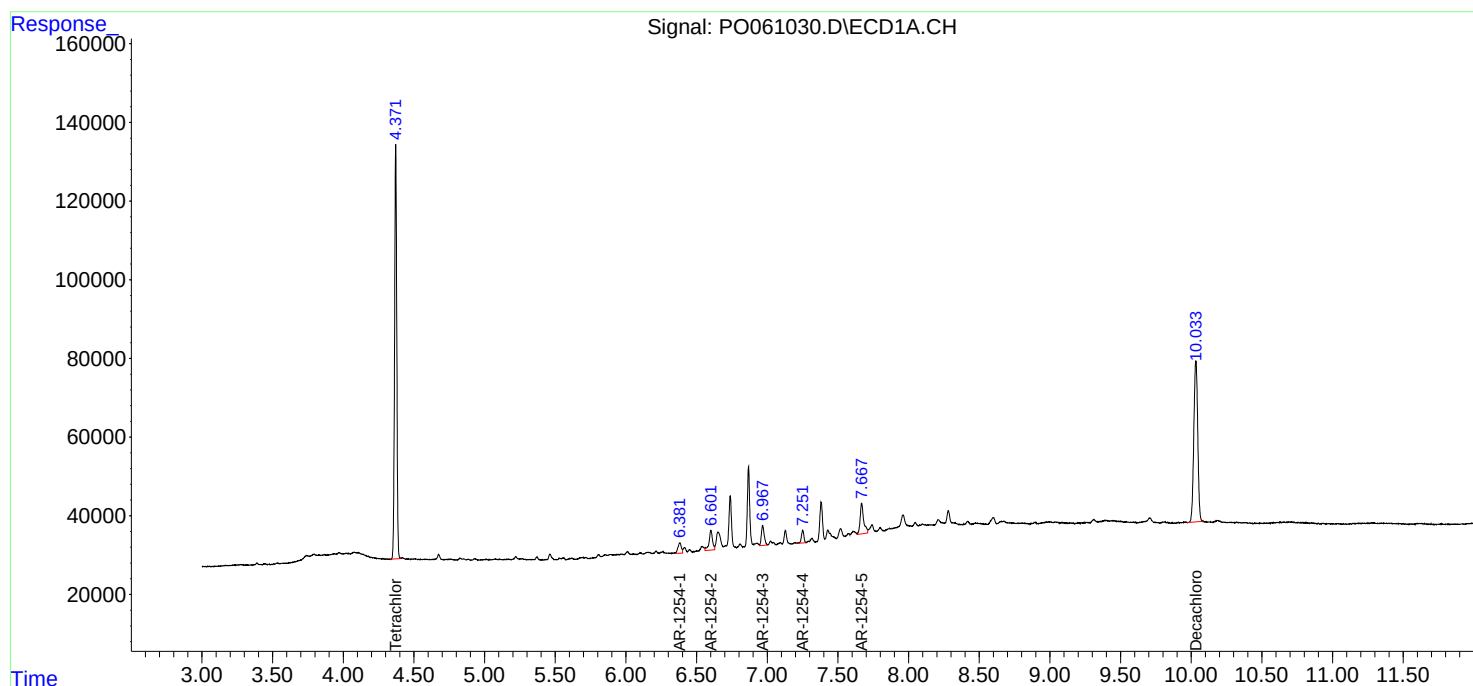

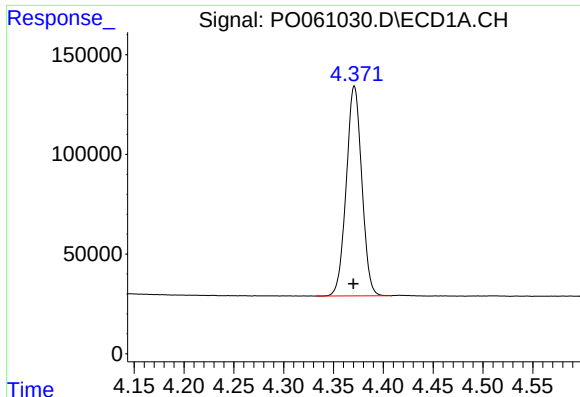


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 1141181
Conc: 31.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP


Manual Integrations
APPROVED

Ankita
9/19/2019 9:02:47 AM

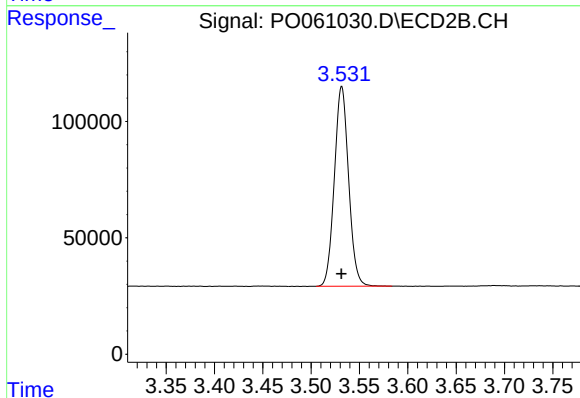


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 883146
Conc: 31.63 ng/ml

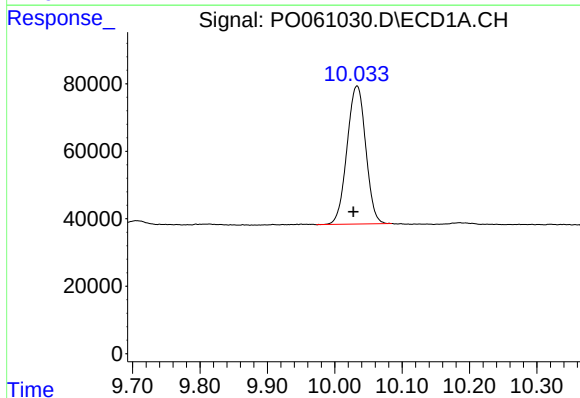


#2 Decachlorobiphenyl

R.T.: 10.033 min
Delta R.T.: 0.005 min
Response: 786506
Conc: 17.12 ng/ml

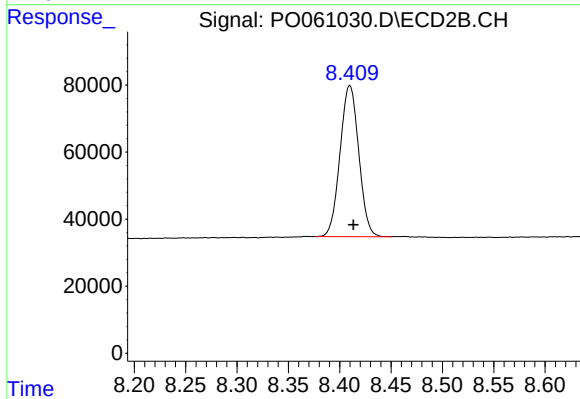

#2 Decachlorobiphenyl

R.T.: 8.410 min
Delta R.T.: -0.003 min
Response: 571668
Conc: 16.31 ng/ml

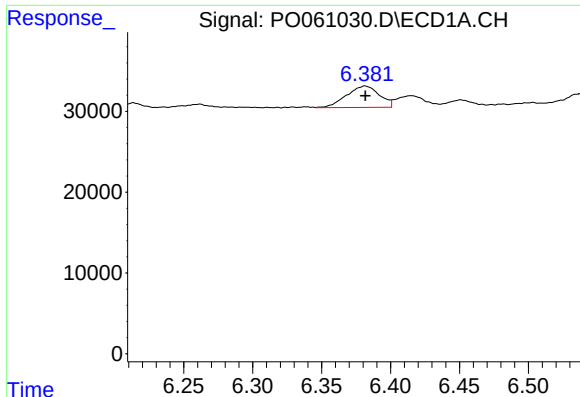


#26 AR-1254-1

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 43816
Conc: 22.74 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP


Manual Integrations
APPROVED

Ankita
9/19/2019 9:02:47 AM

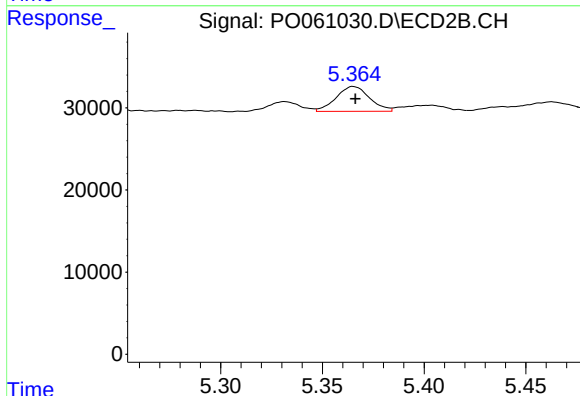


#26 AR-1254-1

R.T.: 5.365 min
Delta R.T.: -0.001 min
Response: 34743
Conc: 16.86 ng/ml

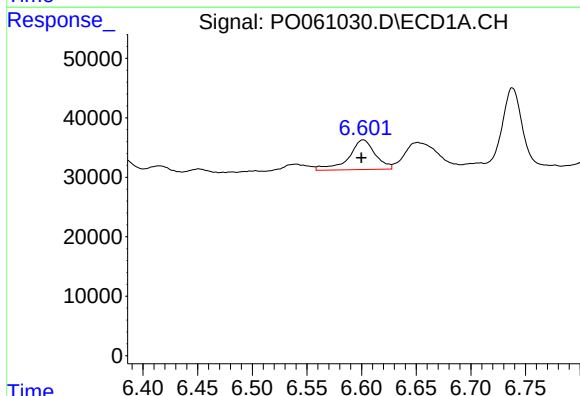


#27 AR-1254-2

R.T.: 6.601 min
Delta R.T.: 0.002 min
Response: 84689
Conc: 26.91 ng/ml

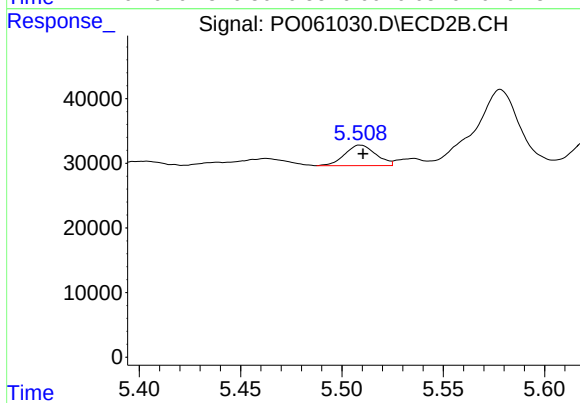

#27 AR-1254-2

R.T.: 5.509 min
Delta R.T.: -0.002 min
Response: 33925
Conc: 17.98 ng/ml

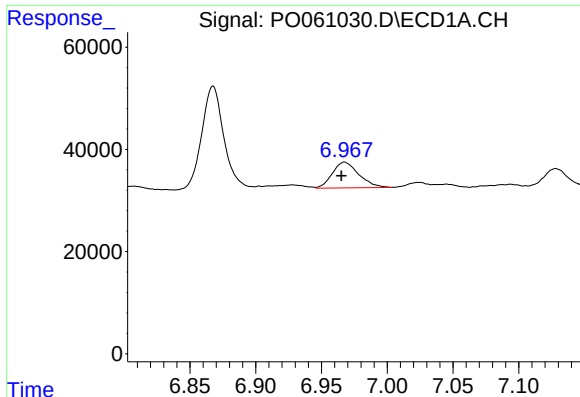


#28 AR-1254-3

R.T.: 6.967 min
Delta R.T.: 0.002 min
Response: 70696
Conc: 20.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP


Manual Integrations
APPROVED

Ankita
9/19/2019 9:02:47 AM

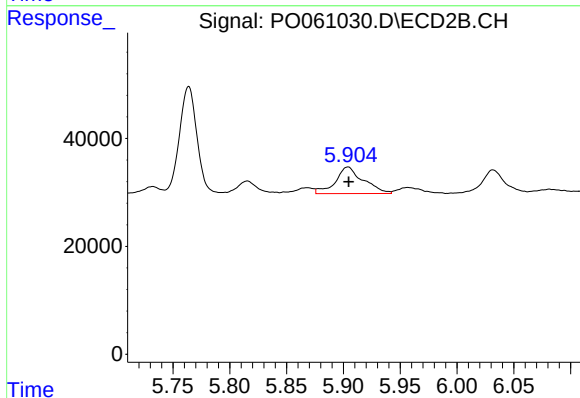


#28 AR-1254-3

R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 84298
Conc: 26.51 ng/ml

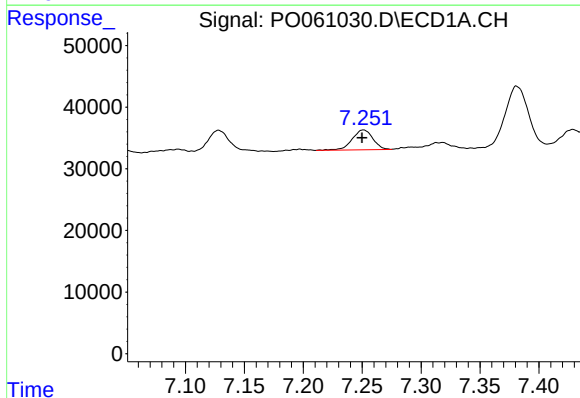


#29 AR-1254-4

R.T.: 7.251 min
Delta R.T.: 0.001 min
Response: 39318
Conc: 14.52 ng/ml

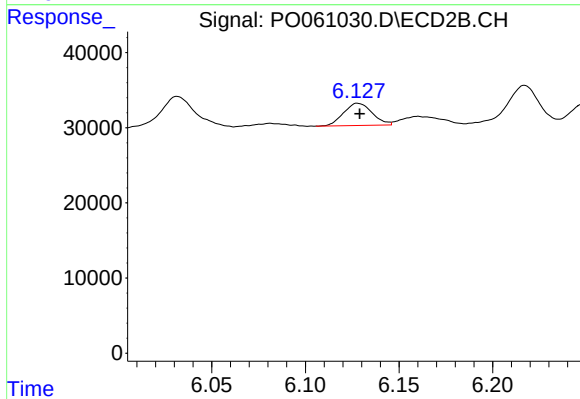

#29 AR-1254-4

R.T.: 6.128 min
Delta R.T.: -0.001 min
Response: 31461
Conc: 15.11 ng/ml

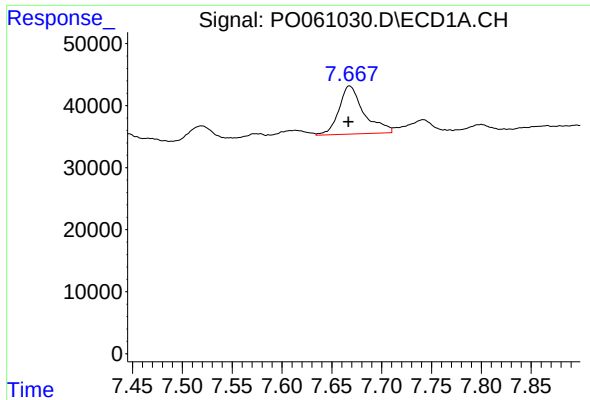


#30 AR-1254-5

R.T.: 7.668 min
Delta R.T.: 0.001 min
Response: 135687
Conc: 46.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

Manual Integrations
APPROVED

Ankita
9/19/2019 9:02:47 AM

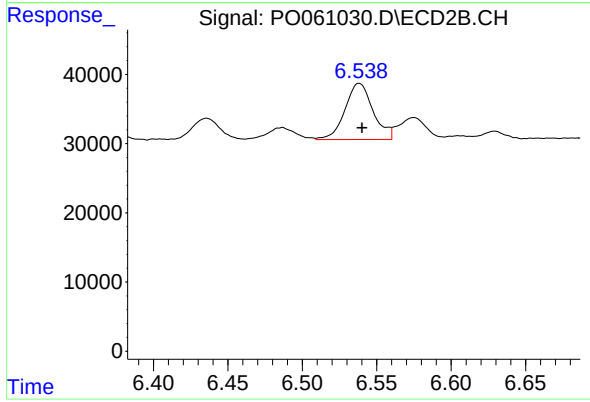

#30 AR-1254-5

R.T.: 6.538 min
Delta R.T.: -0.002 min
Response: 107068
Conc: 33.83 ng/ml