

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
 Data File : P0061053.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Sep 2019 7:23
 Operator : SM/AJ
 Sample : K4920-08 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EXJC-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 08:07:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.529	172107	144241	4.678	5.166
2) SA Decachlor...	10.026	8.404	251919	130469	5.483	3.722 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091719\
Data File : P0061053.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2019 7:23
Operator : SM/AJ
Sample : K4920-08 5X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EXJC-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 08:07:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

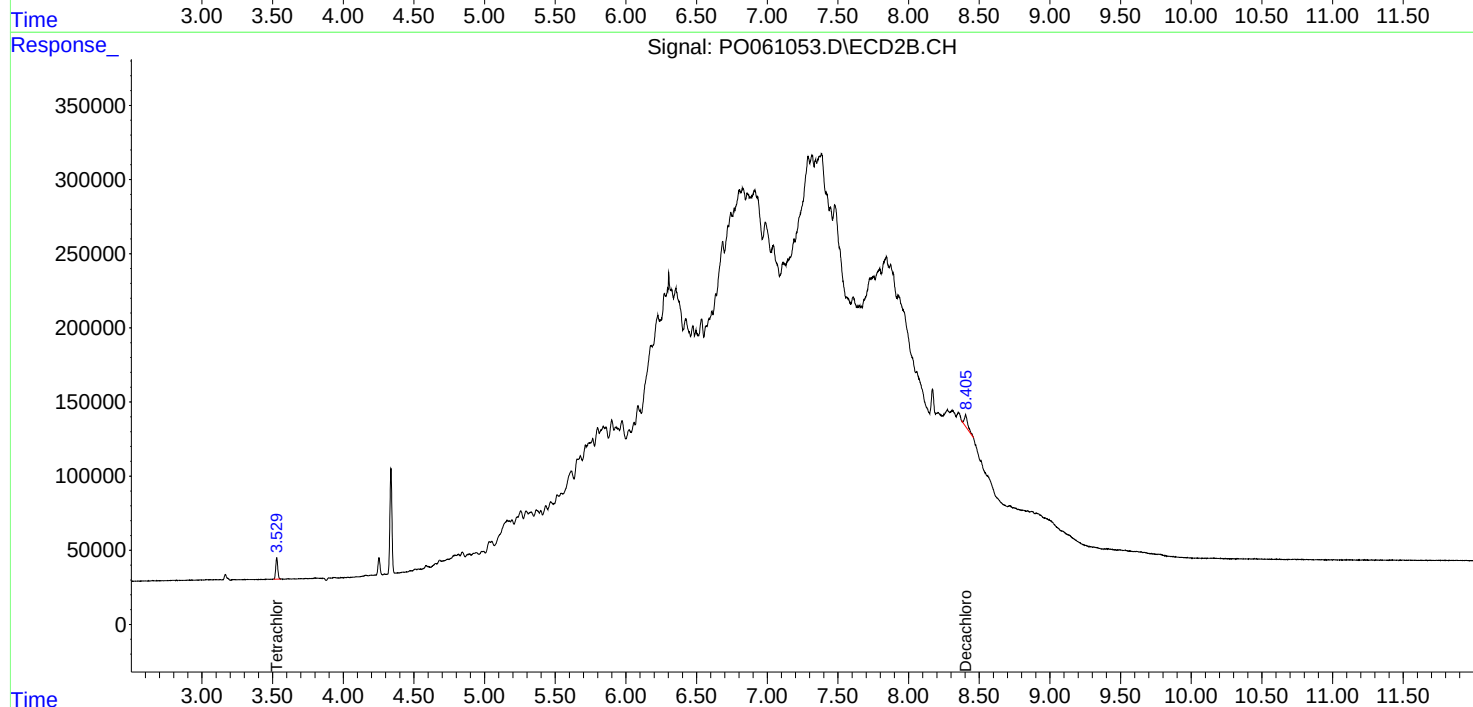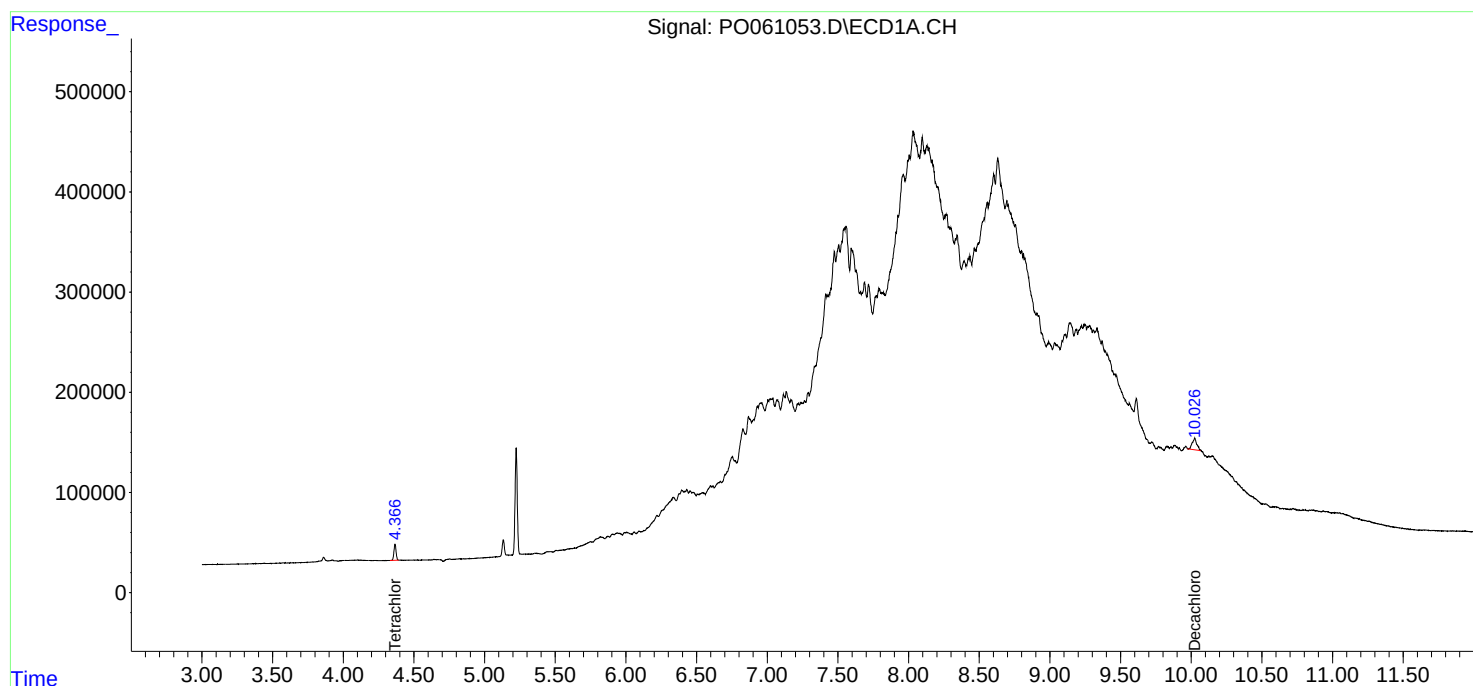


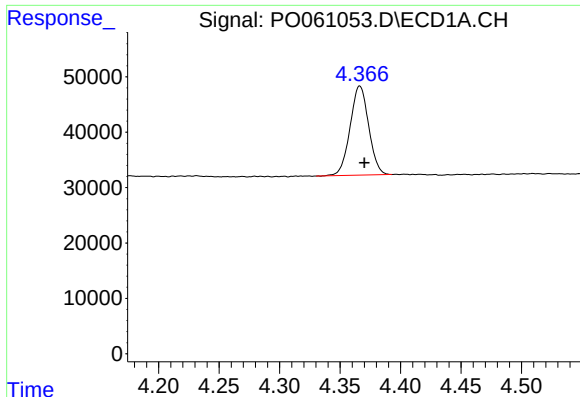

#1 Tetrachloro-m-xylene


R.T.: 4.366 min
Delta R.T.: -0.004 min
Response: 172107
Conc: 4.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
EXJC-1

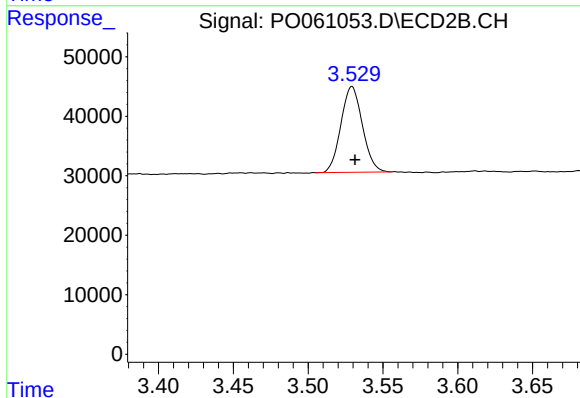


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.002 min
Response: 144241
Conc: 5.17 ng/ml

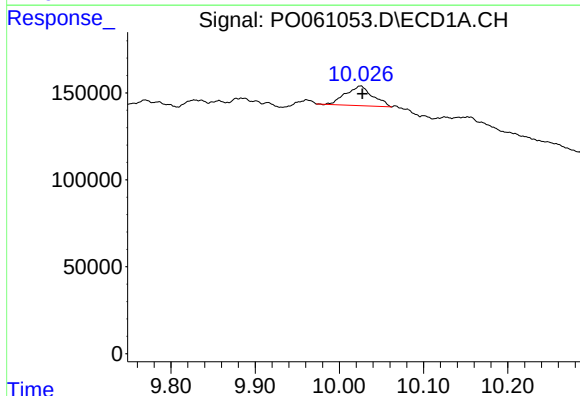

#2 Decachlorobiphenyl

R.T.: 10.026 min
Delta R.T.: -0.002 min
Response: 251919
Conc: 5.48 ng/ml

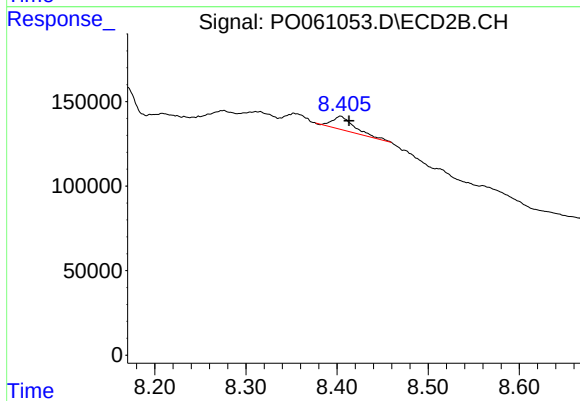

#2 Decachlorobiphenyl

R.T.: 8.404 min
Delta R.T.: -0.009 min
Response: 130469
Conc: 3.72 ng/ml