

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091721\
 Data File : P0081355.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2021 12:30
 Operator : AJ\MA
 Sample : M3774-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SW-CB-02-(0.2)

Manual Integrations
 APPROVED

mohammad
 9/21/2021 3:00:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 13:41:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	4.050	1444482	546783	18.298	22.126
2) SA Decachlor...	10.983	9.406	1249816	564884	21.049	24.198m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091721\
Data File : P0081355.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2021 12:30
Operator : AJ\MA
Sample : M3774-05
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SW-CB-02-(0.2)


Manual Integrations
APPROVED

mohammad
9/21/2021 3:00:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 13:41:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

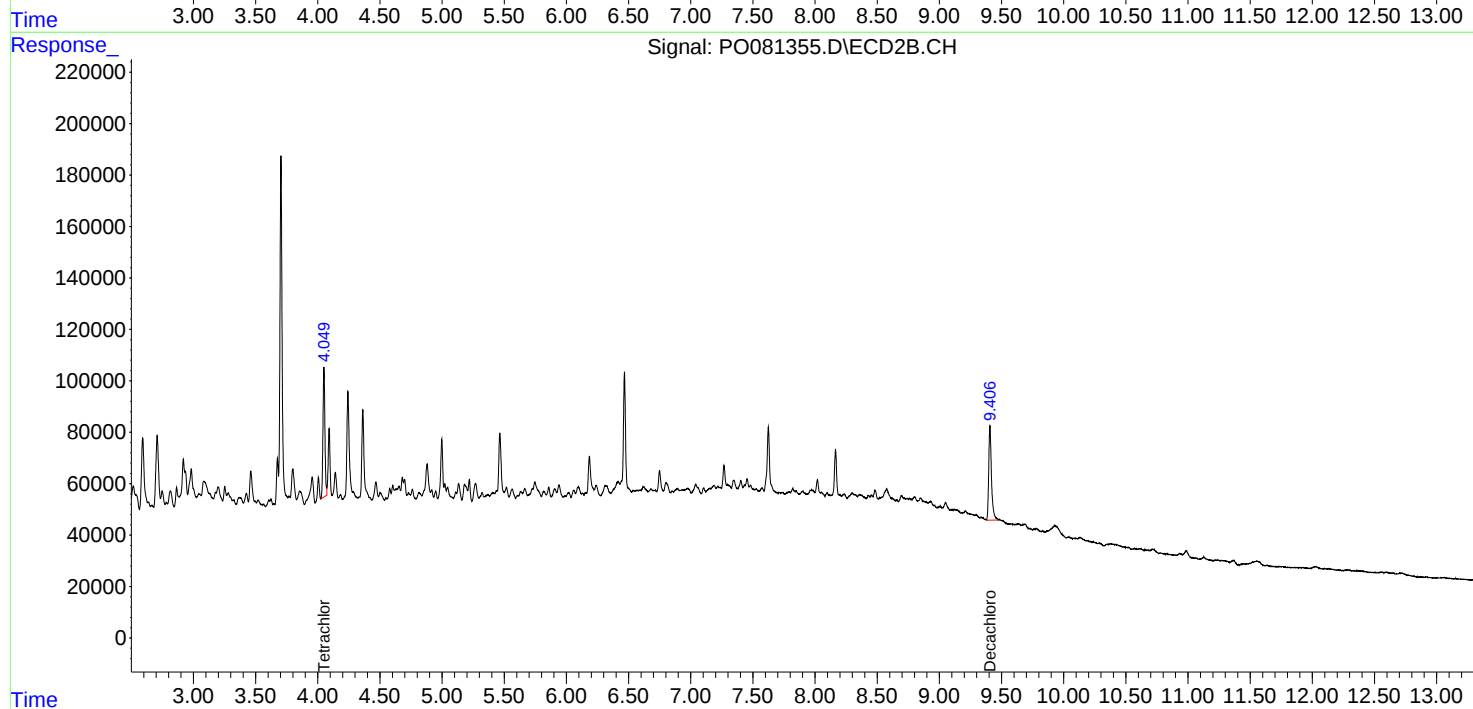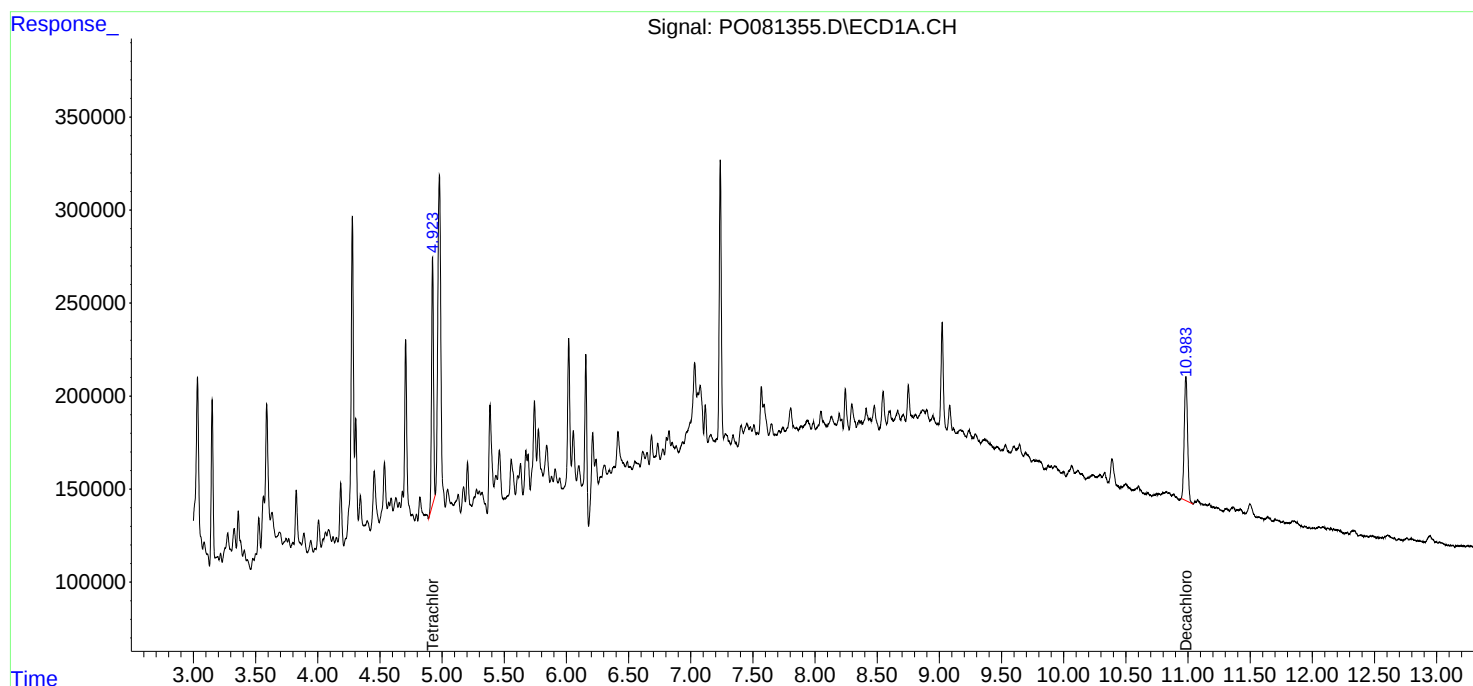

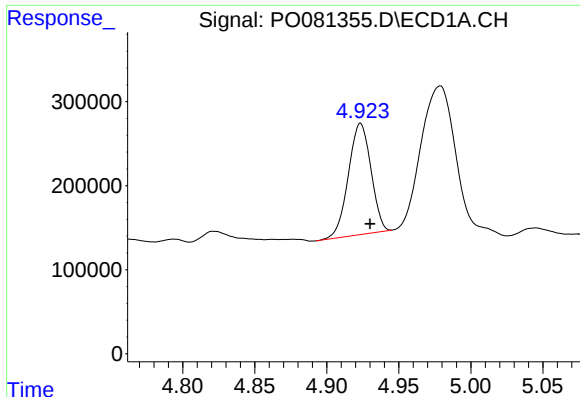


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: -0.007 min
Response: 1444482
Conc: 18.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
SW-CB-02-(0.2)


Manual Integrations
APPROVED

mohammad
9/21/2021 3:00:52 PM

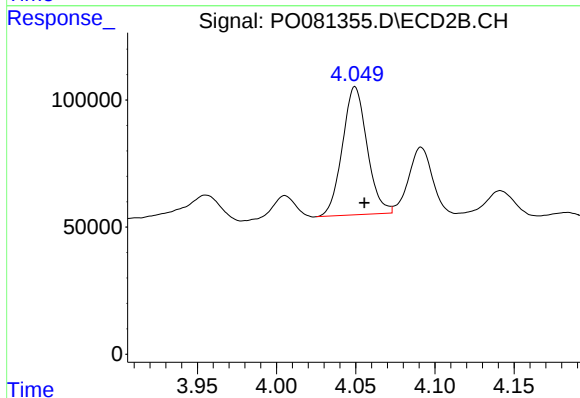


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.006 min
Response: 546783
Conc: 22.13 ng/ml

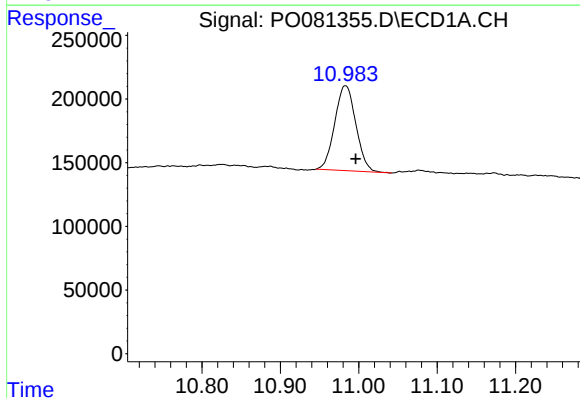

#2 Decachlorobiphenyl

R.T.: 10.983 min
Delta R.T.: -0.013 min
Response: 1249816
Conc: 21.05 ng/ml

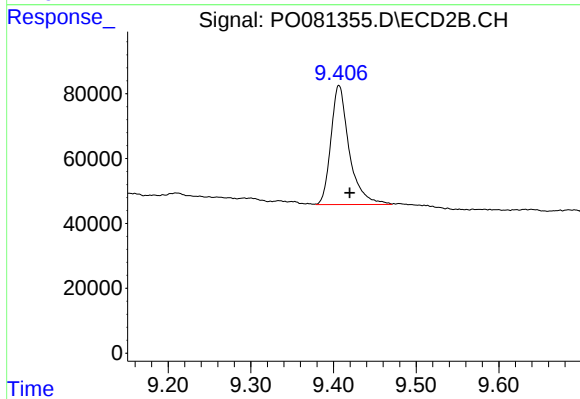

#2 Decachlorobiphenyl

R.T.: 9.406 min
Delta R.T.: -0.014 min
Response: 564884
Conc: 24.20 ng/ml m