

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091721\
 Data File : P0081357.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2021 13:04
 Operator : AJ\MA
 Sample : M3774-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SW-CB-03-(1.0)

Manual Integrations
 APPROVED

mohammad
 9/21/2021 3:00:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 13:41:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	4.050	1366869	533027	17.315	21.570
2) SA Decachlor...	10.982	9.426	1150840	4647595	19.382	199.090m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091721\
Data File : PO081357.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2021 13:04
Operator : AJ\MA
Sample : M3774-09
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SW-CB-03-(1.0)


Manual Integrations
APPROVED

mohammad
9/21/2021 3:00:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 13:41:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

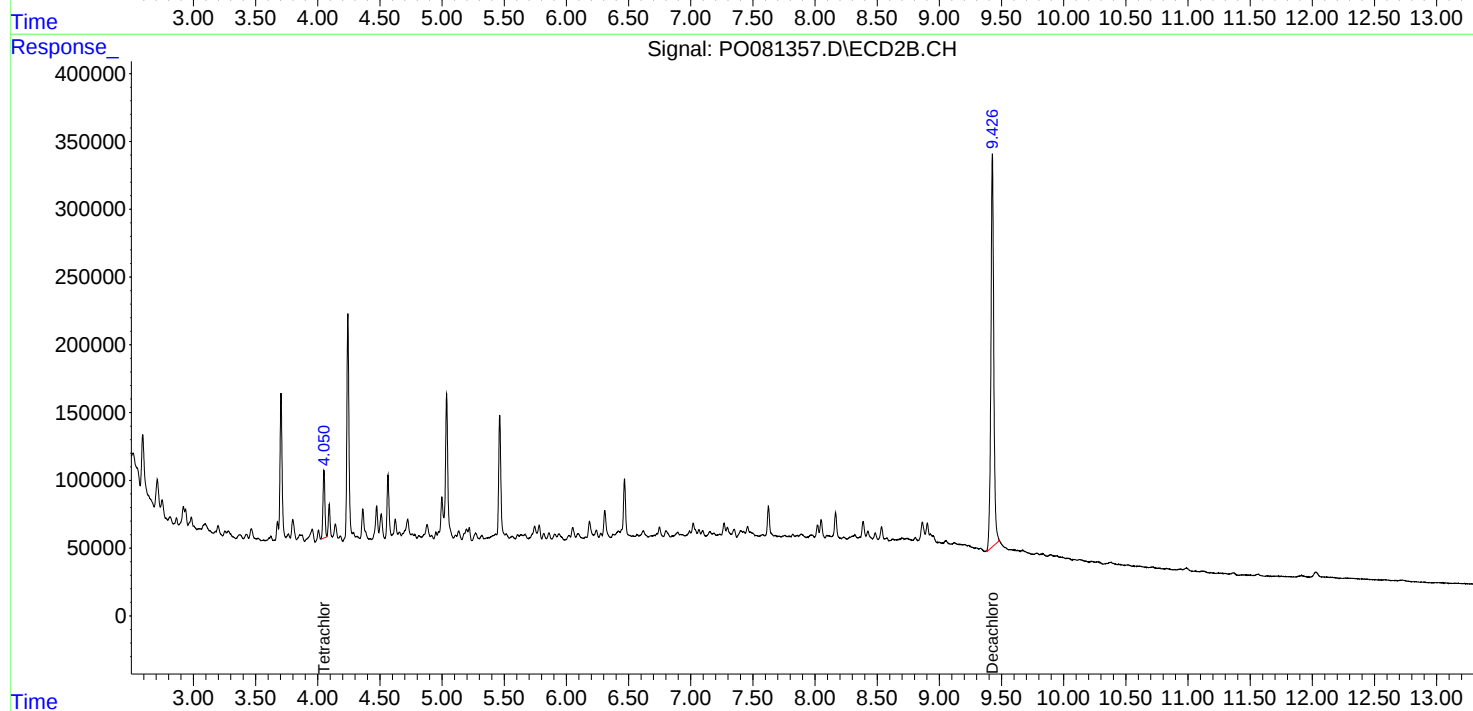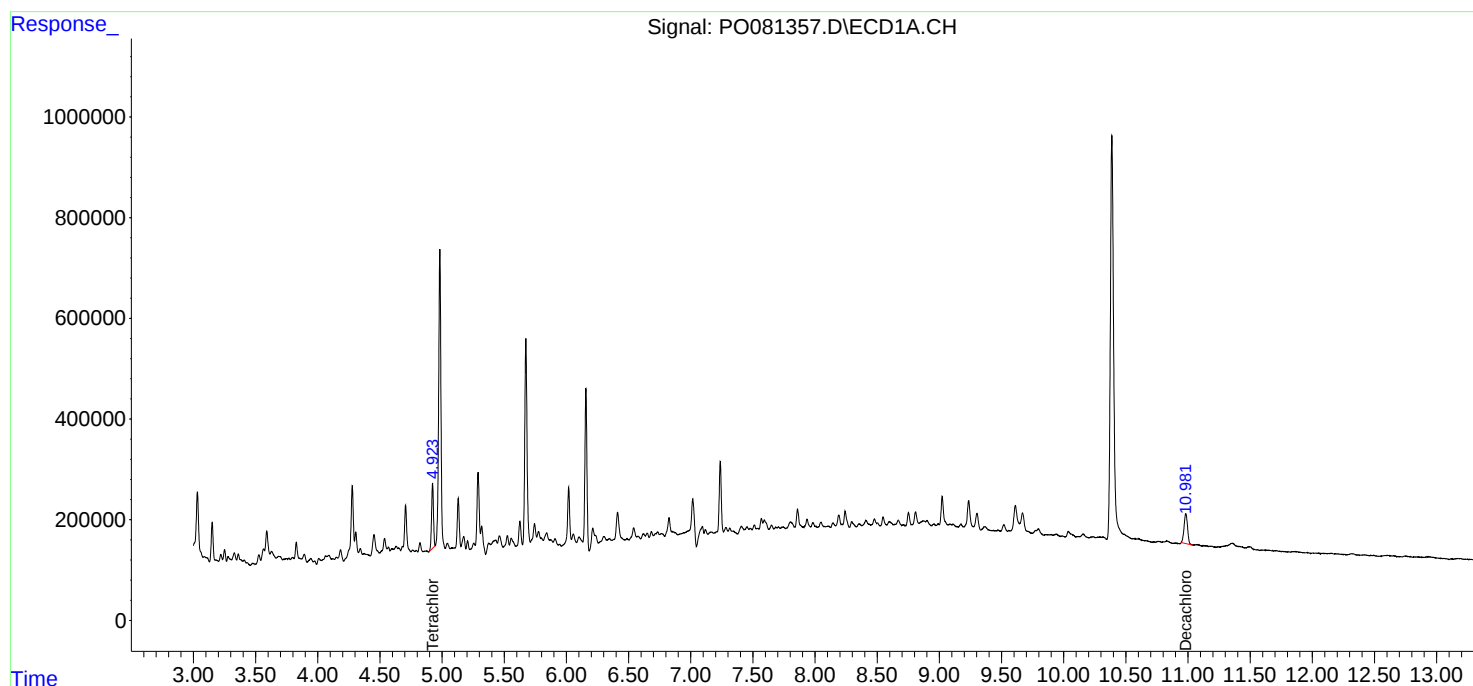

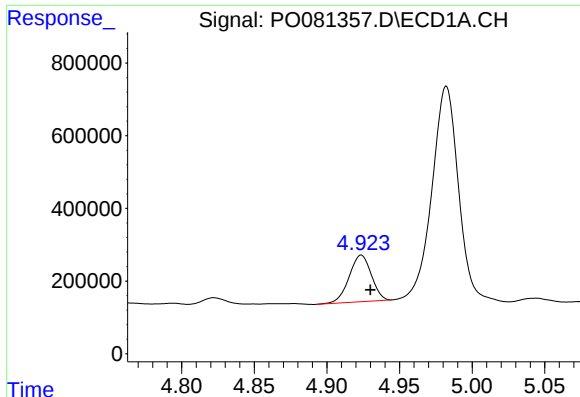


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: -0.006 min
Response: 1366869
Conc: 17.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
SW-CB-03-(1.0)


Manual Integrations
APPROVED

mohammad
9/21/2021 3:00:58 PM

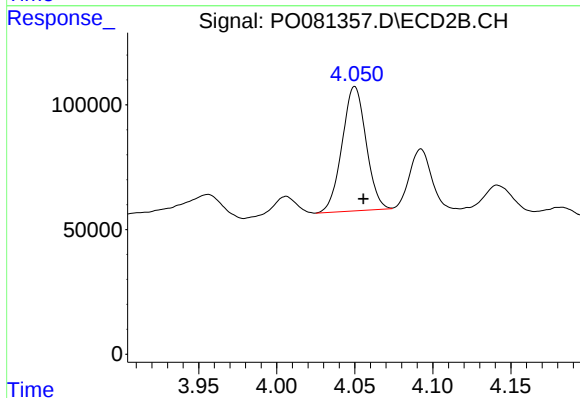


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.005 min
Response: 533027
Conc: 21.57 ng/ml

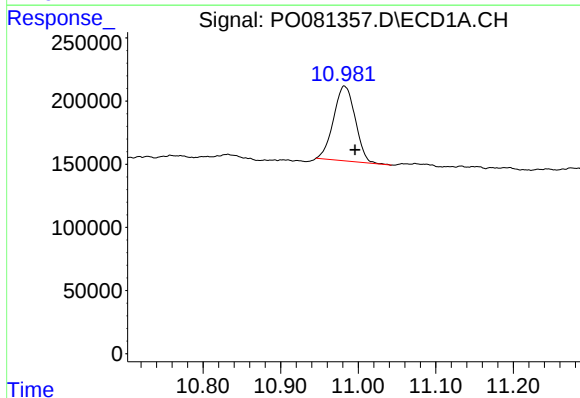

#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.014 min
Response: 1150840
Conc: 19.38 ng/ml

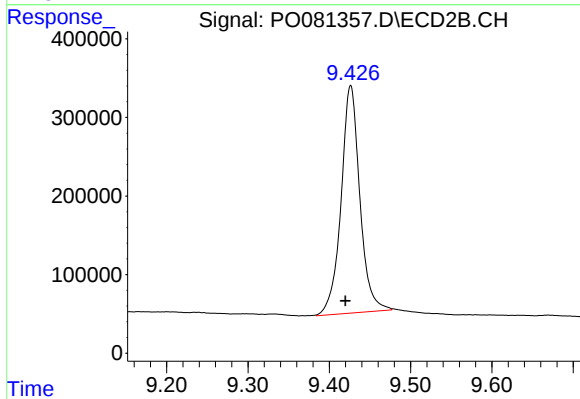

#2 Decachlorobiphenyl

R.T.: 9.426 min
Delta R.T.: 0.006 min
Response: 4647595
Conc: 199.09 ng/ml m