

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091721\
 Data File : P0081358.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2021 13:25
 Operator : AJ\MA
 Sample : M3745-02 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC260212LOK-END-1-2

Manual Integrations
 APPROVED

mohammad
 9/21/2021 3:01:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 17:32:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.049	169076	54682	2.142	2.213
2) SA Decachlor...	10.995	9.411	82394	69630	1.388	2.983m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091721\
Data File : P0081358.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2021 13:25
Operator : AJ\MA
Sample : M3745-02 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC260212LOK-END-1-2


Manual Integrations
APPROVED

mohammad
9/21/2021 3:01:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 17:32:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

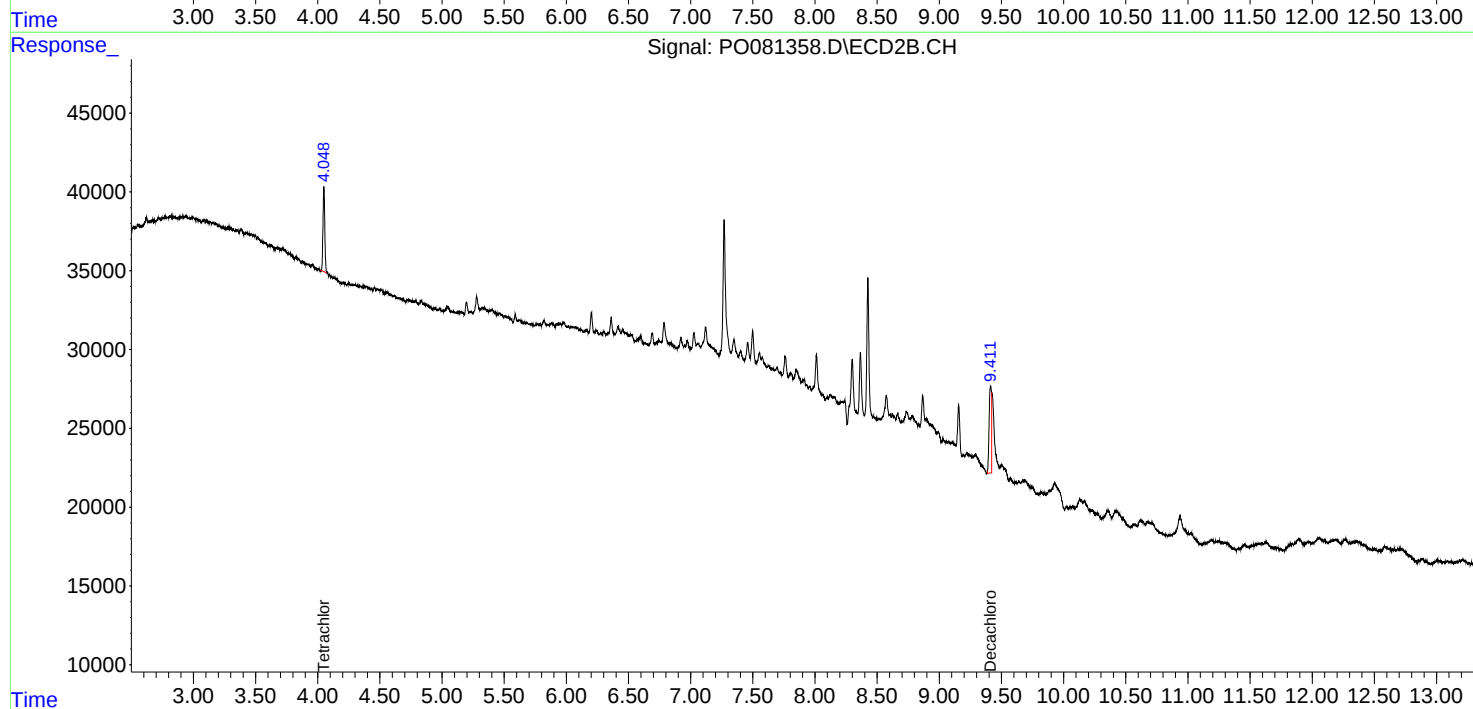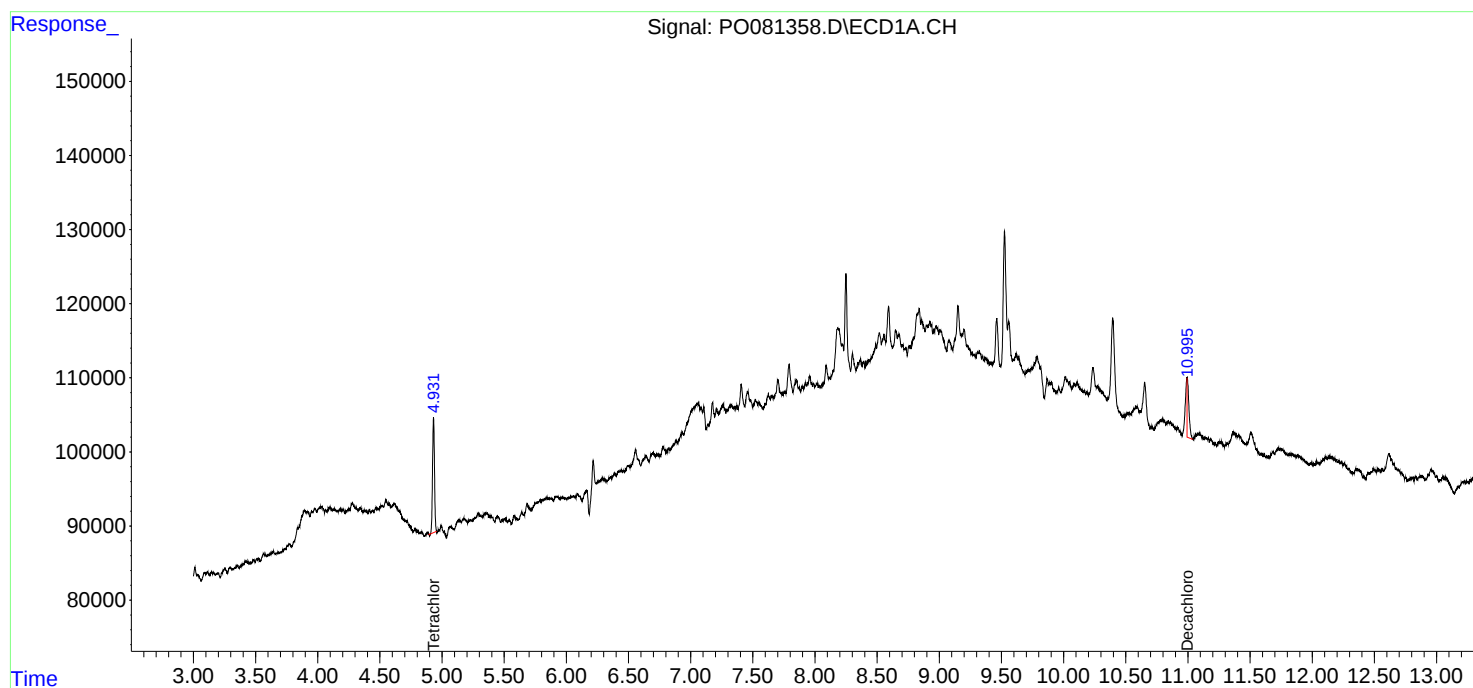

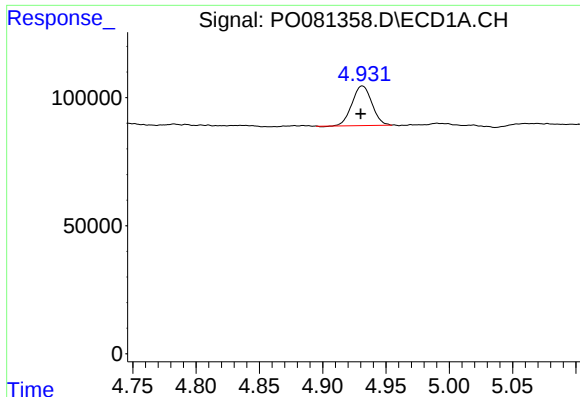


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.001 min
Response: 169076
Conc: 2.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260212LOK-END-1-2


Manual Integrations
APPROVED

mohammad
9/21/2021 3:01:01 PM

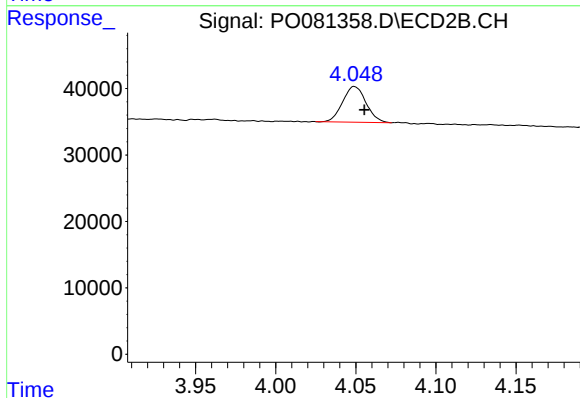


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.006 min
Response: 54682
Conc: 2.21 ng/ml

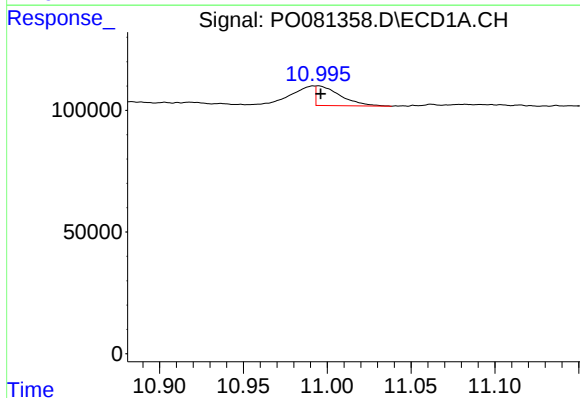

#2 Decachlorobiphenyl

R.T.: 10.995 min
Delta R.T.: 0.000 min
Response: 82394
Conc: 1.39 ng/ml

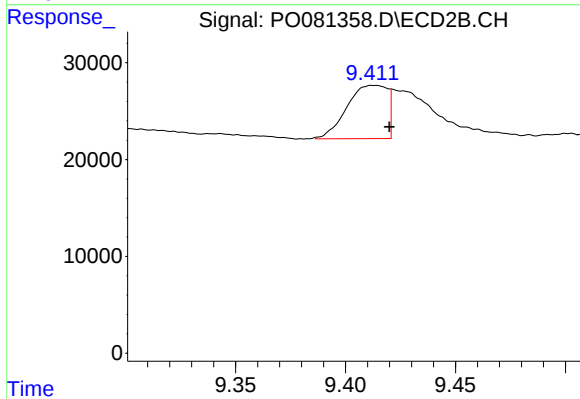

#2 Decachlorobiphenyl

R.T.: 9.411 min
Delta R.T.: -0.009 min
Response: 69630
Conc: 2.98 ng/ml m