

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091721\
 Data File : P0081369.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2021 17:43
 Operator : AJ\MA
 Sample : M3773-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TRE-1203

Manual Integrations
 APPROVED

mohammad
 9/21/2021 3:01:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 04:40:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	4.051	1218667	473098	15.437	19.144
2) SA Decachlor...	10.994	9.416	1058383	445820	17.825	19.098
Target Compounds						
26) L6 AR-1254-1	7.172	6.205	171283	30320	53.000	19.167m#
27) L6 AR-1254-2	7.405	6.367	288856	72999	58.039	50.492m
28) L6 AR-1254-3	7.787	6.792	314365	102848	62.172	45.970m#
29) L6 AR-1254-4	8.087	7.035	246084	99433	65.850m	70.242
30) L6 AR-1254-5	8.518	7.467	340479	166922	82.309	79.112

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091721\
Data File : PO081369.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2021 17:43
Operator : AJ\MA
Sample : M3773-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TRE-1203


Manual Integrations
APPROVED

mohammad
9/21/2021 3:01:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 04:40:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

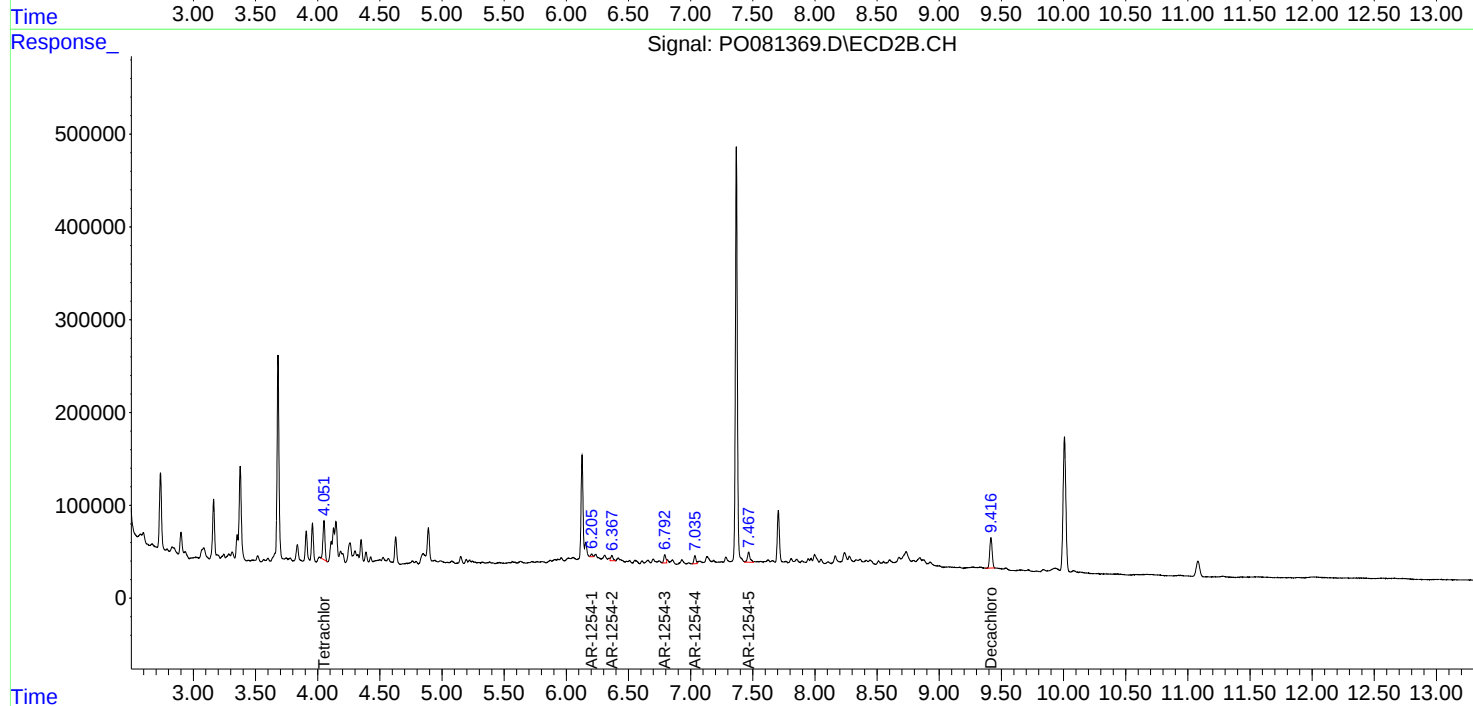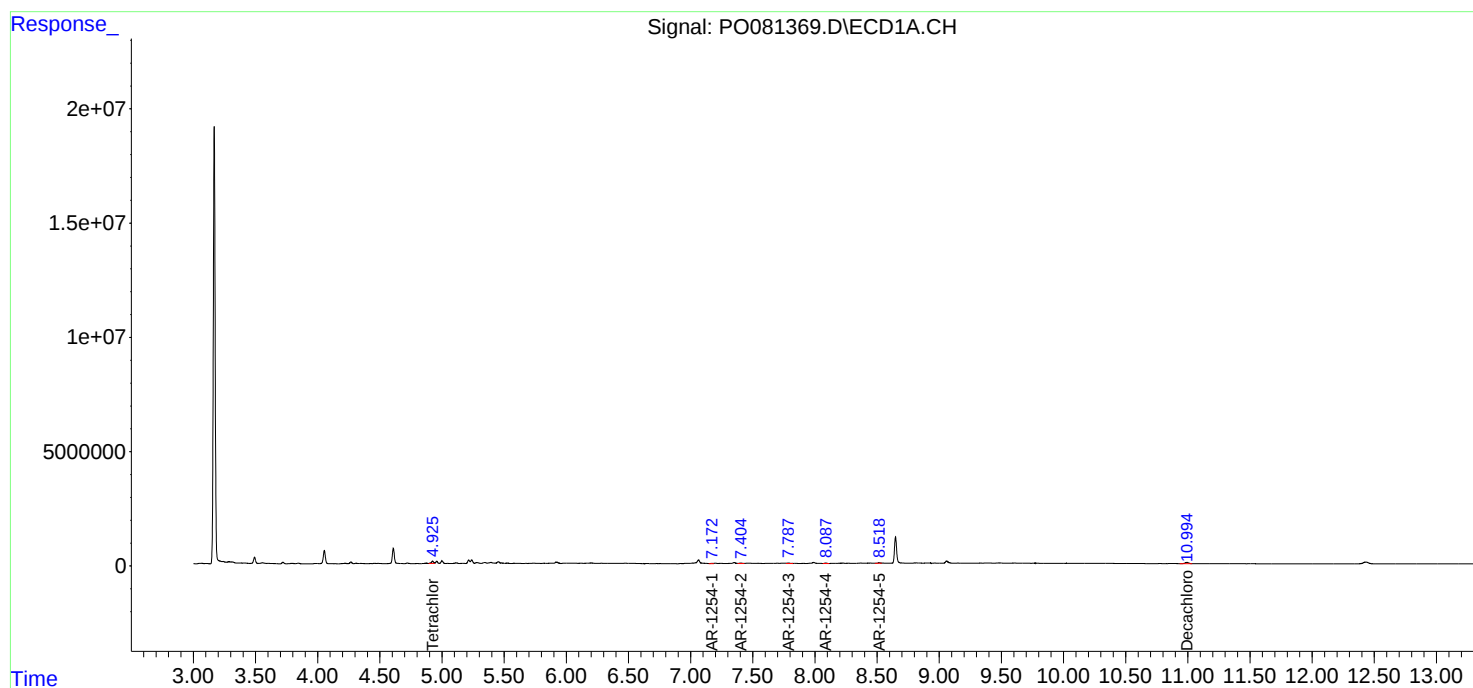

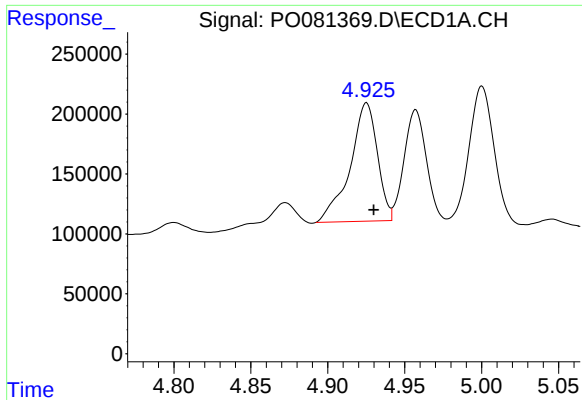


#1 Tetrachloro-m-xylene

R.T.: 4.925 min
Delta R.T.: -0.005 min
Response: 1218667
Conc: 15.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1203


Manual Integrations
APPROVED

mohammad
9/21/2021 3:01:23 PM

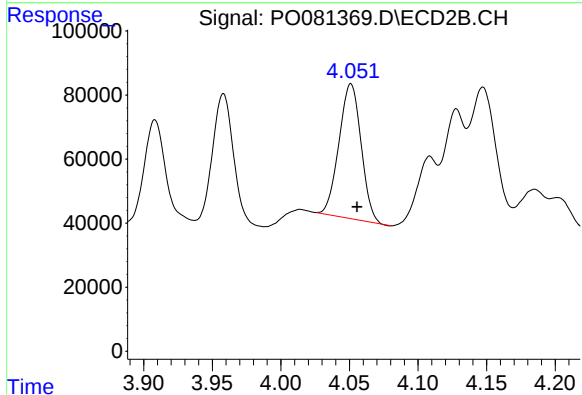


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: -0.004 min
Response: 473098
Conc: 19.14 ng/ml

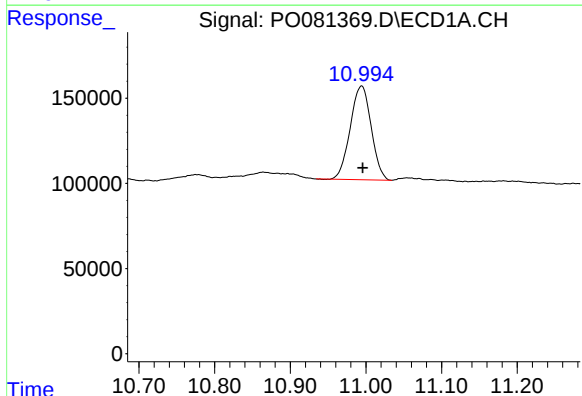


#2 Decachlorobiphenyl

R.T.: 10.994 min
Delta R.T.: -0.002 min
Response: 1058383
Conc: 17.83 ng/ml

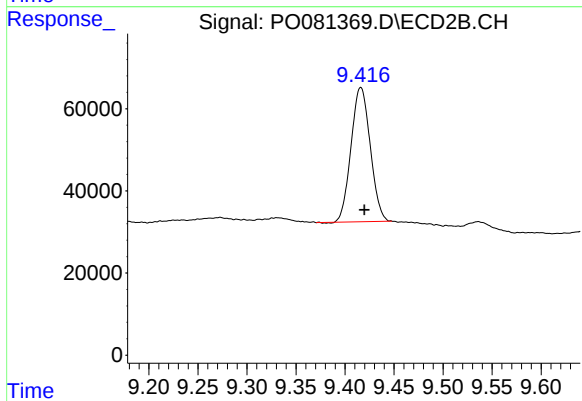

#2 Decachlorobiphenyl

R.T.: 9.416 min
Delta R.T.: -0.004 min
Response: 445820
Conc: 19.10 ng/ml

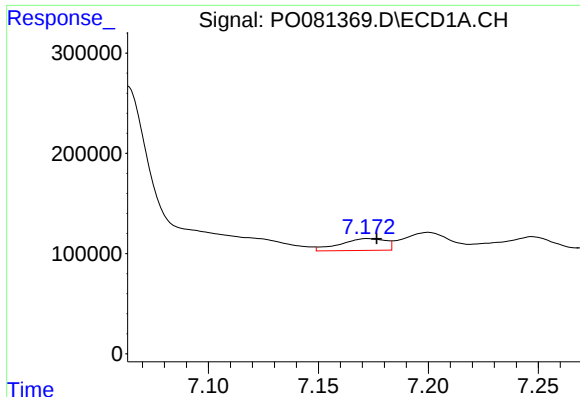


#26 AR-1254-1

R.T.: 7.172 min
Delta R.T.: -0.004 min
Response: 171283
Conc: 53.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1203


Manual Integrations
APPROVED

mohammad
9/21/2021 3:01:23 PM

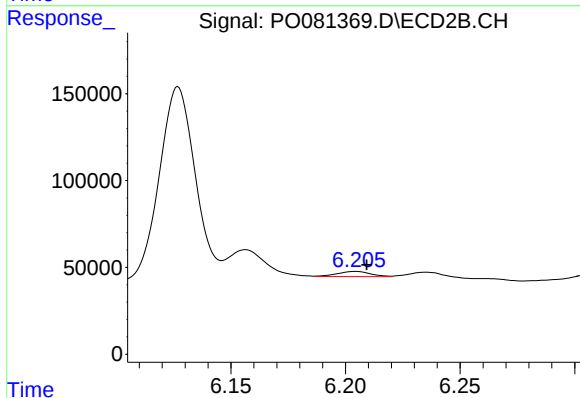


#26 AR-1254-1

R.T.: 6.205 min
Delta R.T.: -0.005 min
Response: 30320
Conc: 19.17 ng/ml m

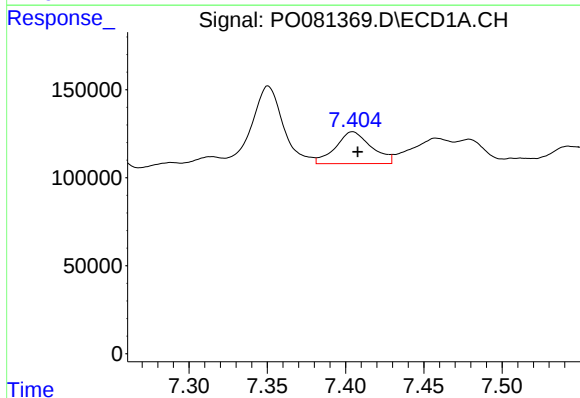


#27 AR-1254-2

R.T.: 7.405 min
Delta R.T.: -0.003 min
Response: 288856
Conc: 58.04 ng/ml

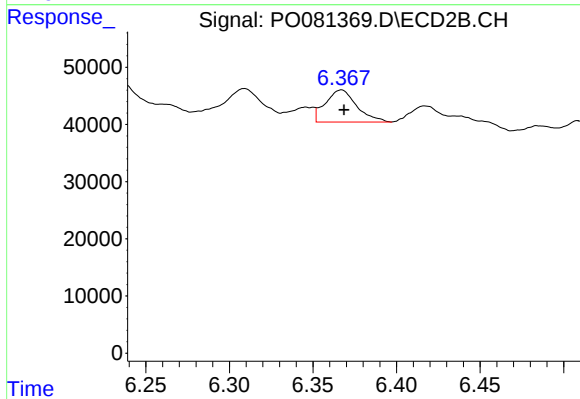

#27 AR-1254-2

R.T.: 6.367 min
Delta R.T.: -0.002 min
Response: 72999
Conc: 50.49 ng/ml m

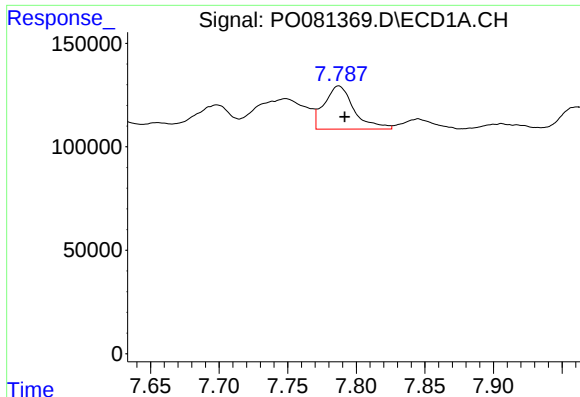


#28 AR-1254-3

R.T.: 7.787 min
Delta R.T.: -0.004 min
Response: 314365
Conc: 62.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1203


Manual Integrations
APPROVED

mohammad
9/21/2021 3:01:23 PM

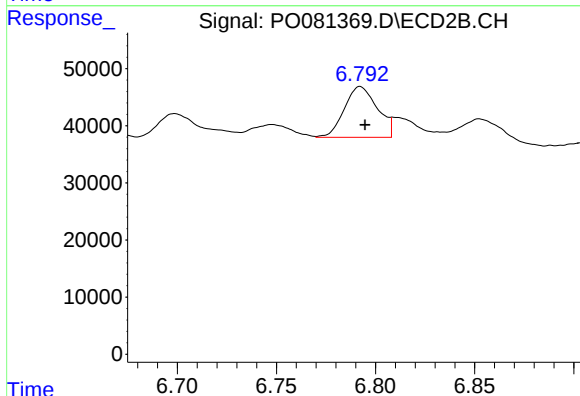


#28 AR-1254-3

R.T.: 6.792 min
Delta R.T.: -0.003 min
Response: 102848
Conc: 45.97 ng/ml m

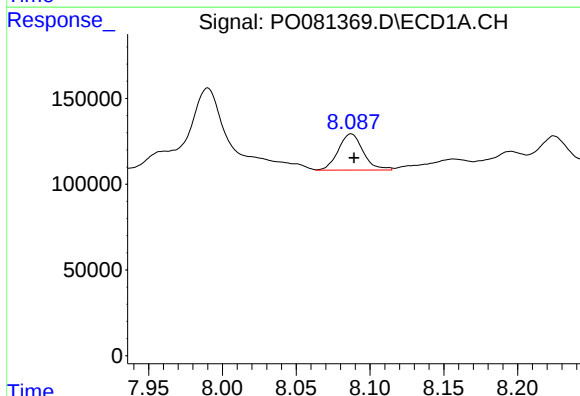


#29 AR-1254-4

R.T.: 8.087 min
Delta R.T.: -0.002 min
Response: 246084
Conc: 65.85 ng/ml m

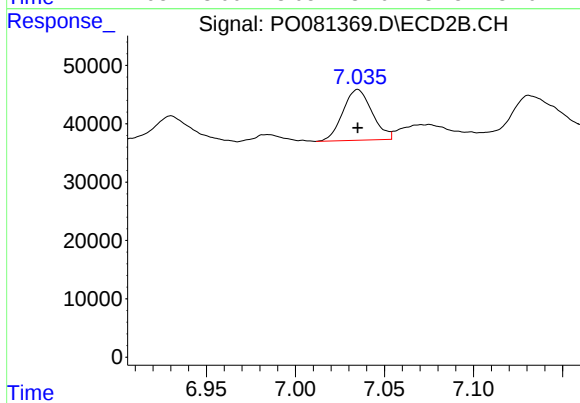

#29 AR-1254-4

R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 99433
Conc: 70.24 ng/ml

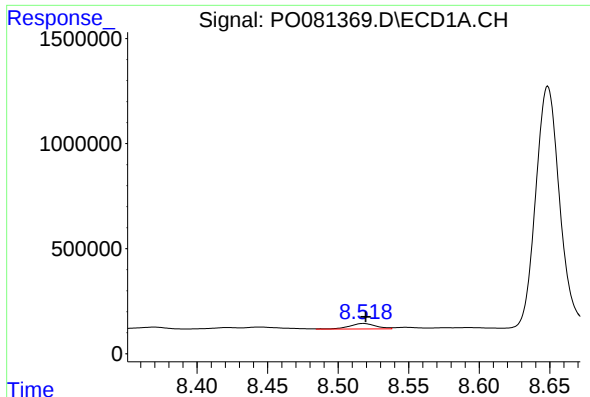


#30 AR-1254-5

R.T.: 8.518 min
Delta R.T.: -0.002 min
Response: 340479
Conc: 82.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1203

Manual Integrations
APPROVED

mohammad
9/21/2021 3:01:23 PM

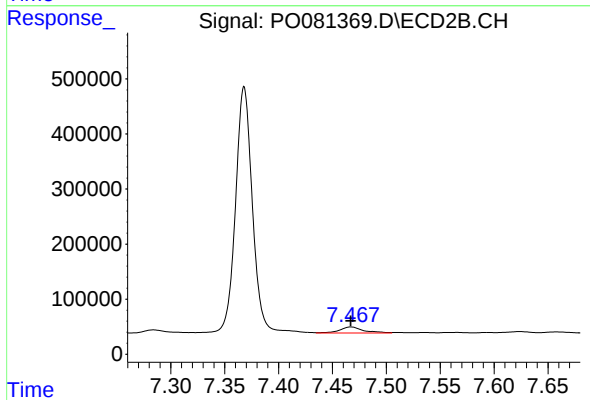

#30 AR-1254-5

R.T.: 7.467 min
Delta R.T.: 0.000 min
Response: 166922
Conc: 79.11 ng/ml