

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091819\
 Data File : P0061075.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Sep 2019 14:01
 Operator : SM/AJ
 Sample : K4923-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-40-COMP

Manual Integrations
 APPROVED

Ankita
 9/19/2019 4:37:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:00:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.369	3.530	970395	762058	26.376	27.292
2)	SA Decachlor...	10.030	8.405	798725	583369	17.384	16.643
Target Compounds							
26)	L6 AR-1254-1	6.383	5.363	464941	47246	241.321	22.924 #
27)	L6 AR-1254-2	6.599	5.506	72566	56338	23.059	29.855m#
28)	L6 AR-1254-3	6.969	5.900	222269	81205	63.109	25.540m#
29)	L6 AR-1254-4	7.249	6.125	64795	57985	23.936m	27.851
30)	L6 AR-1254-5	7.667	6.535	178345	149827	60.480	47.340

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091819\
Data File : PO061075.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2019 14:01
Operator : SM/AJ
Sample : K4923-04
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-40-COMP


Manual Integrations
APPROVED

Ankita
9/19/2019 4:37:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:00:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

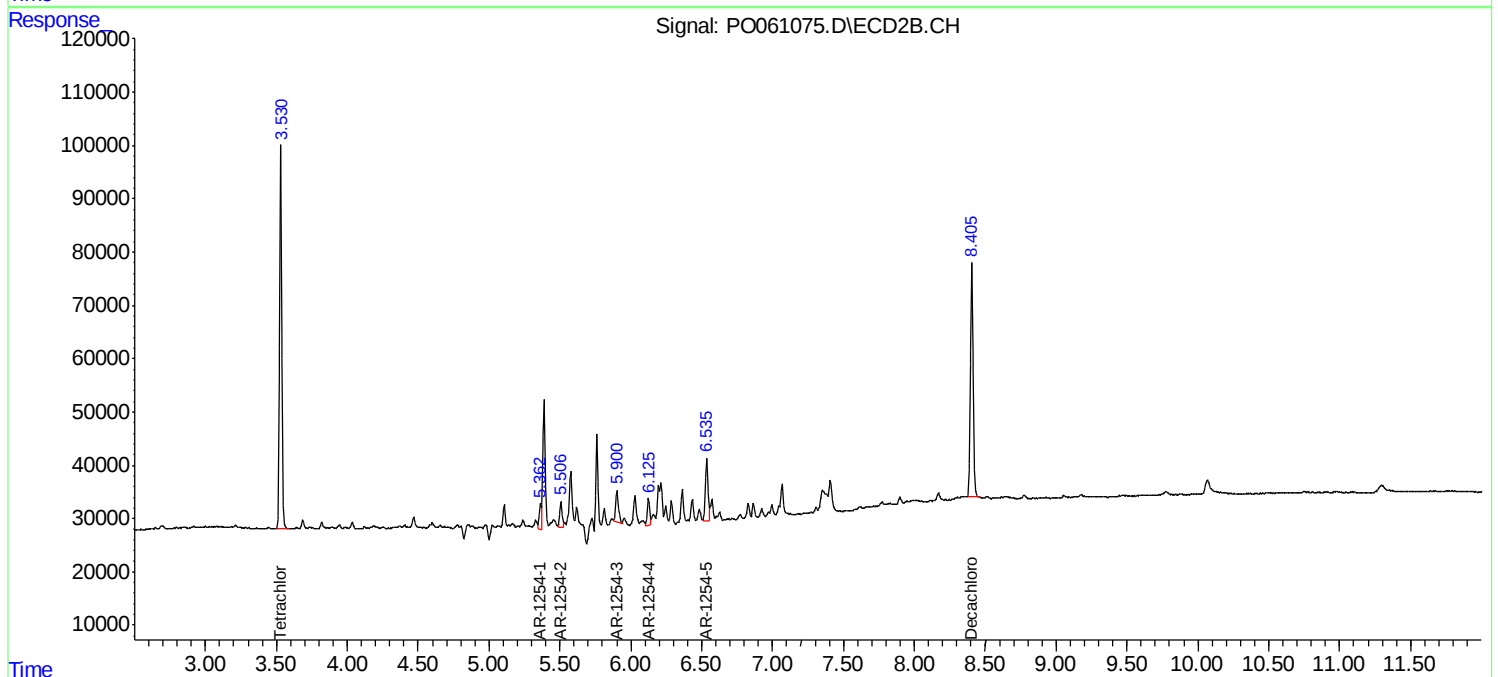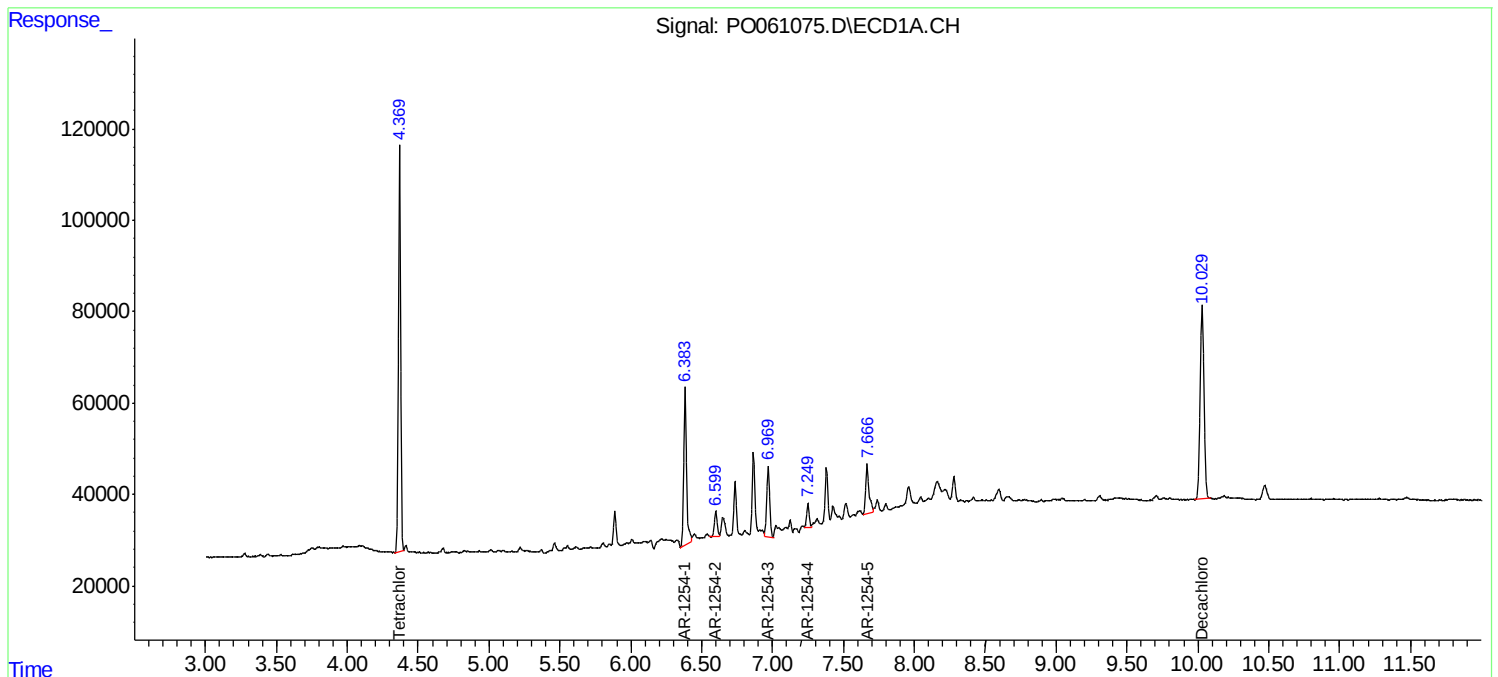

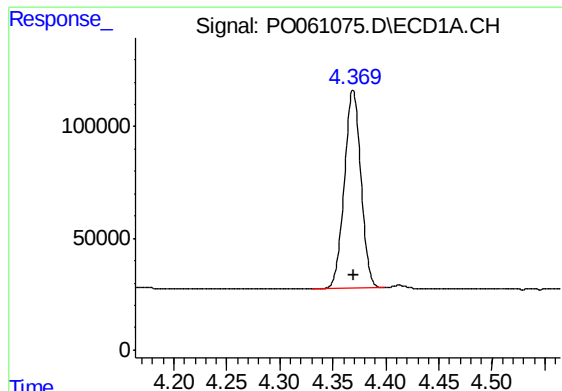


#1 Tetrachloro-m-xylene

R.T.: 4.369 min
Delta R.T.: -0.001 min
Response: 970395
Conc: 26.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP


Manual Integrations
APPROVED

Ankita
9/19/2019 4:37:52 PM

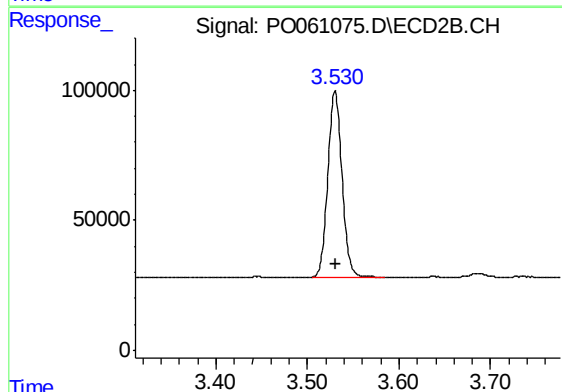


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.001 min
Response: 762058
Conc: 27.29 ng/ml

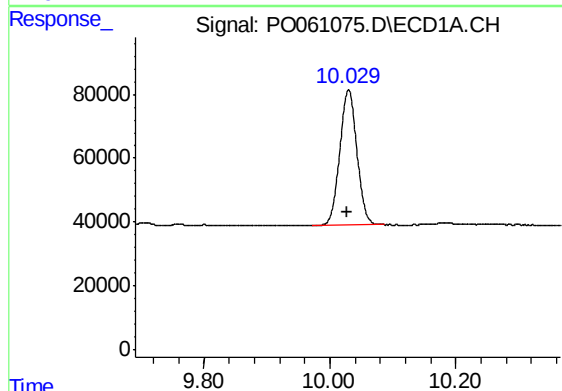


#2 Decachlorobiphenyl

R.T.: 10.030 min
Delta R.T.: 0.002 min
Response: 798725
Conc: 17.38 ng/ml

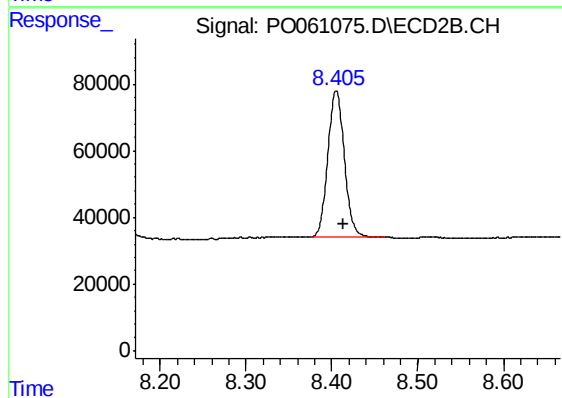

#2 Decachlorobiphenyl

R.T.: 8.405 min
Delta R.T.: -0.008 min
Response: 583369
Conc: 16.64 ng/ml

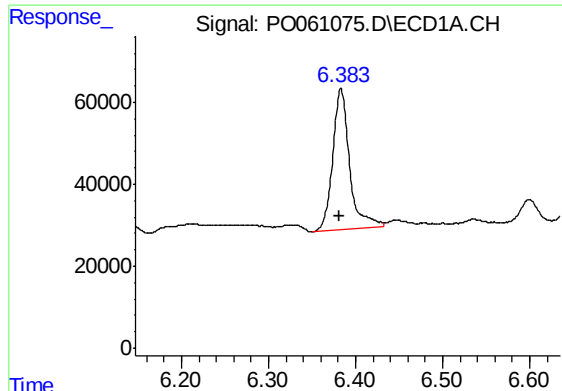


#26 AR-1254-1

R.T.: 6.383 min
Delta R.T.: 0.001 min
Response: 464941
Conc: 241.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP


Manual Integrations
APPROVED

Ankita
9/19/2019 4:37:52 PM

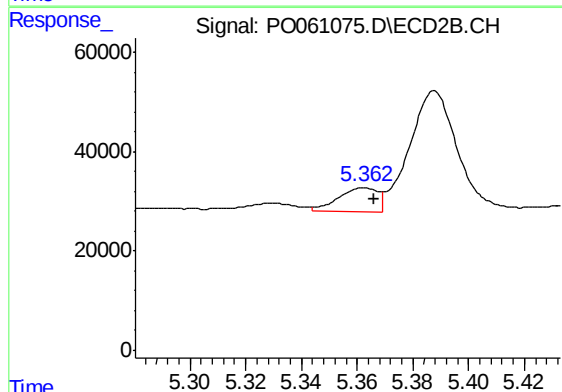


#26 AR-1254-1

R.T.: 5.363 min
Delta R.T.: -0.003 min
Response: 47246
Conc: 22.92 ng/ml

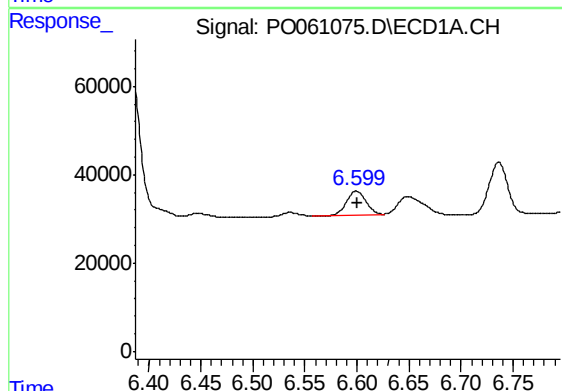


#27 AR-1254-2

R.T.: 6.599 min
Delta R.T.: 0.000 min
Response: 72566
Conc: 23.06 ng/ml

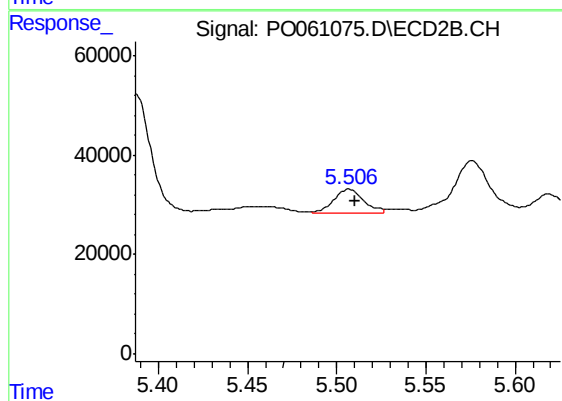

#27 AR-1254-2

R.T.: 5.506 min
Delta R.T.: -0.004 min
Response: 56338
Conc: 29.86 ng/ml m

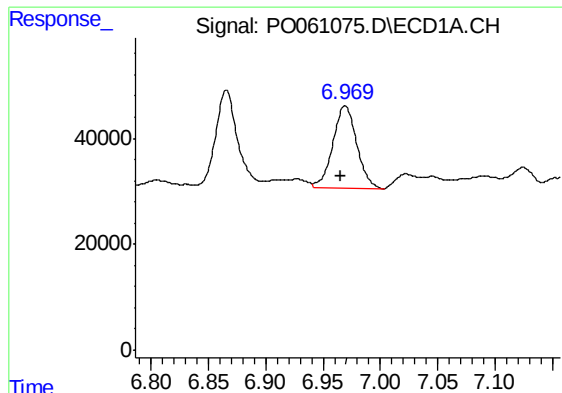


#28 AR-1254-3

R.T.: 6.969 min
Delta R.T.: 0.004 min
Response: 222269
Conc: 63.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP


Manual Integrations
APPROVED

Ankita
9/19/2019 4:37:52 PM

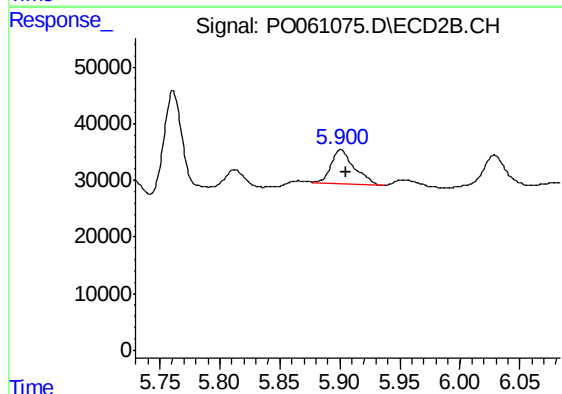


#28 AR-1254-3

R.T.: 5.900 min
Delta R.T.: -0.005 min
Response: 81205
Conc: 25.54 ng/ml m

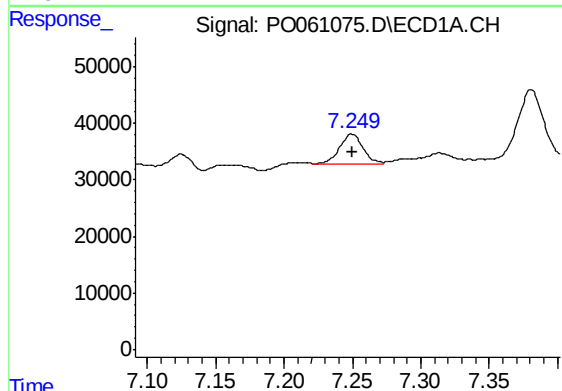


#29 AR-1254-4

R.T.: 7.249 min
Delta R.T.: 0.000 min
Response: 64795
Conc: 23.94 ng/ml m

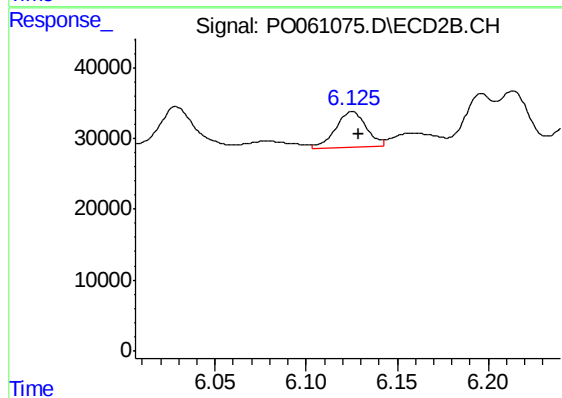

#29 AR-1254-4

R.T.: 6.125 min
Delta R.T.: -0.004 min
Response: 57985
Conc: 27.85 ng/ml

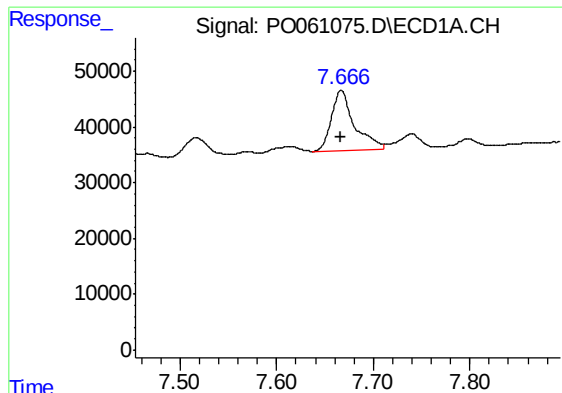


#30 AR-1254-5

R.T.: 7.667 min
Delta R.T.: 0.000 min
Response: 178345
Conc: 60.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-40-COMP

Manual Integrations
APPROVED

Ankita
9/19/2019 4:37:52 PM

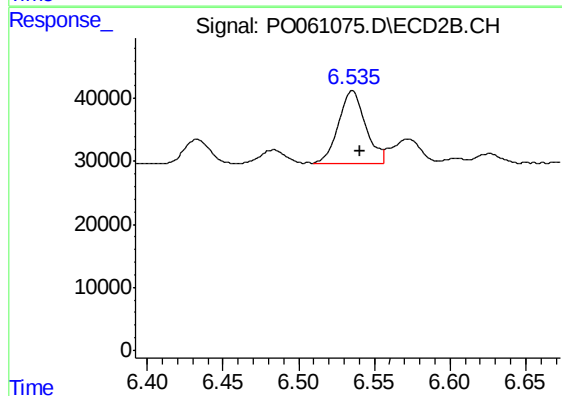

#30 AR-1254-5

R.T.: 6.535 min
Delta R.T.: -0.005 min
Response: 149827
Conc: 47.34 ng/ml