

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091819\
 Data File : P0061086.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Sep 2019 18:04
 Operator : SM/AJ
 Sample : K4922-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GRAB-40303

Manual Integrations
 APPROVED

Ankita
 9/19/2019 4:38:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:07:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.362	3.524	447364	410579	12.160	14.704m
2)	SA Decachlor...	10.021	8.402	647132	465079	14.085	13.268

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091819\
Data File : PO061086.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2019 18:04
Operator : SM/AJ
Sample : K4922-02
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
GRAB-40303


Manual Integrations
APPROVED

Ankita
9/19/2019 4:38:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:07:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

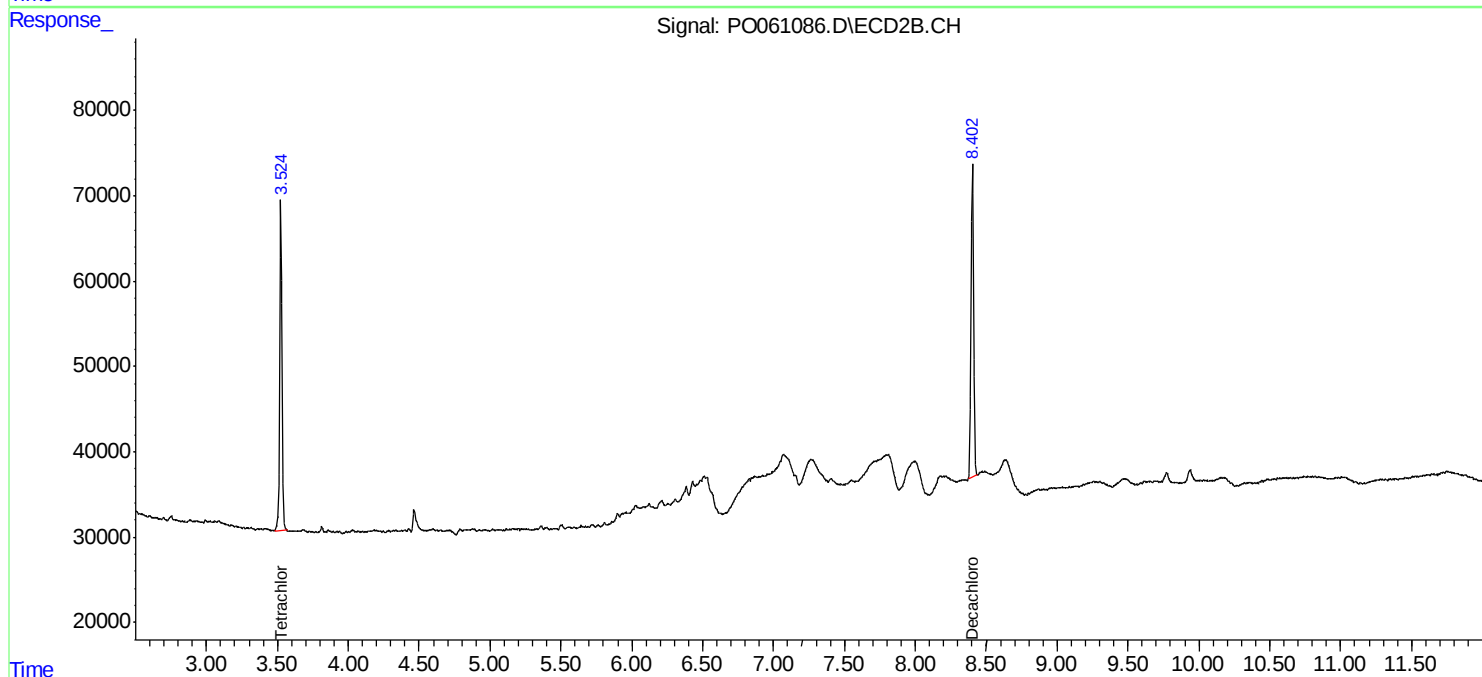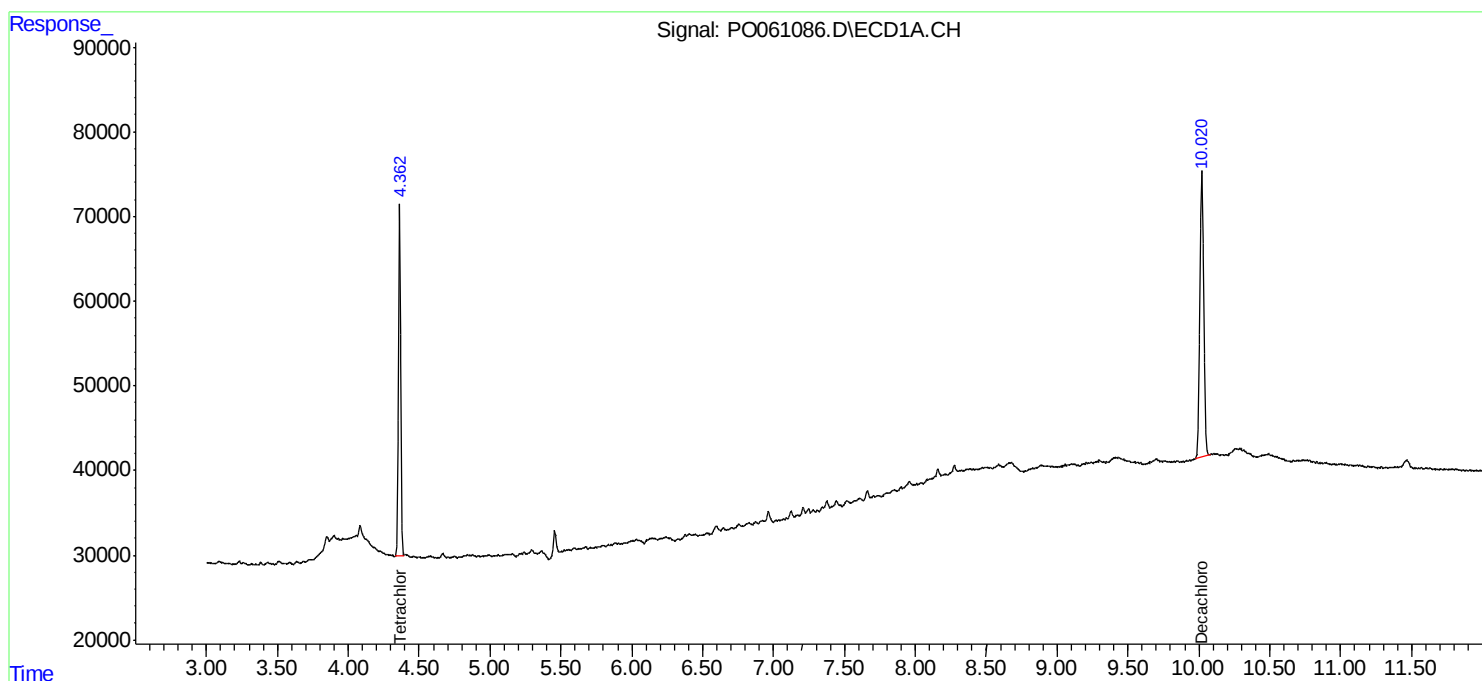

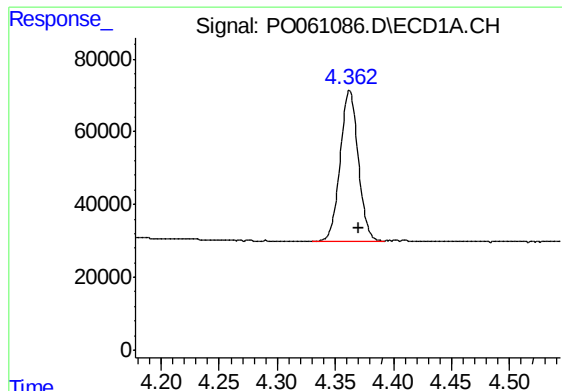


#1 Tetrachloro-m-xylene

R.T.: 4.362 min
Delta R.T.: -0.008 min
Response: 447364
Conc: 12.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
GRAB-40303


Manual Integrations
APPROVED

Ankita
9/19/2019 4:38:04 PM

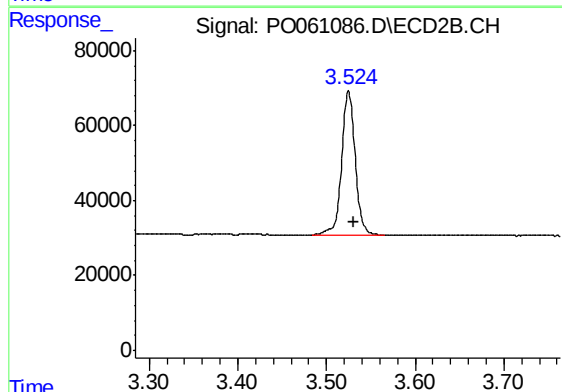


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: -0.007 min
Response: 410579
Conc: 14.70 ng/ml m

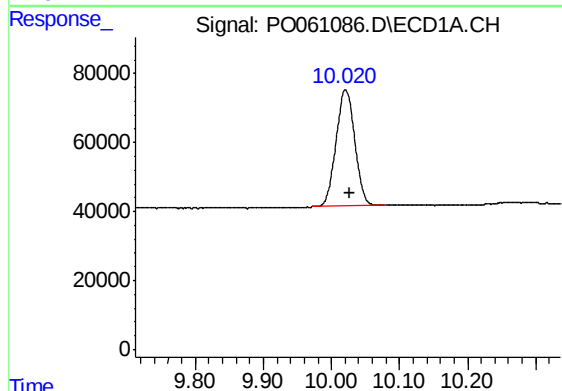

#2 Decachlorobiphenyl

R.T.: 10.021 min
Delta R.T.: -0.007 min
Response: 647132
Conc: 14.08 ng/ml

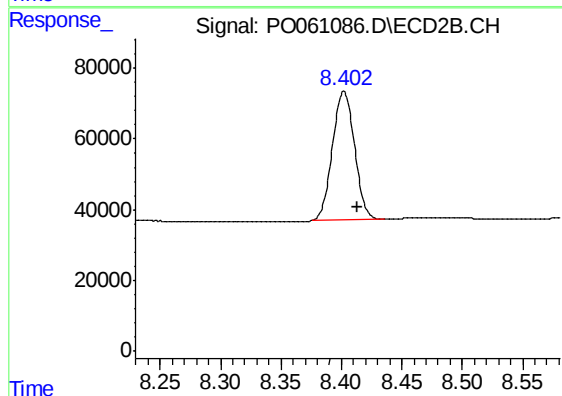

#2 Decachlorobiphenyl

R.T.: 8.402 min
Delta R.T.: -0.011 min
Response: 465079
Conc: 13.27 ng/ml