Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091819\
Data File : PO061119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2019 3:46
Operator : SM/AJ
Sample : K4937-04 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument : ECD_O
ClientSampleId : HA15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:03:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	4.365	3.528	254654	243121	6.922	8.707 #
2)	SA Decachlor...	10.024	8.403	161830	121074	3.522	3.454
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091819\
Data File : PO061119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2019 3:46
Operator : SM/AJ
Sample : K4937-04 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument : ECD_O
ClientSampleId : HA15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:03:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

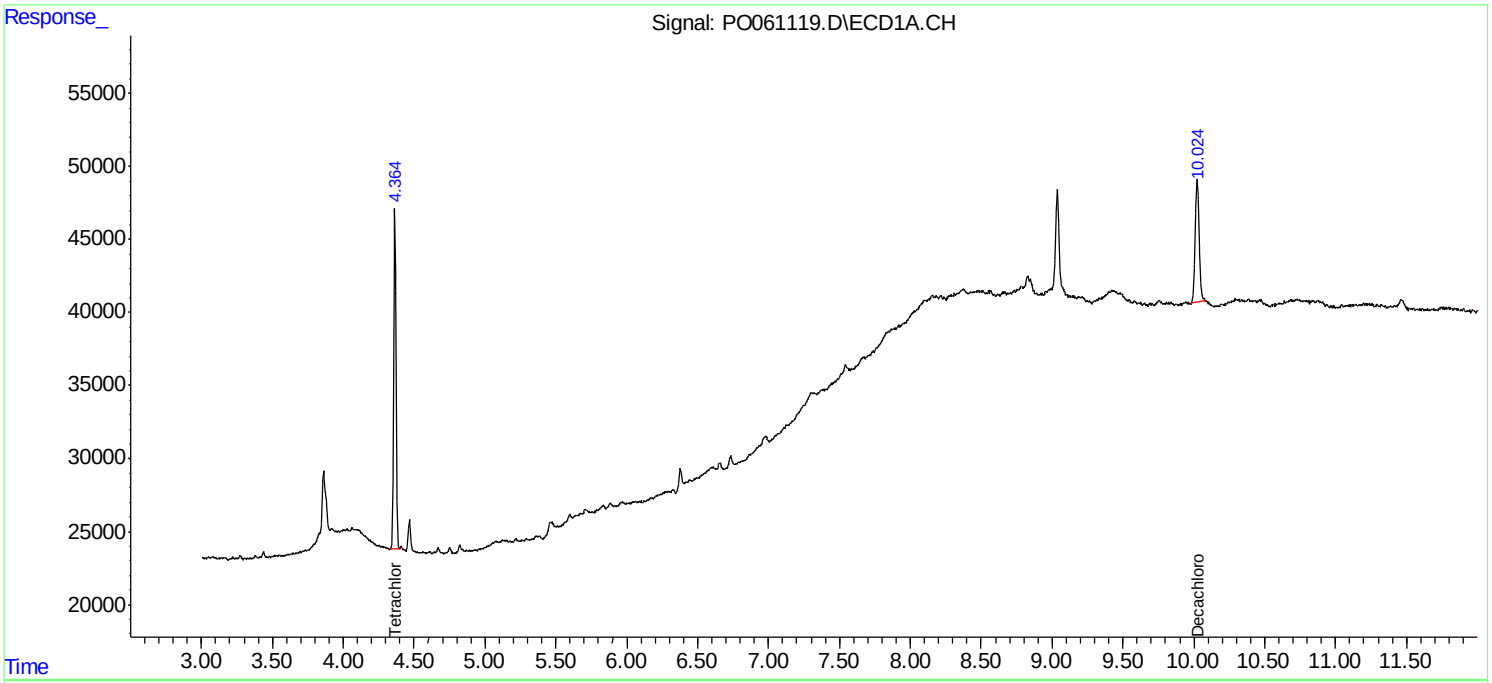

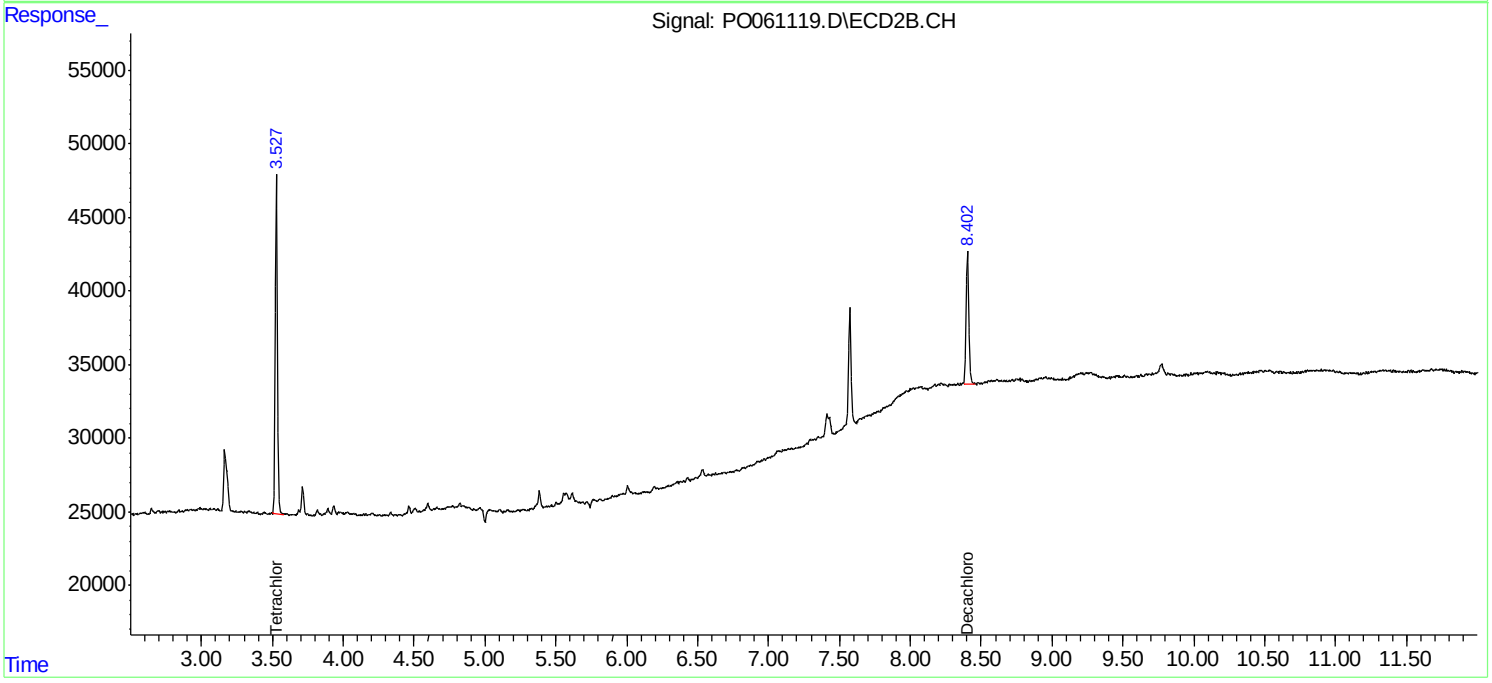

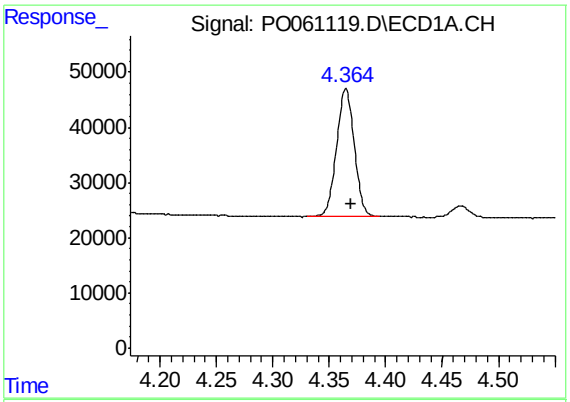

#1 Tetrachloro-m-xylene

R.T.: 4.365 min
Delta R.T.: -0.005 min
Response: 254654
Conc: 6.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA15

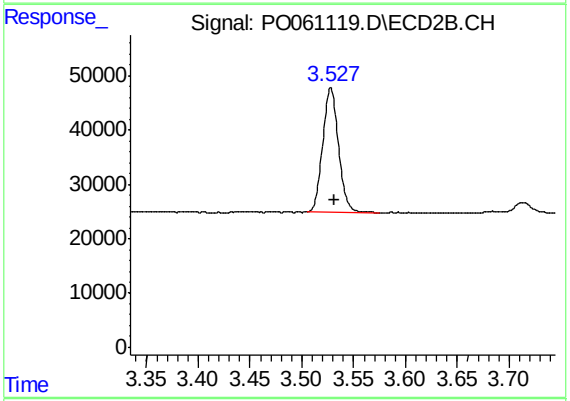

#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: -0.004 min
Response: 243121
Conc: 8.71 ng/ml

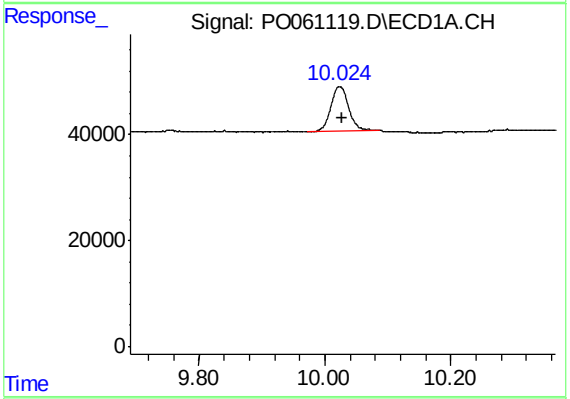

#2 Decachlorobiphenyl

R.T.: 10.024 min
Delta R.T.: -0.004 min
Response: 161830
Conc: 3.52 ng/ml

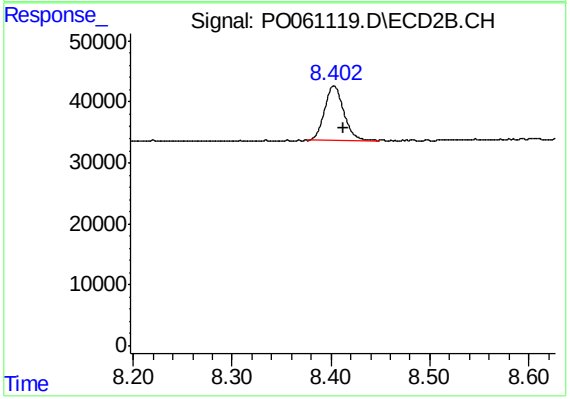

#2 Decachlorobiphenyl

R.T.: 8.403 min
Delta R.T.: -0.010 min
Response: 121074
Conc: 3.45 ng/ml