

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091820\
 Data File : P0071445.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Sep 2020 15:15
 Operator : DD\AJ
 Sample : PB131719BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 02:34:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.342	3.527	1310016	730813	18.486	18.719
2)	SA Decachlor...	9.956	8.707	1894233	1036228	20.313	18.812
Target Compounds							
3)	L1 AR-1016-1	5.661	0.000	175158	0	60.258	N.D. #
4)	L1 AR-1016-2	5.661	0.000	175158	0	41.047	N.D. #
13)	L3 AR-1232-3	5.661	0.000	175158	0	102.231	N.D. #
16)	L4 AR-1242-1	5.661	0.000	175158	0	74.843	N.D. #
17)	L4 AR-1242-2	5.661	0.000	175158	0	51.672	N.D. #
21)	L5 AR-1248-1	5.661	0.000	175158	0	104.140	N.D. #
35)	L7 AR-1260-5	8.491f	0.000	42318	0	3.337	N.D. #
37)	L8 AR-1262-2	8.491f	0.000	42318	0	2.931	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091820\
Data File : PO071445.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2020 15:15
Operator : DD\AJ
Sample : PB131719BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 02:34:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

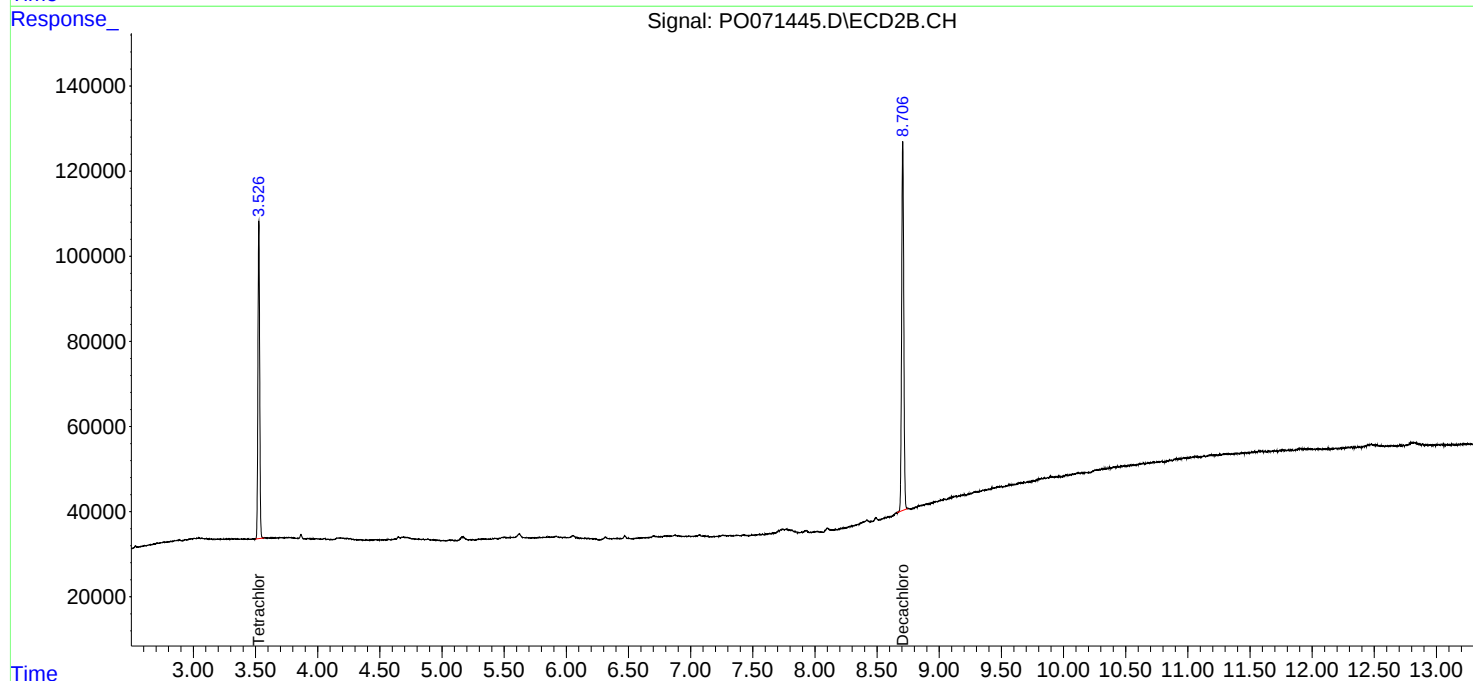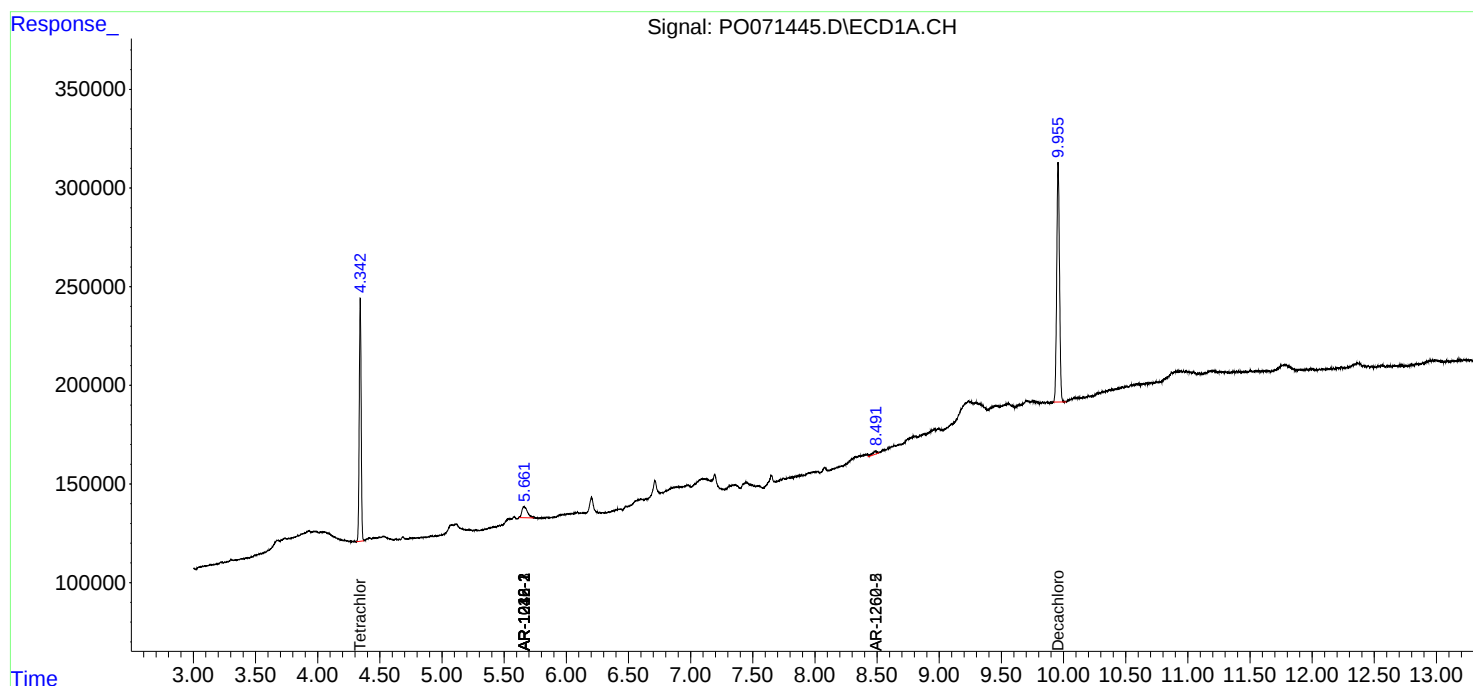


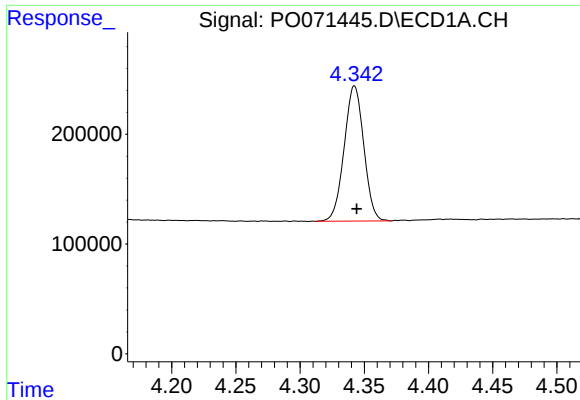

#1 Tetrachloro-m-xylene


R.T.: 4.342 min
Delta R.T.: -0.002 min
Response: 1310016
Conc: 18.49 ng/ml

Instrument :
ECD_O
ClientSampleId :

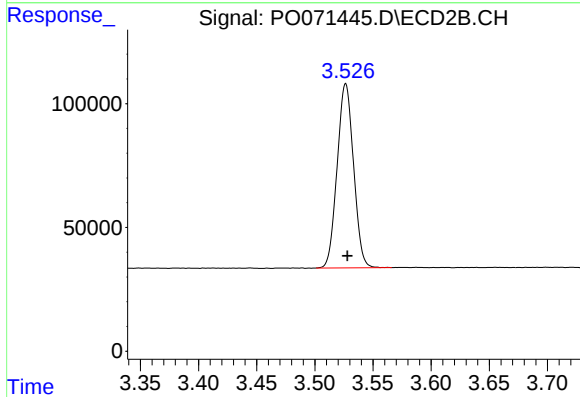


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: -0.001 min
Response: 730813
Conc: 18.72 ng/ml

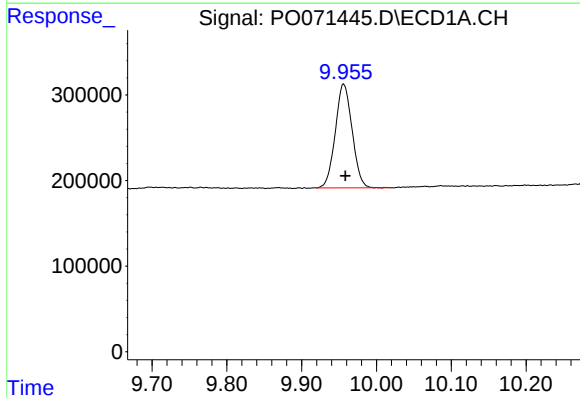


#2 Decachlorobiphenyl

R.T.: 9.956 min
Delta R.T.: -0.002 min
Response: 1894233
Conc: 20.31 ng/ml

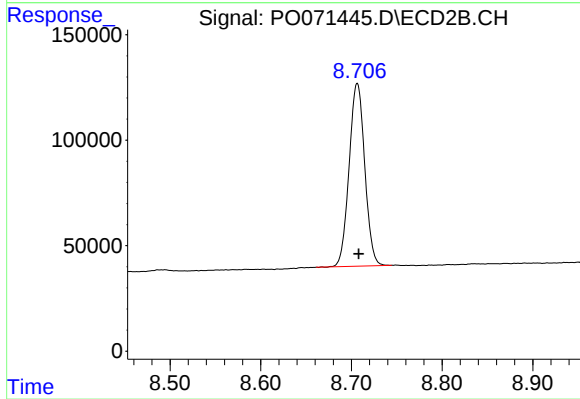

#2 Decachlorobiphenyl


R.T.: 8.707 min
Delta R.T.: -0.002 min
Response: 1036228
Conc: 18.81 ng/ml

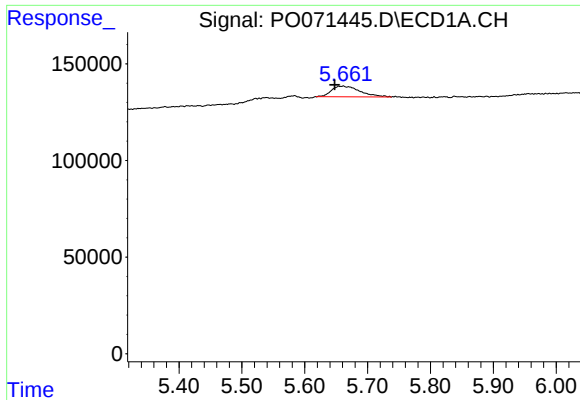

#3 AR-1016-1


R.T.: 5.661 min
Delta R.T.: 0.013 min
Response: 175158
Conc: 60.26 ng/ml

Instrument :
ECD_O
ClientSampleId :

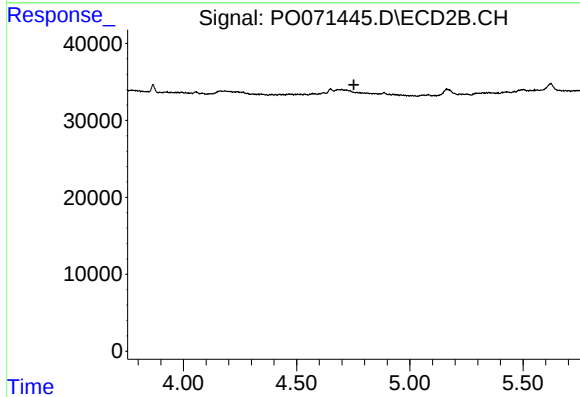


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.753 min
Response: 0
Conc: N.D.

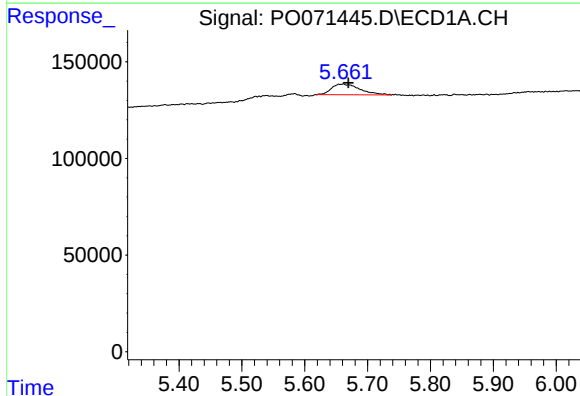


#4 AR-1016-2

R.T.: 5.661 min
Delta R.T.: -0.008 min
Response: 175158
Conc: 41.05 ng/ml

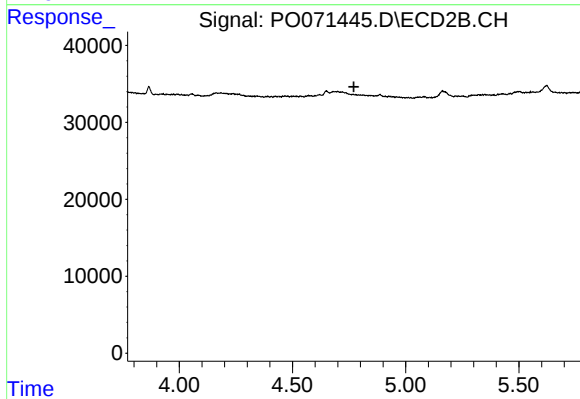

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.771 min
Response: 0
Conc: N.D.

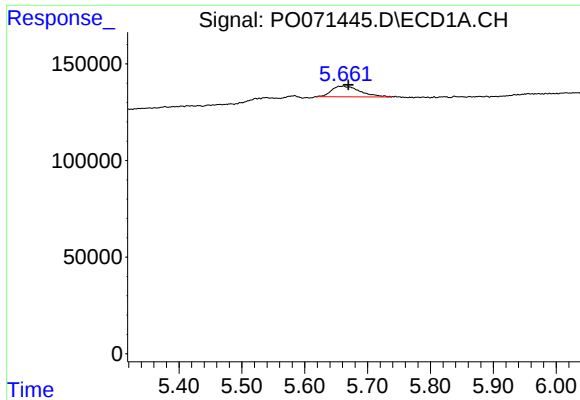

#13 AR-1232-3


R.T.: 5.661 min
Delta R.T.: -0.008 min
Response: 175158
Conc: 102.23 ng/ml

Instrument :
ECD_O
ClientSampleId :

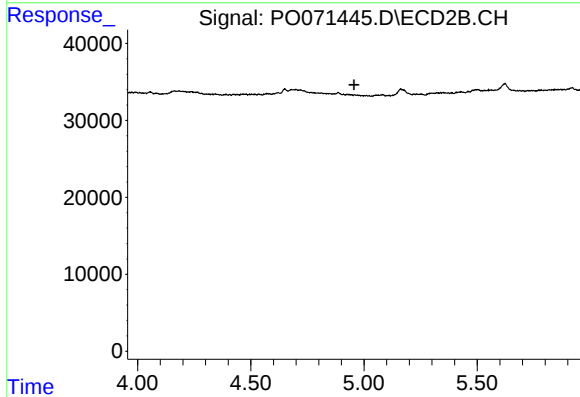


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

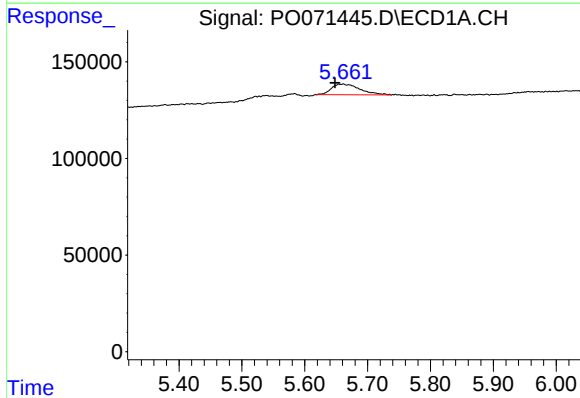


#16 AR-1242-1

R.T.: 5.661 min
Delta R.T.: 0.013 min
Response: 175158
Conc: 74.84 ng/ml

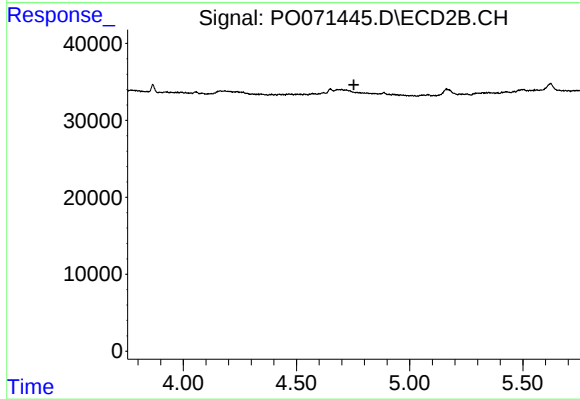

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.754 min
Response: 0
Conc: N.D.

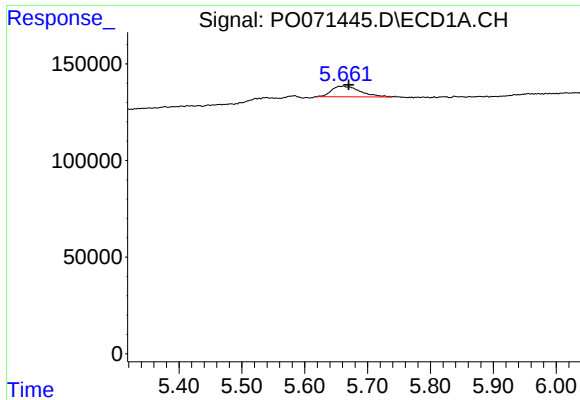

#17 AR-1242-2


R.T.: 5.661 min
Delta R.T.: -0.008 min
Response: 175158
Conc: 51.67 ng/ml

Instrument :
ECD_O
ClientSampleId :

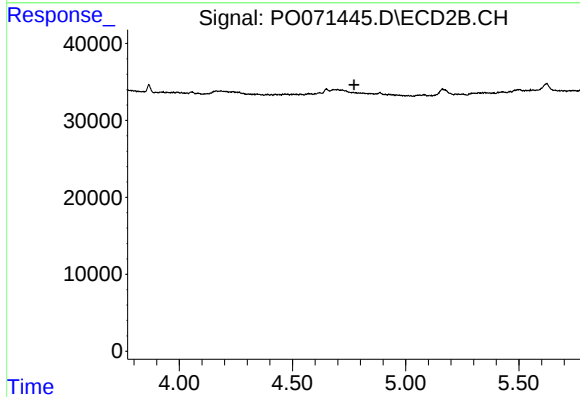


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.771 min
Response: 0
Conc: N.D.

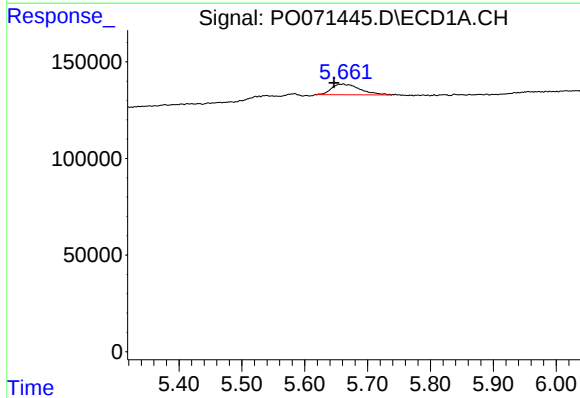


#21 AR-1248-1

R.T.: 5.661 min
Delta R.T.: 0.014 min
Response: 175158
Conc: 104.14 ng/ml

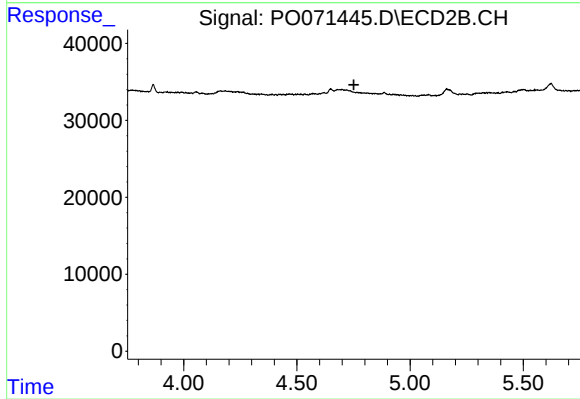

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.752 min
Response: 0
Conc: N.D.

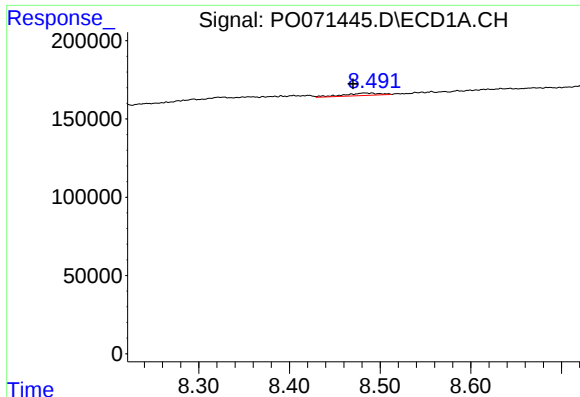

#35 AR-1260-5


R.T.: 8.491 min
Delta R.T.: 0.021 min
Response: 42318
Conc: 3.34 ng/ml

Instrument :
ECD_O
ClientSampleId :

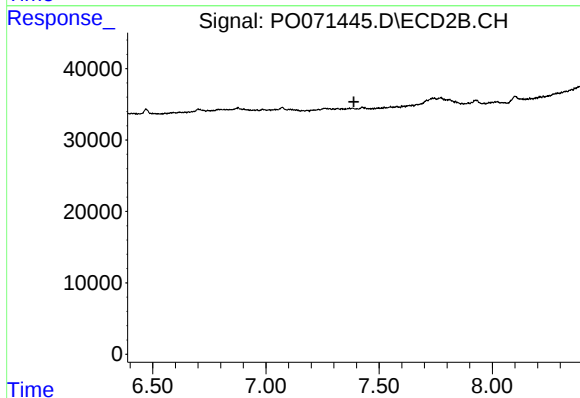


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

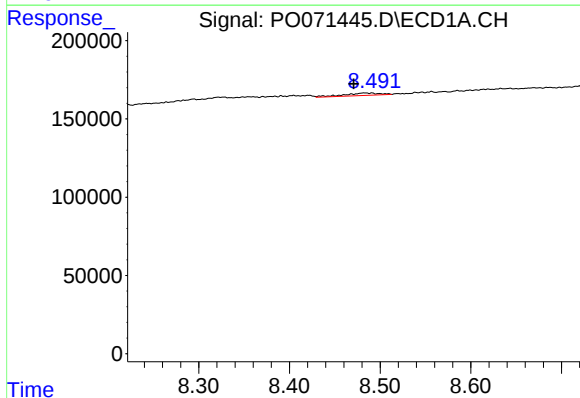

#37 AR-1262-2

R.T.: 8.491 min
Delta R.T.: 0.020 min
Response: 42318
Conc: 2.93 ng/ml

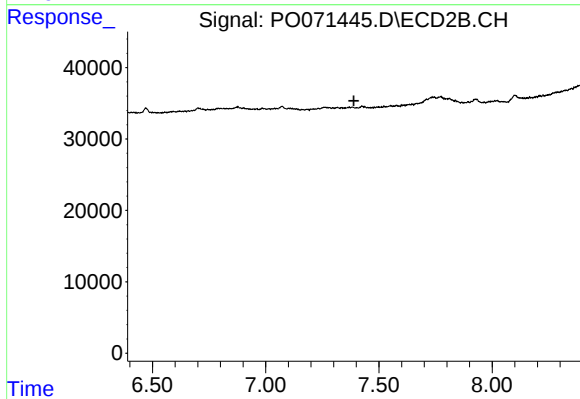

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.