

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091820\
 Data File : P0071453.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Sep 2020 17:35
 Operator : DD\AJ
 Sample : L4056-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 228

Manual Integrations
 APPROVED

Ankita
 9/21/2020 1:05:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 02:37:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.342	3.527	976668	549332	13.782m	14.071
2) SA Decachlor...	9.957	8.706	1078342	753051	11.563	13.671

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091820\
Data File : P0071453.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2020 17:35
Operator : DD\AJ
Sample : L4056-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
228


Manual Integrations
APPROVED

Ankita
9/21/2020 1:05:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 02:37:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

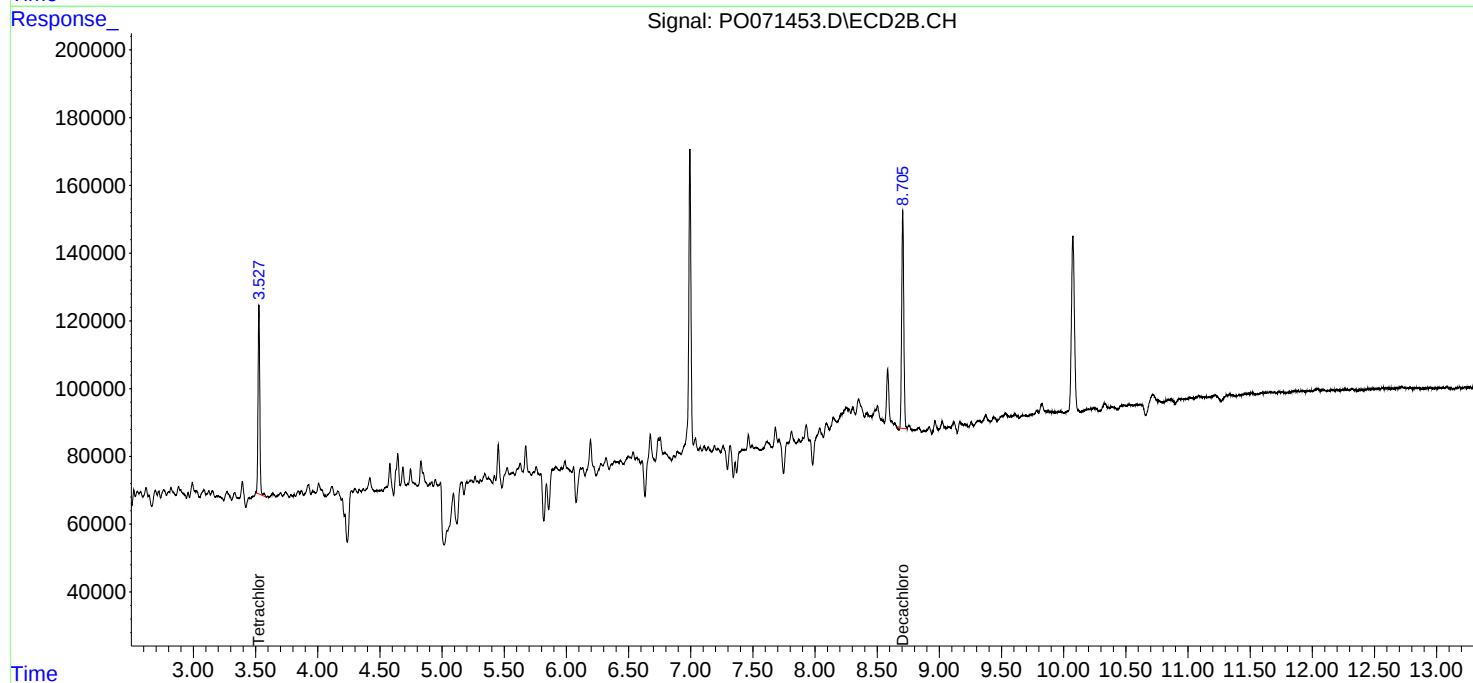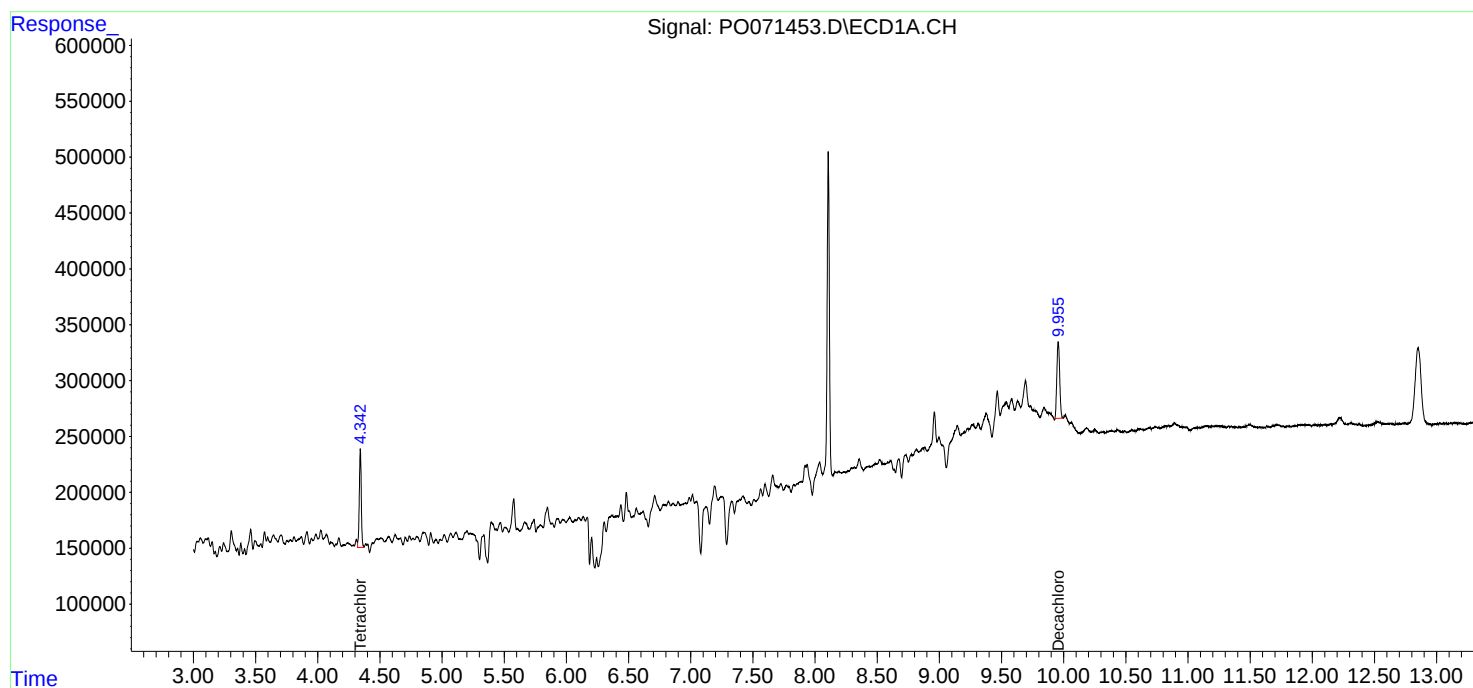

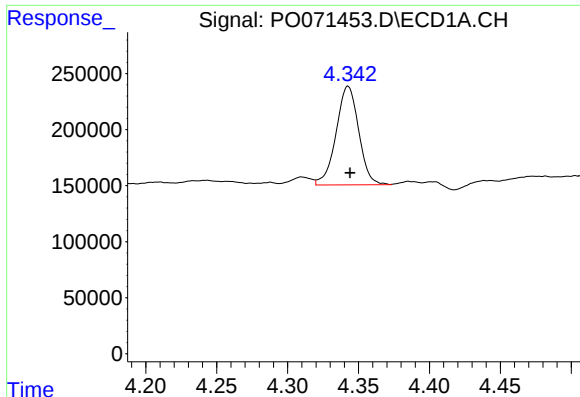


#1 Tetrachloro-m-xylene

R.T.: 4.342 min
Delta R.T.: -0.002 min
Response: 976668
Conc: 13.78 ng/ml m

Instrument :
ECD_O
ClientSampleId :
228


Manual Integrations
APPROVED

Ankita
9/21/2020 1:05:18 PM

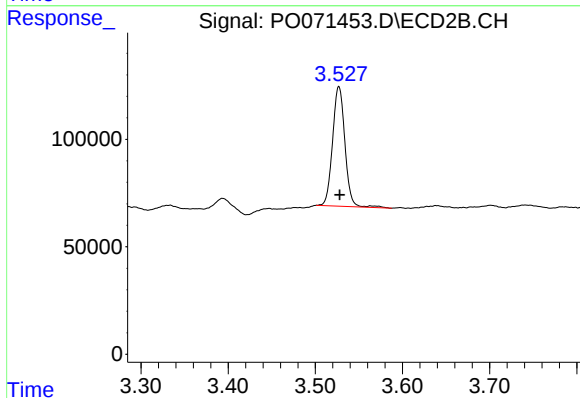


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 549332
Conc: 14.07 ng/ml

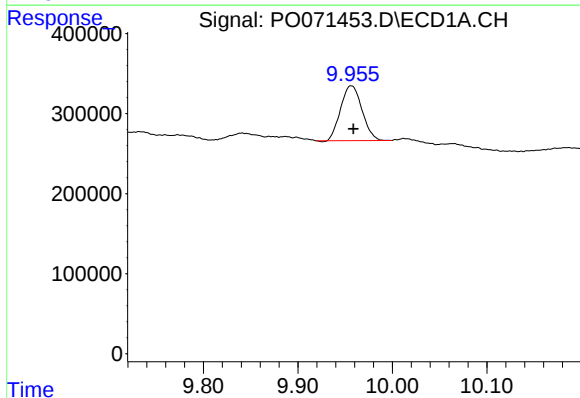

#2 Decachlorobiphenyl

R.T.: 9.957 min
Delta R.T.: -0.002 min
Response: 1078342
Conc: 11.56 ng/ml

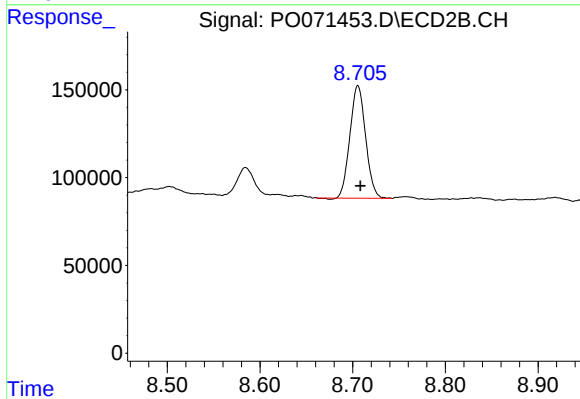

#2 Decachlorobiphenyl

R.T.: 8.706 min
Delta R.T.: -0.002 min
Response: 753051
Conc: 13.67 ng/ml