

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091820\
 Data File : P0071476.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Sep 2020 00:26
 Operator : DD\AJ
 Sample : L4074-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KTS-IB-0102-0-6

Manual Integrations
 APPROVED

Ankita
 9/21/2020 1:05:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 02:47:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.527	1808186	974299	25.515m	24.956
2) SA Decachlor...	9.956	8.706	2367199	1234406	25.384	22.409
Target Compounds						
31) L7 AR-1260-1	7.303	6.310	554890	362272	122.374	130.029
32) L7 AR-1260-2	7.571	6.511	800858	359209	114.878	99.373
33) L7 AR-1260-3	7.927	6.657	753147	355544	124.276	110.179
34) L7 AR-1260-4	8.154	7.133	668303	308406	116.747	106.462
35) L7 AR-1260-5	8.468	7.386	1373790	666349	108.339	87.878

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091820\
Data File : P0071476.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2020 00:26
Operator : DD\AJ
Sample : L4074-01
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
KTS-IB-0102-0-6


Manual Integrations
APPROVED

Ankita
9/21/2020 1:05:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 02:47:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

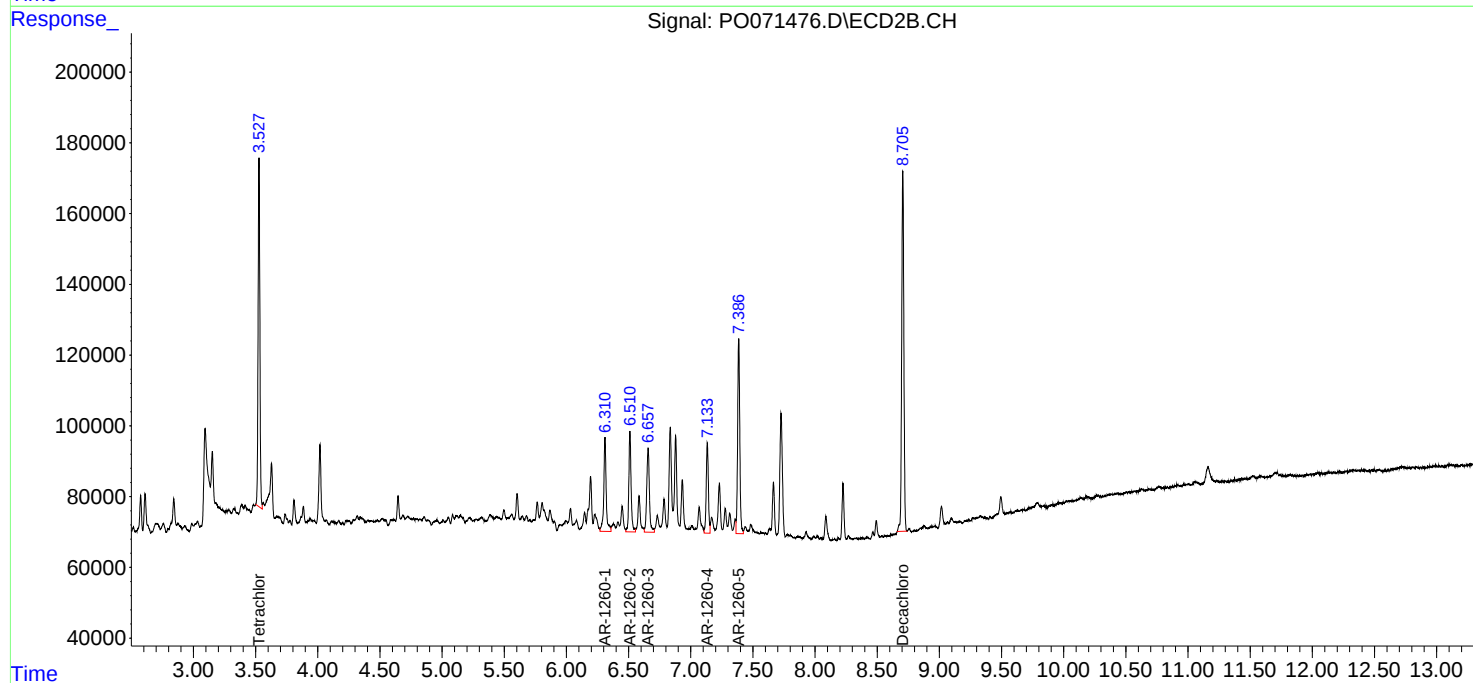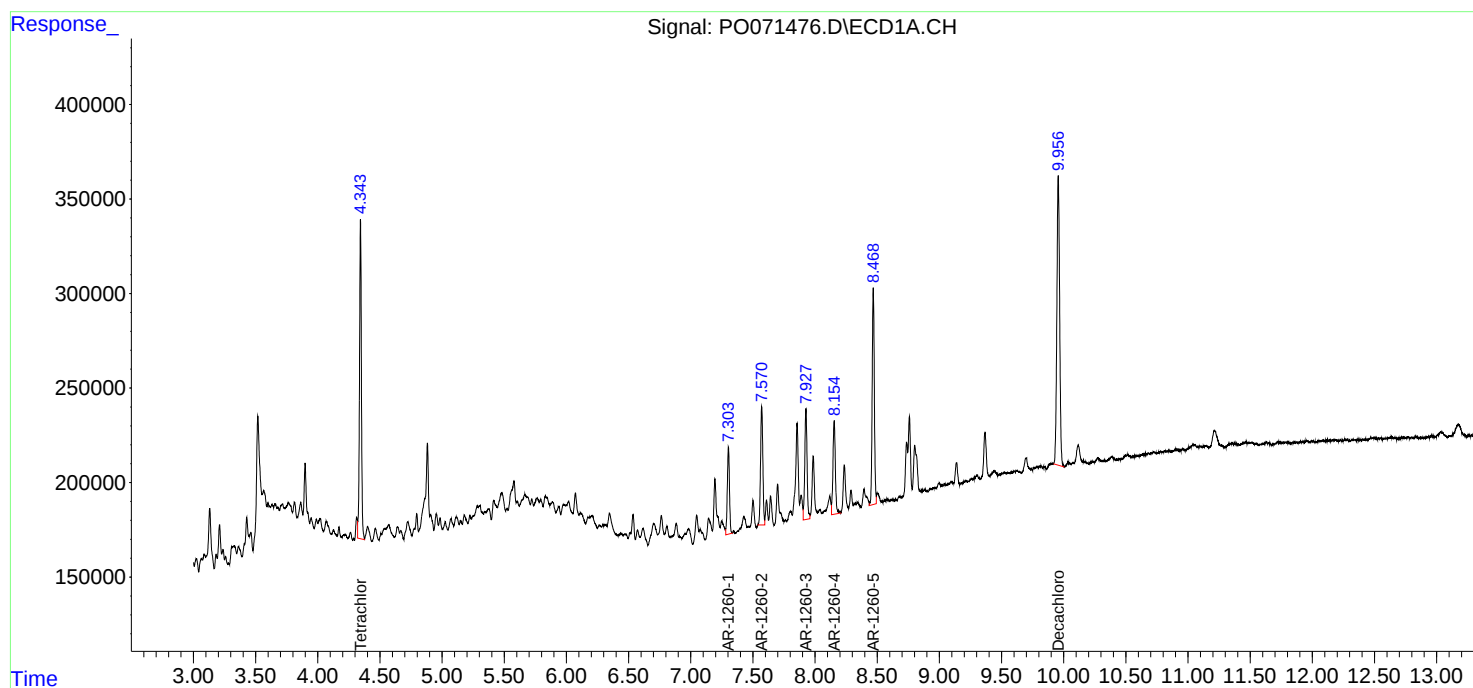

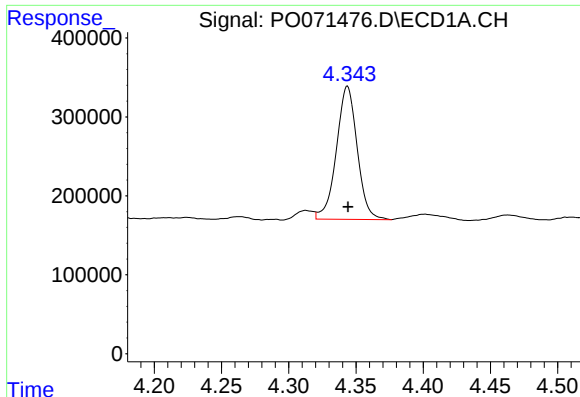


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 1808186
Conc: 25.52 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KTS-IB-0102-0-6


Manual Integrations
APPROVED

Ankita
9/21/2020 1:05:29 PM

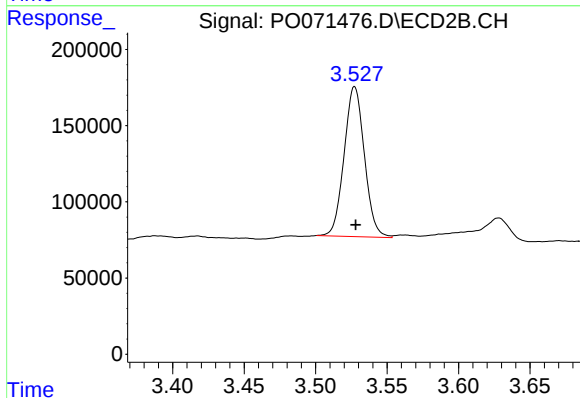


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 974299
Conc: 24.96 ng/ml

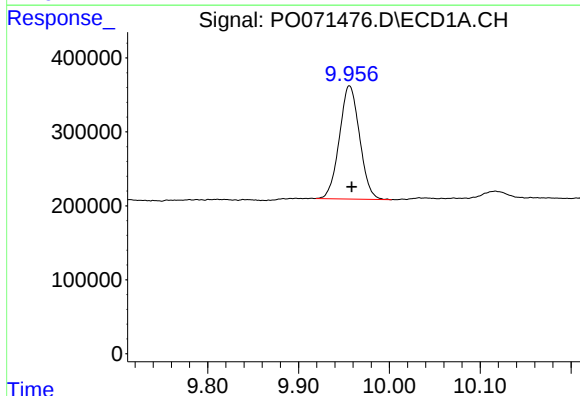


#2 Decachlorobiphenyl

R.T.: 9.956 min
Delta R.T.: -0.002 min
Response: 2367199
Conc: 25.38 ng/ml

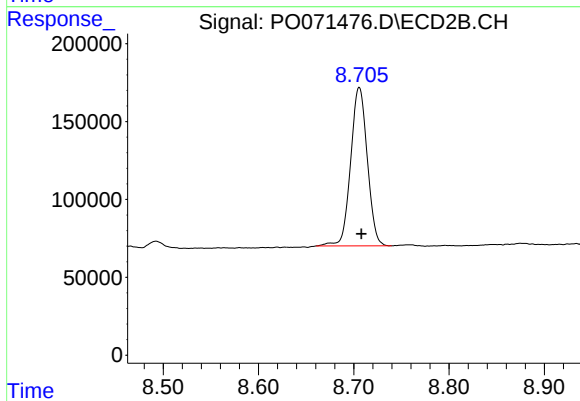

#2 Decachlorobiphenyl

R.T.: 8.706 min
Delta R.T.: -0.002 min
Response: 1234406
Conc: 22.41 ng/ml

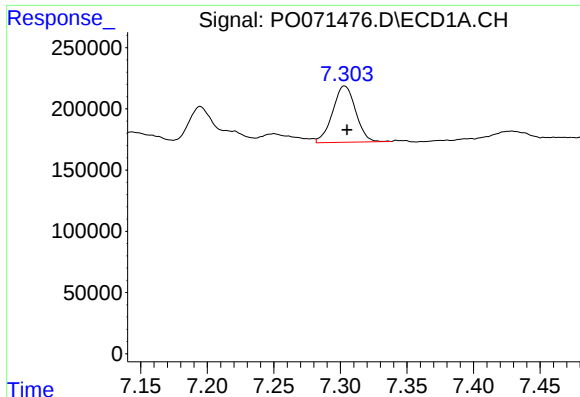


#31 AR-1260-1

R.T.: 7.303 min
Delta R.T.: -0.002 min
Response: 554890
Conc: 122.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
KTS-IB-0102-0-6


Manual Integrations
APPROVED

Ankita
9/21/2020 1:05:29 PM

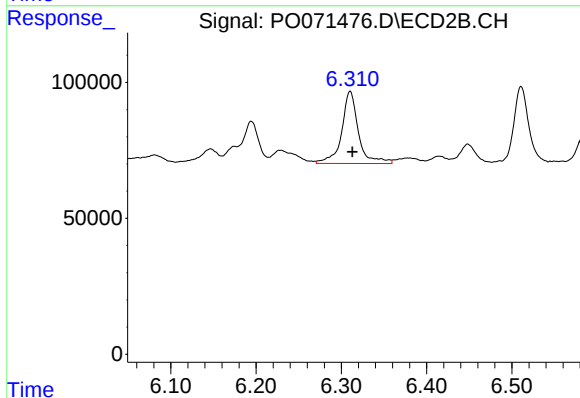


#31 AR-1260-1

R.T.: 6.310 min
Delta R.T.: -0.003 min
Response: 362272
Conc: 130.03 ng/ml

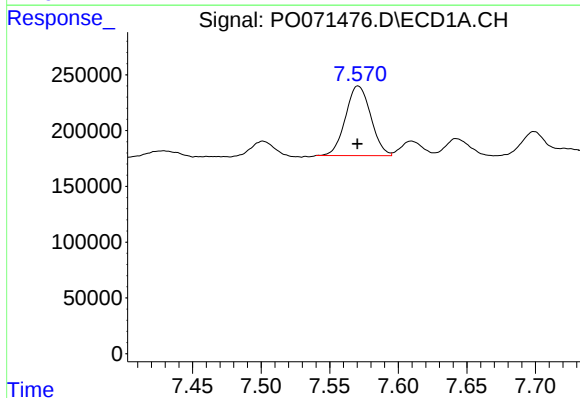


#32 AR-1260-2

R.T.: 7.571 min
Delta R.T.: 0.000 min
Response: 800858
Conc: 114.88 ng/ml

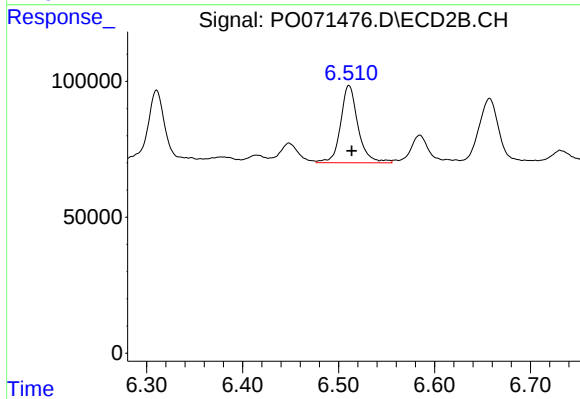

#32 AR-1260-2

R.T.: 6.511 min
Delta R.T.: -0.003 min
Response: 359209
Conc: 99.37 ng/ml

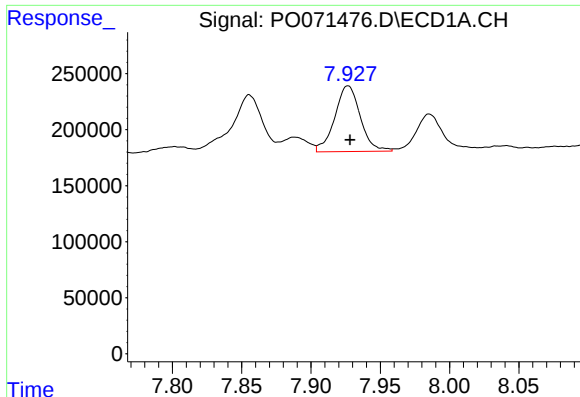


#33 AR-1260-3

R.T.: 7.927 min
Delta R.T.: -0.002 min
Response: 753147
Conc: 124.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
KTS-IB-0102-0-6


Manual Integrations
APPROVED

Ankita
9/21/2020 1:05:29 PM

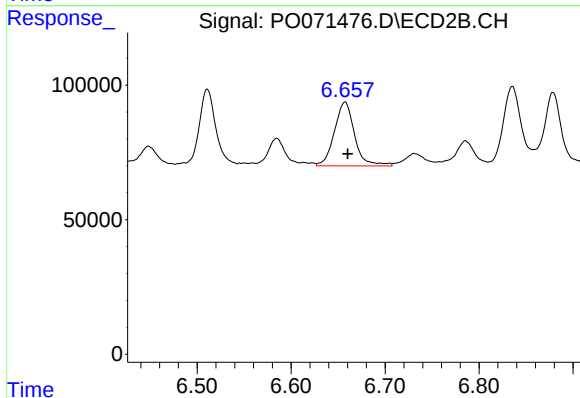


#33 AR-1260-3

R.T.: 6.657 min
Delta R.T.: -0.003 min
Response: 355544
Conc: 110.18 ng/ml

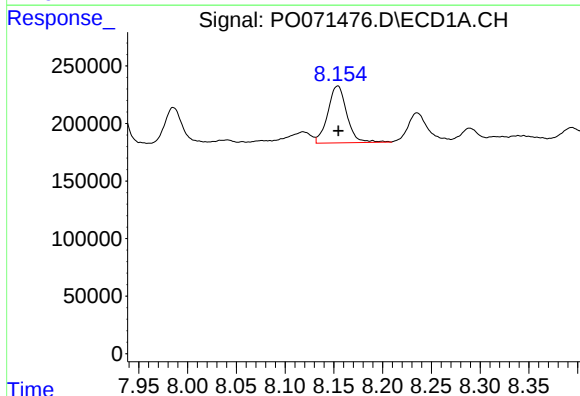


#34 AR-1260-4

R.T.: 8.154 min
Delta R.T.: 0.000 min
Response: 668303
Conc: 116.75 ng/ml

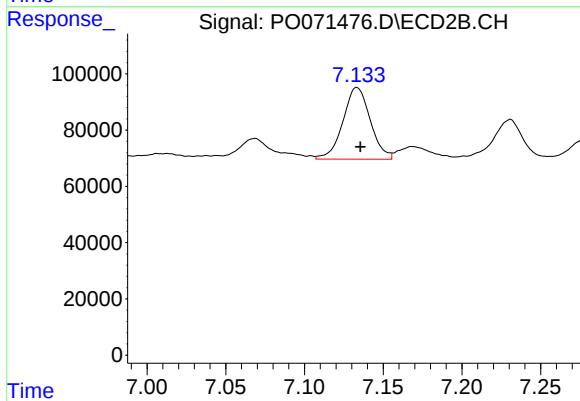

#34 AR-1260-4

R.T.: 7.133 min
Delta R.T.: -0.002 min
Response: 308406
Conc: 106.46 ng/ml

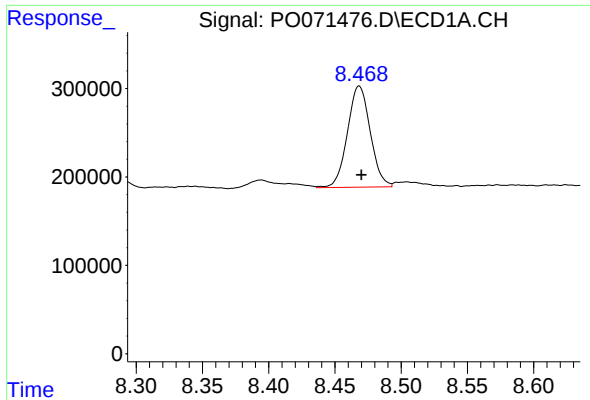


#35 AR-1260-5

R.T.: 8.468 min
Delta R.T.: -0.002 min
Response: 1373790
Conc: 108.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
KTS-IB-0102-0-6

Manual Integrations
APPROVED

Ankita
9/21/2020 1:05:29 PM

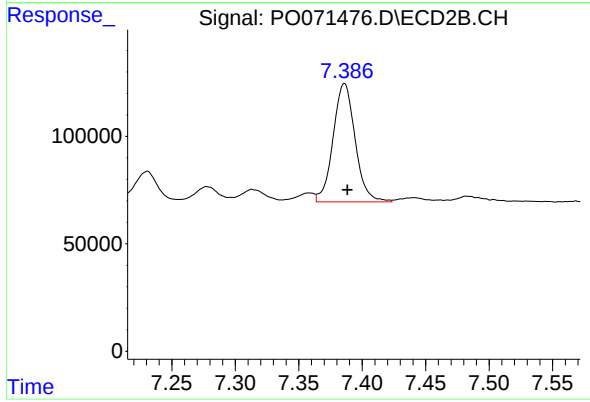

#35 AR-1260-5

R.T.: 7.386 min
Delta R.T.: -0.002 min
Response: 666349
Conc: 87.88 ng/ml