

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091823\
 Data File : P0098126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 04:08
 Operator : YP/AJ
 Sample : 04413-04 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMA915W-END-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 04:49:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 02:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.501	3.614	3686345	1568146	1.254	1.080
2) SA Decachlor...	10.348	8.641	2552430	1070241	1.488	1.090 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091823\
Data File : PO098126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 04:08
Operator : YP/AJ
Sample : 04413-04 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
KMA915W-END-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 04:49:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 02:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

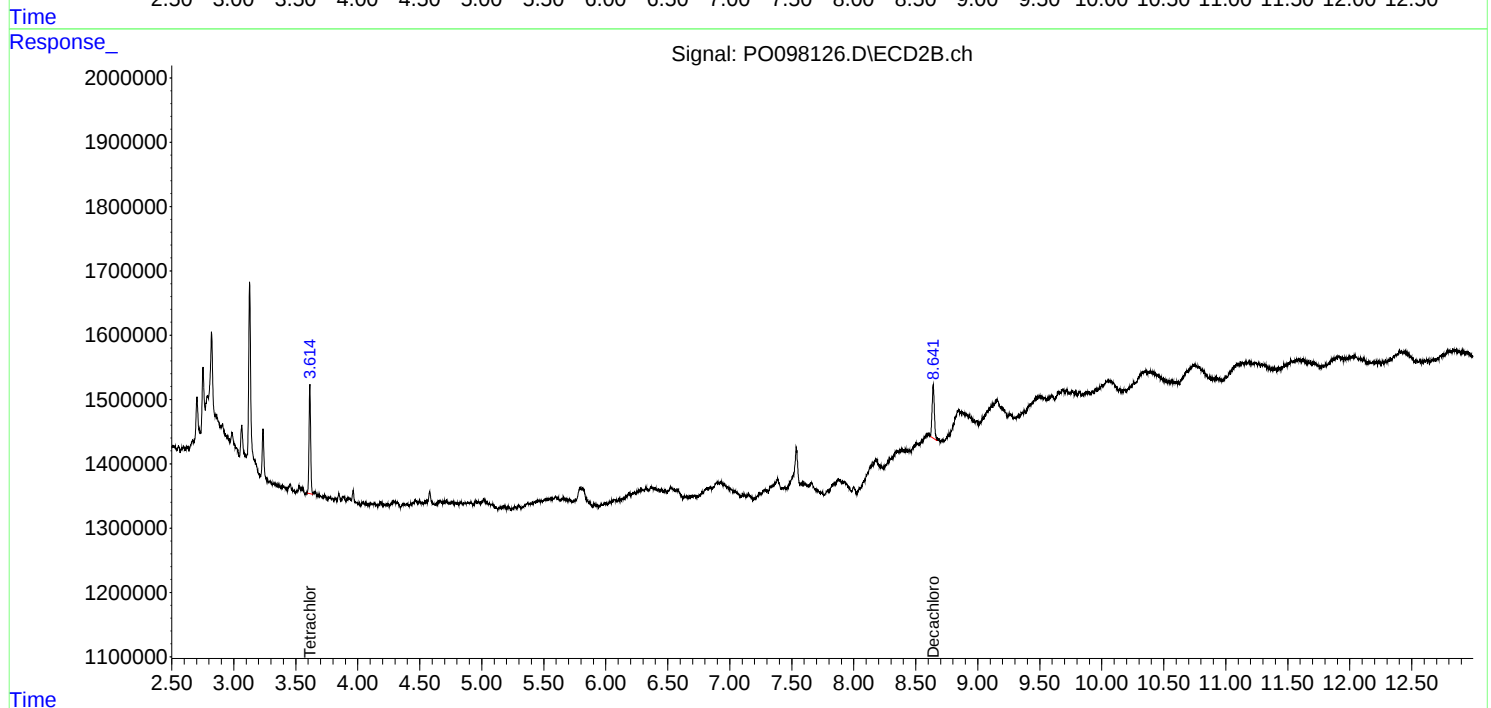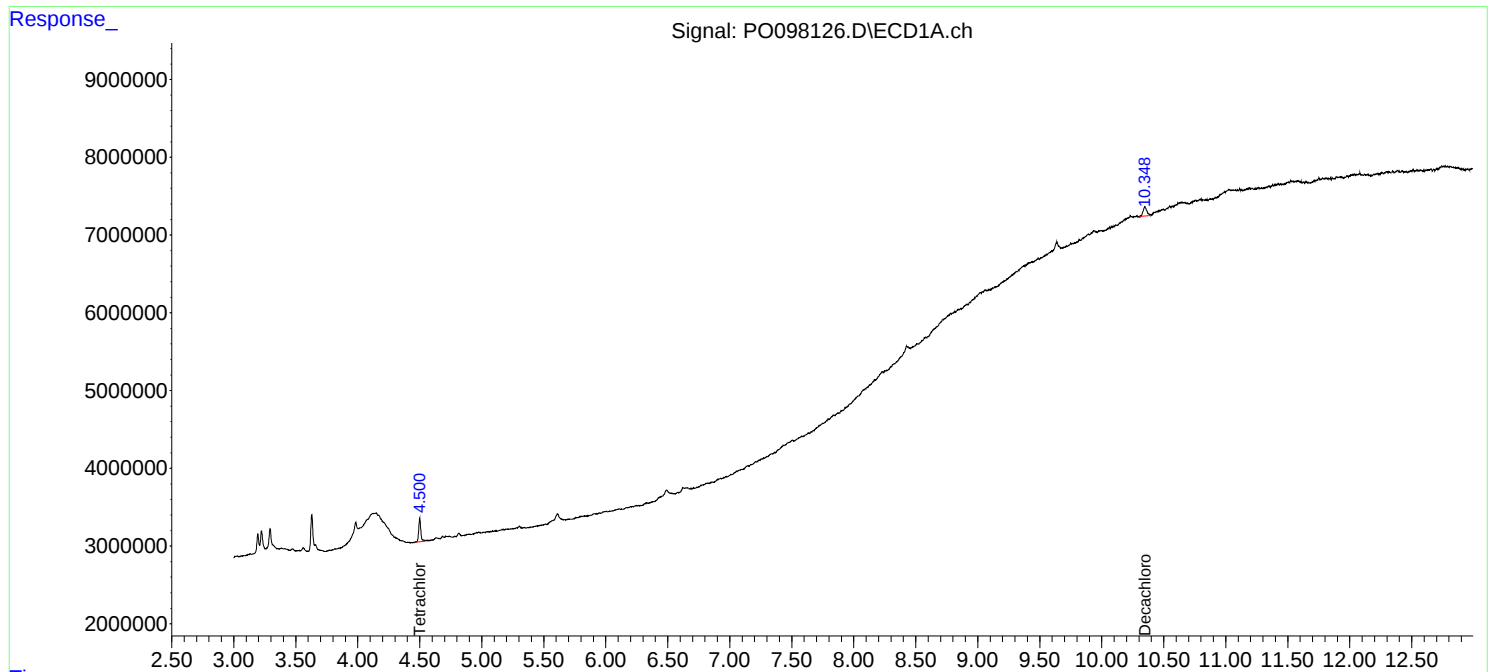


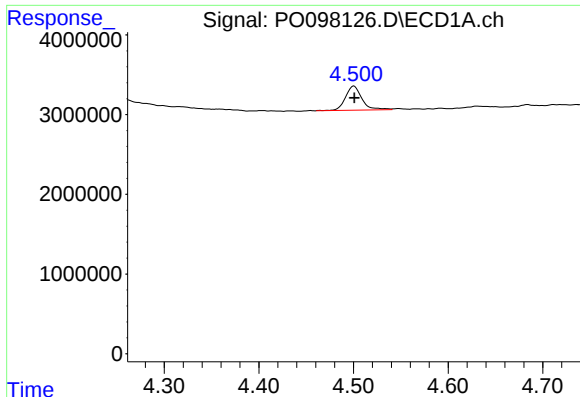

#1 Tetrachloro-m-xylene


R.T.: 4.501 min
Delta R.T.: 0.000 min
Response: 3686345
Conc: 1.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMA915W-END-1-2

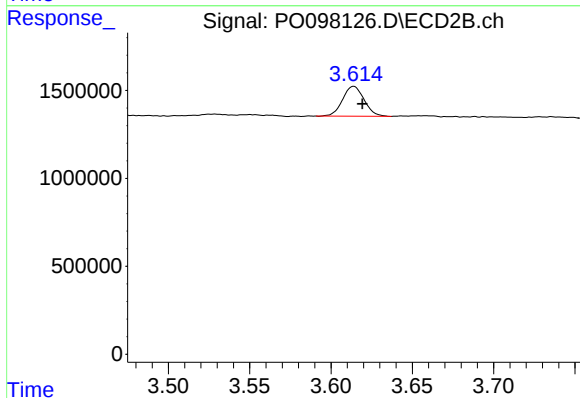


#1 Tetrachloro-m-xylene

R.T.: 3.614 min
Delta R.T.: -0.005 min
Response: 1568146
Conc: 1.08 ng/ml

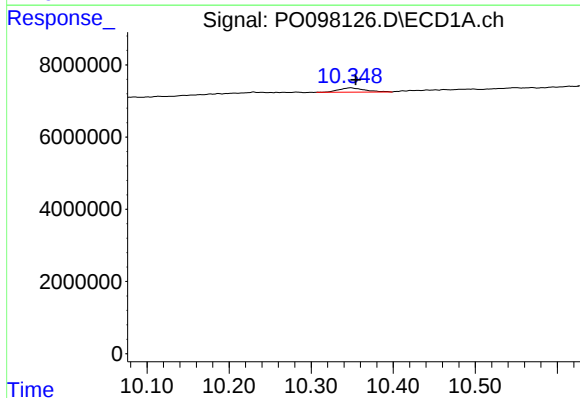

#2 Decachlorobiphenyl

R.T.: 10.348 min
Delta R.T.: -0.006 min
Response: 2552430
Conc: 1.49 ng/ml

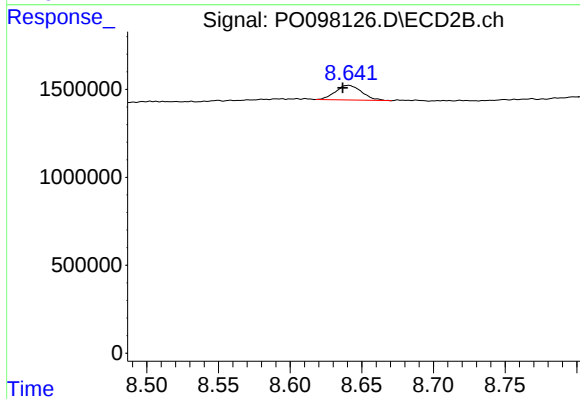

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.004 min
Response: 1070241
Conc: 1.09 ng/ml