

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091823\
 Data File : P0098127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 04:25
 Operator : YP/AJ
 Sample : 04413-05 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMA382K-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/19/2023
 Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 04:49:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 02:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.499	3.614	4993671	2502001	1.698m	1.722m
2) SA Decachlor...	10.354	8.647	3097789	1181328	1.806	1.203m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091823\
Data File : PO098127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 04:25
Operator : YP/AJ
Sample : 04413-05 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMA382K-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2023
Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 04:49:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 02:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

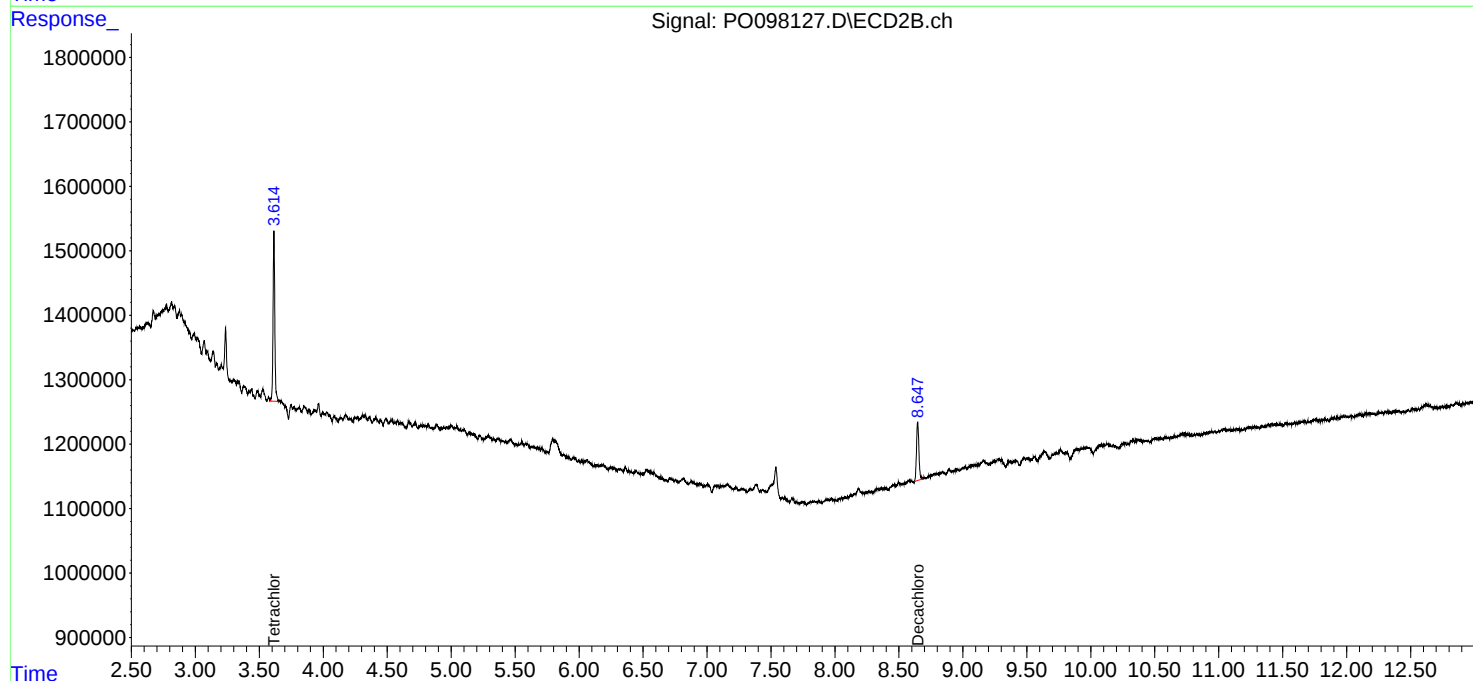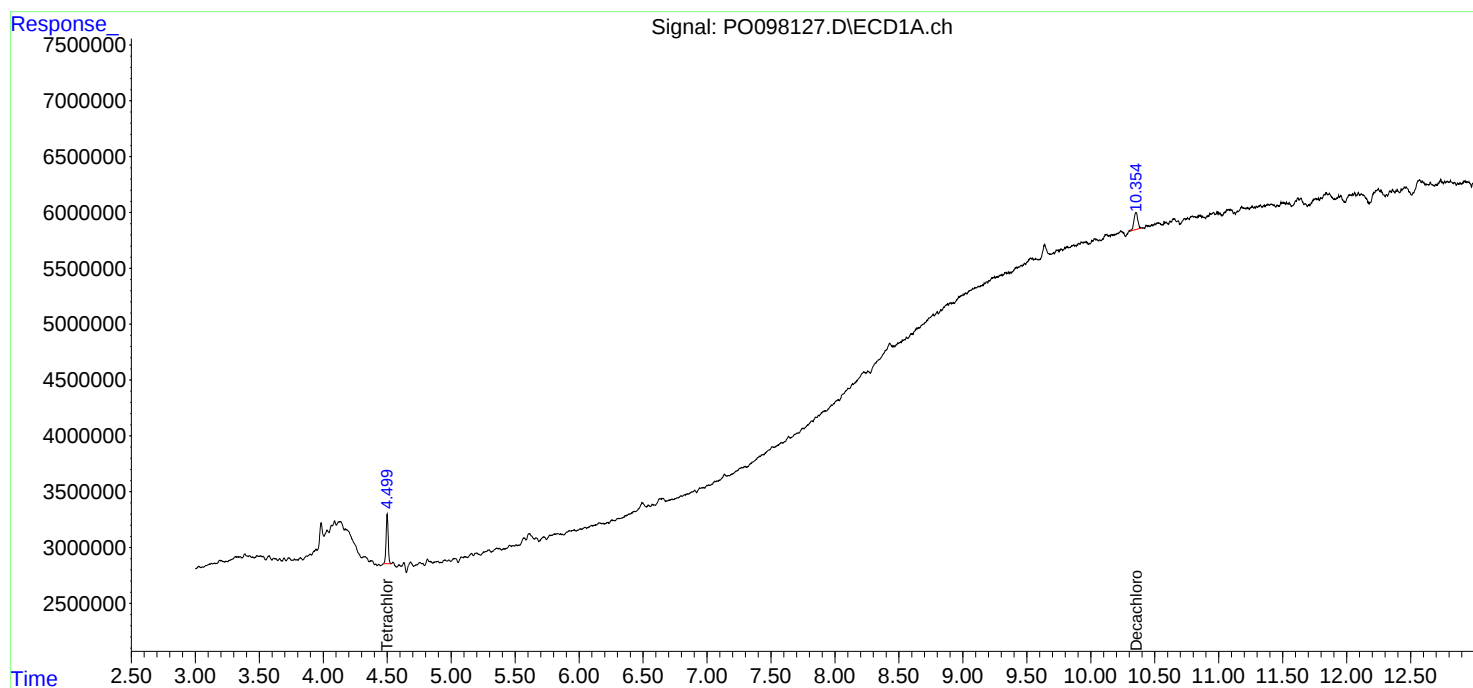

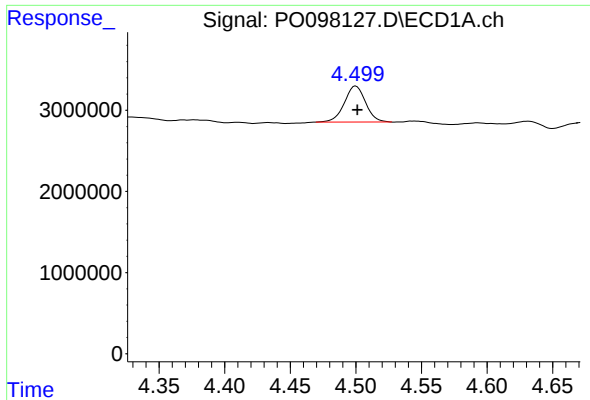


#1 Tetrachloro-m-xylene

R.T.: 4.499 min
Delta R.T.: -0.002 min
Response: 4993671
Conc: 1.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMA382K-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2023
Supervised By :Ankita Jodhani 09/19/2023

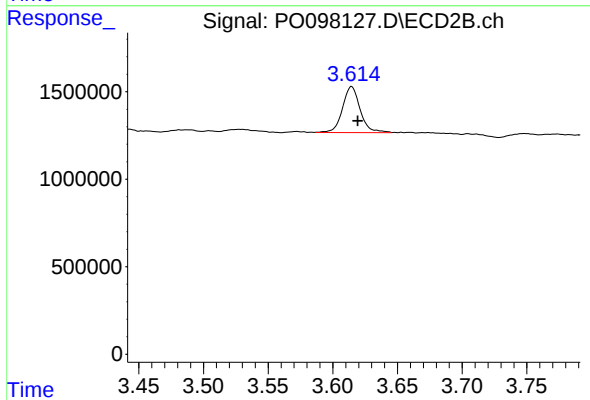


#1 Tetrachloro-m-xylene

R.T.: 3.614 min
Delta R.T.: -0.005 min
Response: 2502001
Conc: 1.72 ng/ml m

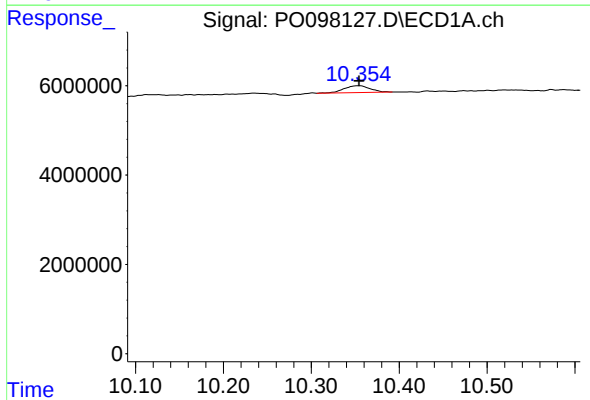

#2 Decachlorobiphenyl

R.T.: 10.354 min
Delta R.T.: 0.000 min
Response: 3097789
Conc: 1.81 ng/ml

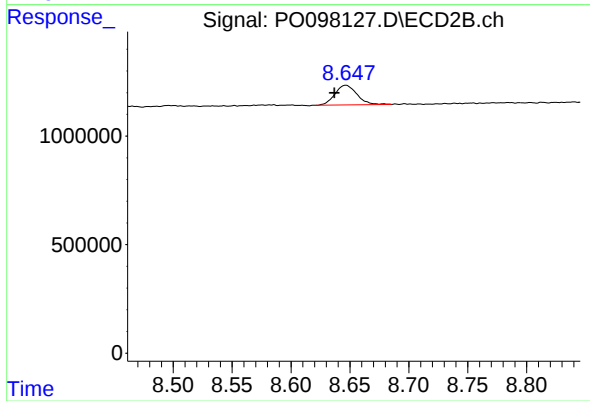

#2 Decachlorobiphenyl

R.T.: 8.647 min
Delta R.T.: 0.010 min
Response: 1181328
Conc: 1.20 ng/ml m