

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091823\
 Data File : P0098128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 04:42
 Operator : YP/AJ
 Sample : 04413-06 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMA382K-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/19/2023
 Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:48:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 02:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.500	3.614	4087235	2065928	1.390m	1.422m
2) SA Decachlor...	10.352	8.645	3323162	1242290	1.938	1.265m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091823\
Data File : PO098128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 04:42
Operator : YP/AJ
Sample : 04413-06 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMA382K-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2023
Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:48:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 02:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

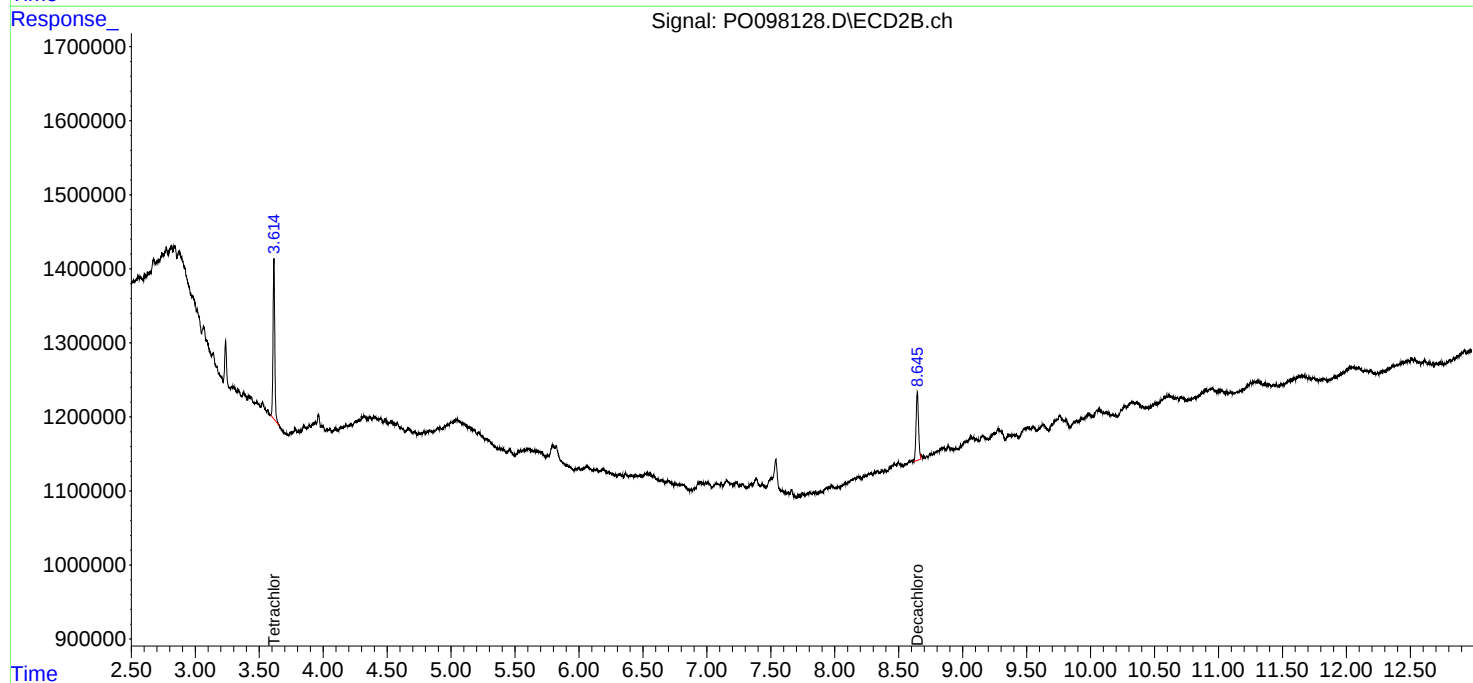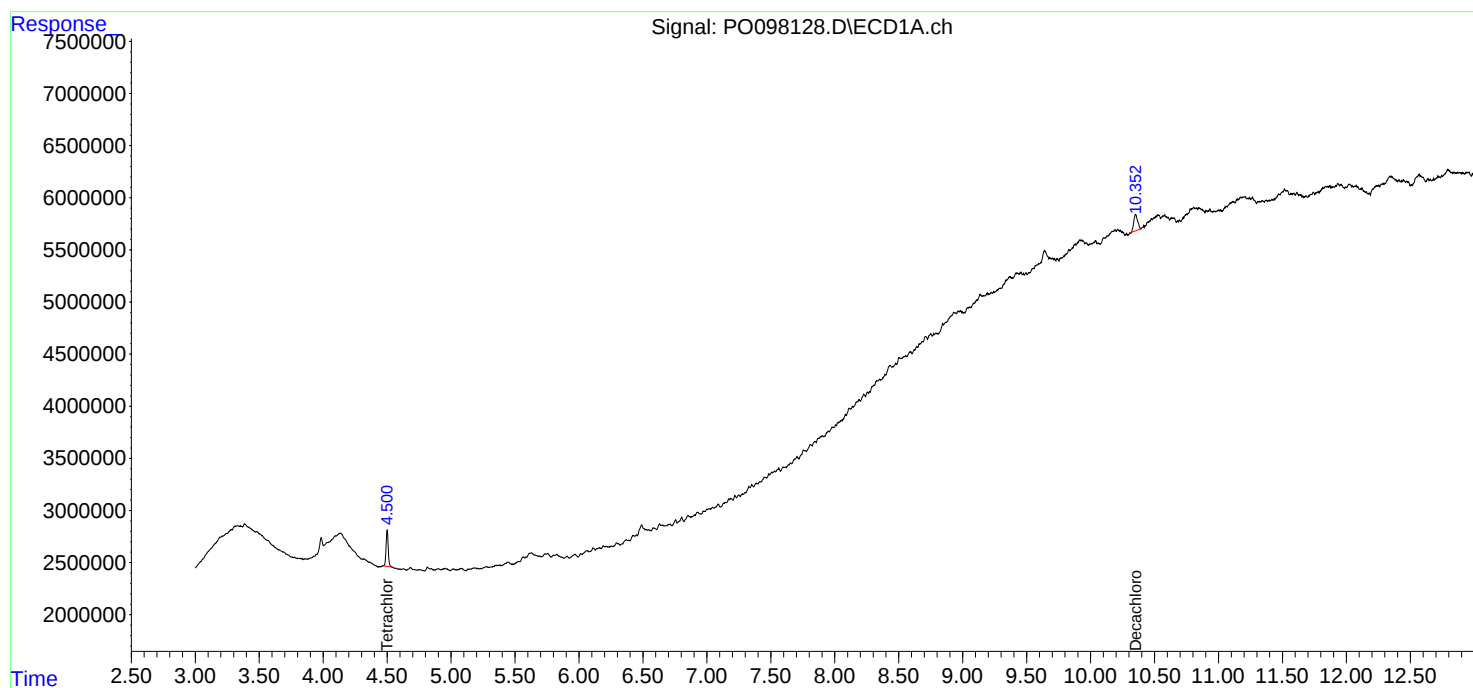

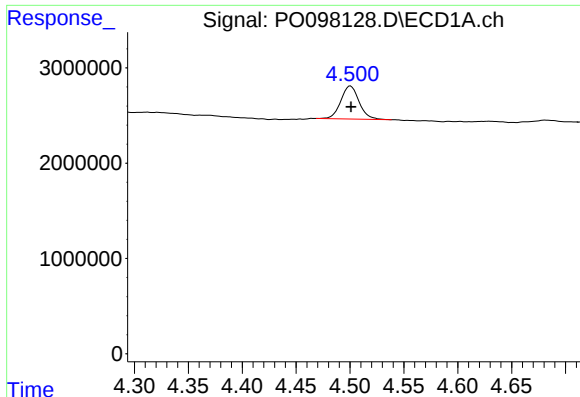


#1 Tetrachloro-m-xylene

R.T.: 4.500 min
Delta R.T.: -0.001 min
Response: 4087235
Conc: 1.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMA382K-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2023
Supervised By :Ankita Jodhani 09/19/2023

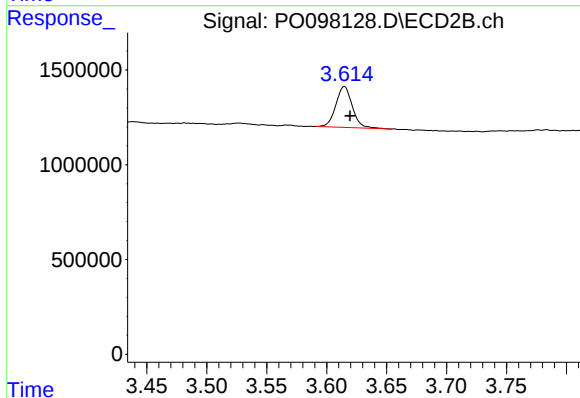


#1 Tetrachloro-m-xylene

R.T.: 3.614 min
Delta R.T.: -0.005 min
Response: 2065928
Conc: 1.42 ng/ml m

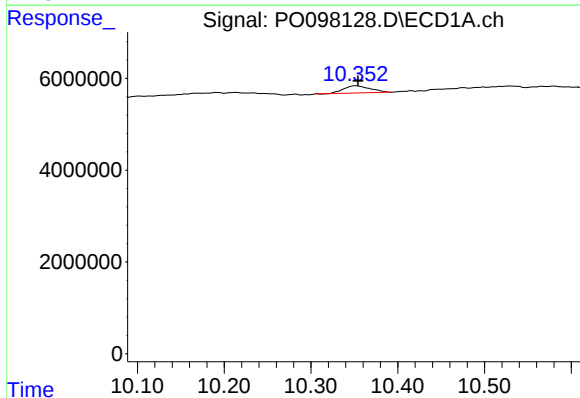

#2 Decachlorobiphenyl

R.T.: 10.352 min
Delta R.T.: -0.003 min
Response: 3323162
Conc: 1.94 ng/ml

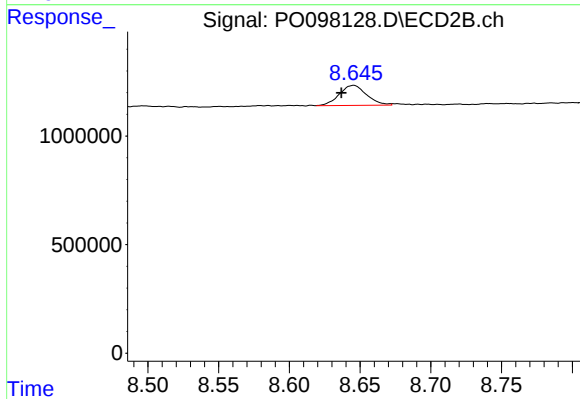

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: 0.008 min
Response: 1242290
Conc: 1.26 ng/ml m