

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091823\
 Data File : P0098132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 13:02
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/19/2023
 Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 13:25:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 02:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.501	3.617	57127656	26180157	19.428	18.024
2) SA Decachlor...	10.353	8.652	34712520	17662570	20.242	17.981m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO091823\
Data File : PO098132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 13:02
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2023
Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 13:25:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 02:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

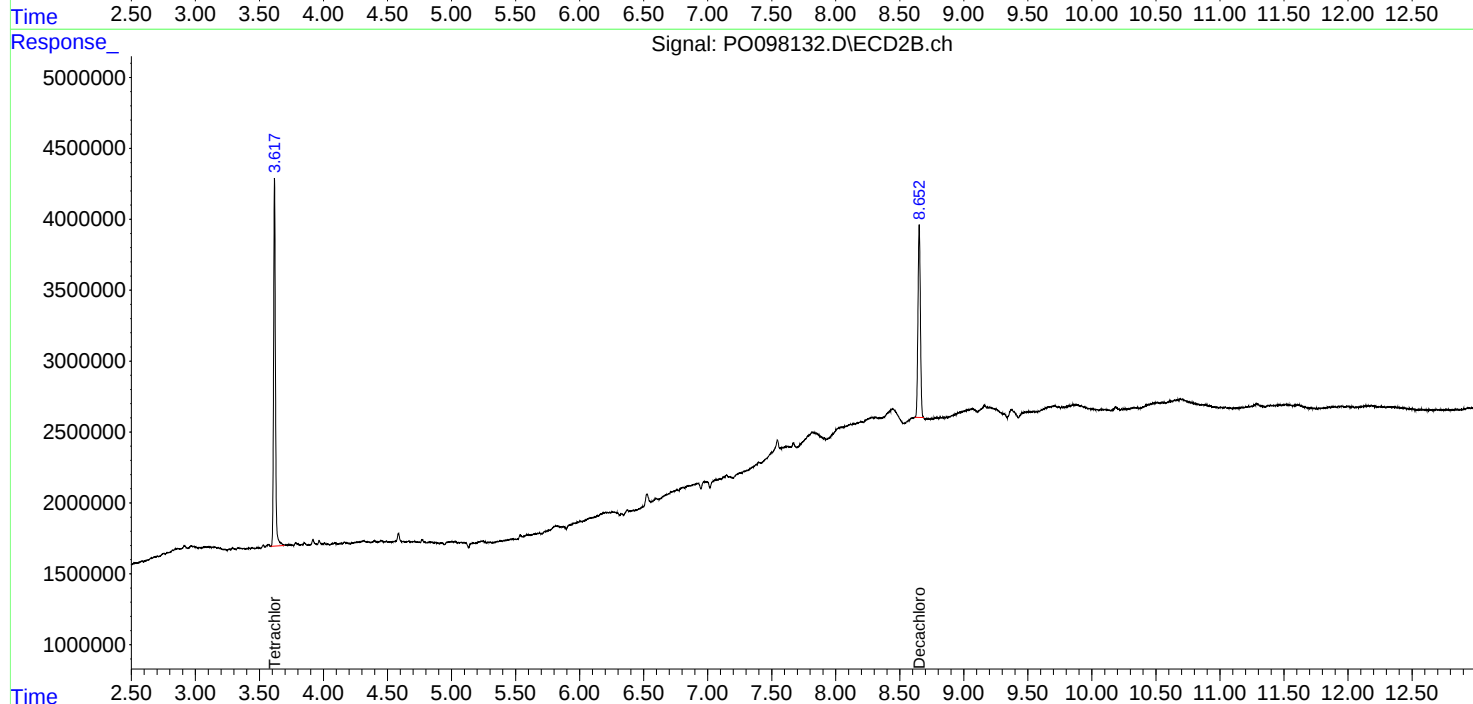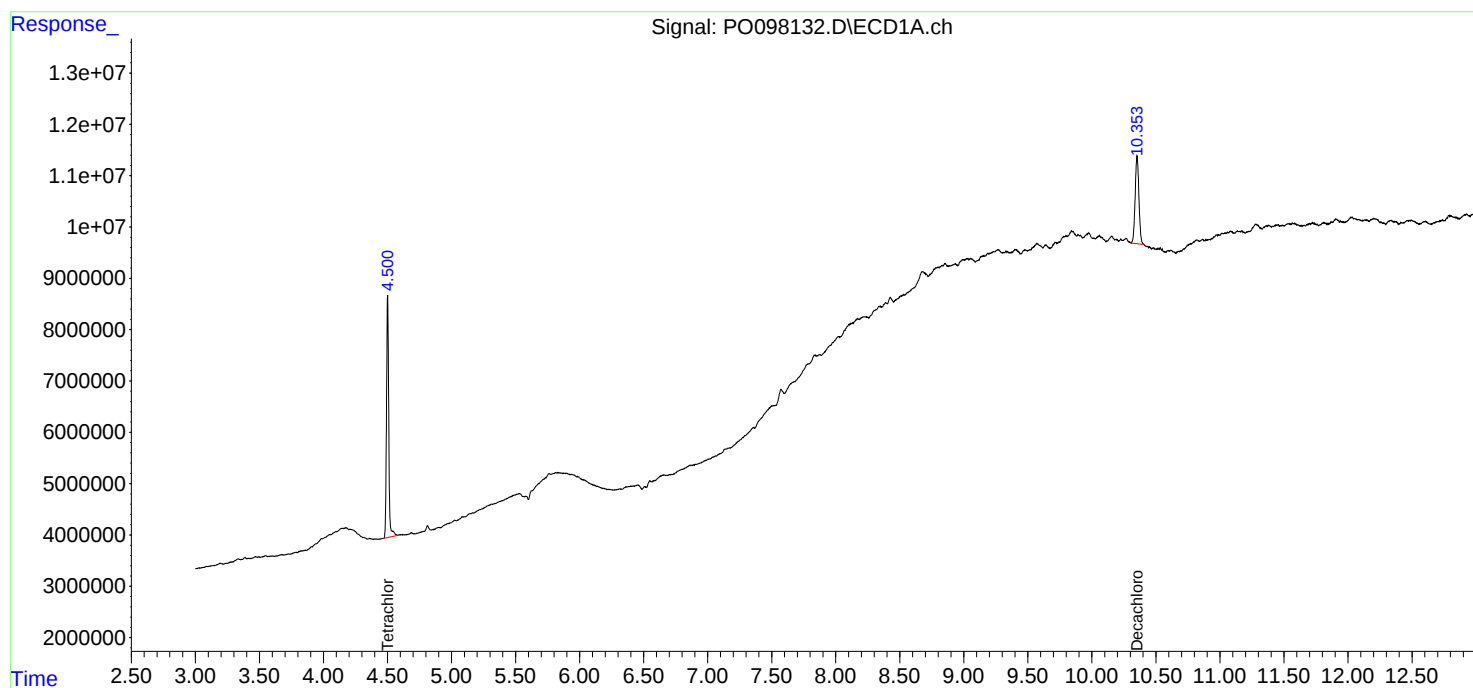

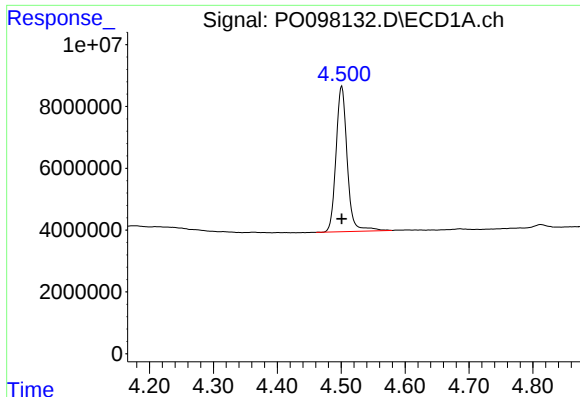


#1 Tetrachloro-m-xylene

R.T.: 4.501 min
Delta R.T.: 0.000 min
Response: 57127656
Conc: 19.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2023
Supervised By :Ankita Jodhani 09/19/2023

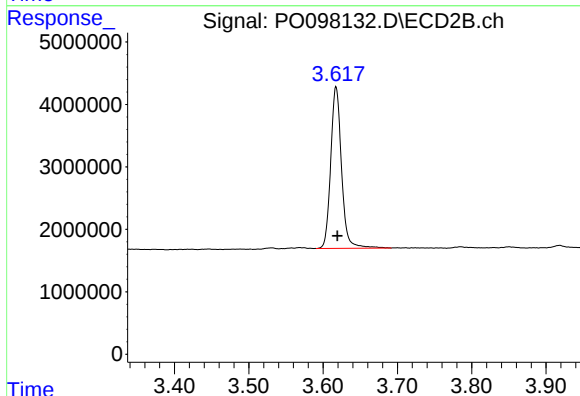


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.002 min
Response: 26180157
Conc: 18.02 ng/ml

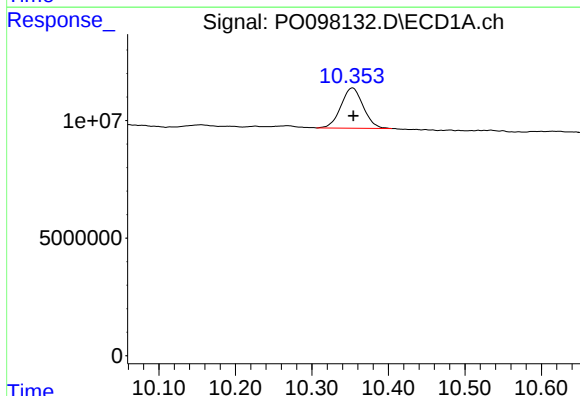

#2 Decachlorobiphenyl

R.T.: 10.353 min
Delta R.T.: -0.001 min
Response: 34712520
Conc: 20.24 ng/ml

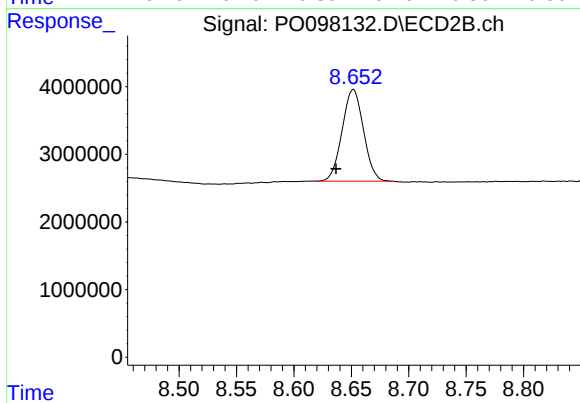

#2 Decachlorobiphenyl

R.T.: 8.652 min
Delta R.T.: 0.015 min
Response: 17662570
Conc: 17.98 ng/ml m