

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091824\
 Data File : P0106647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 19:19
 Operator : YP/AJ
 Sample : P4088-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-614-COMP-07

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/19/2024
 Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 07:40:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.713	156.8E6	48454186	20.909m	18.139
2) SA Decachlor...	10.195	8.737	79116122	34832572	16.006	17.414m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091824\
Data File : PO106647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 19:19
Operator : YP/AJ
Sample : P4088-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NB-614-COMP-07


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2024
Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 07:40:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

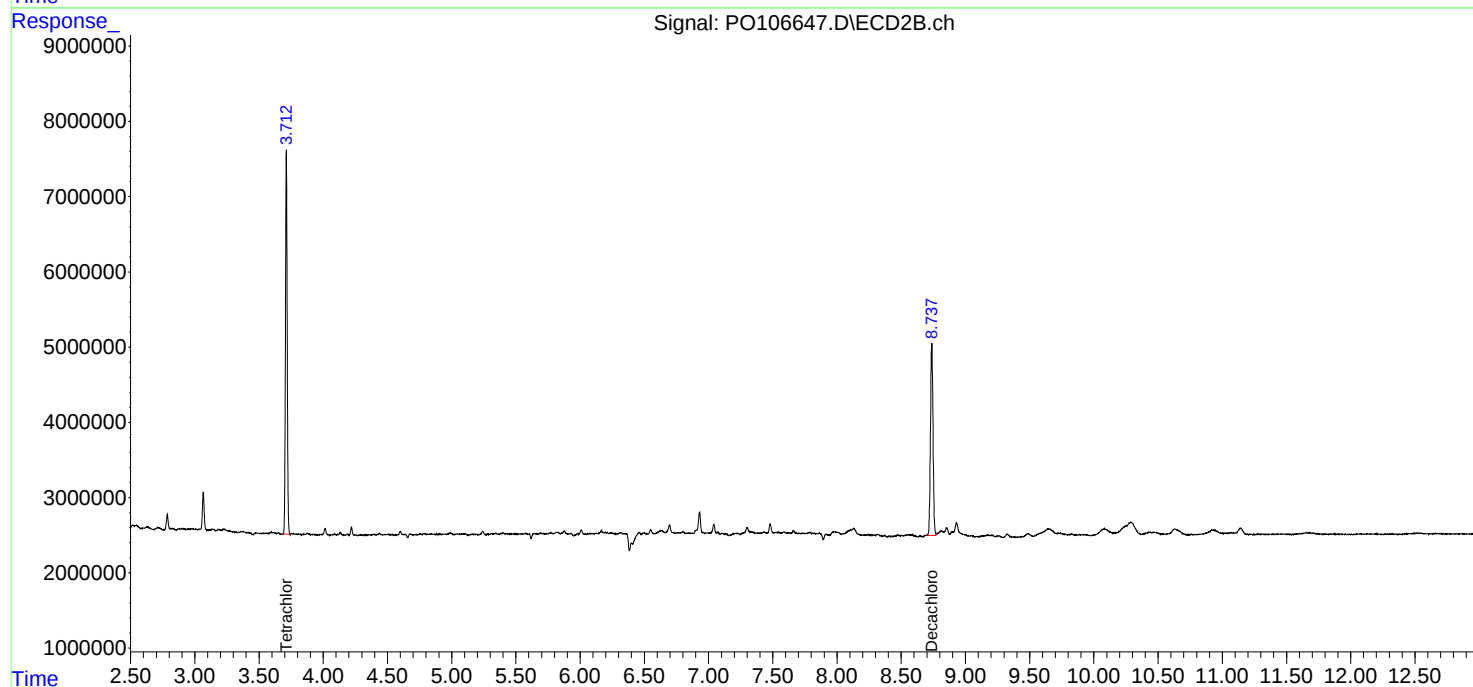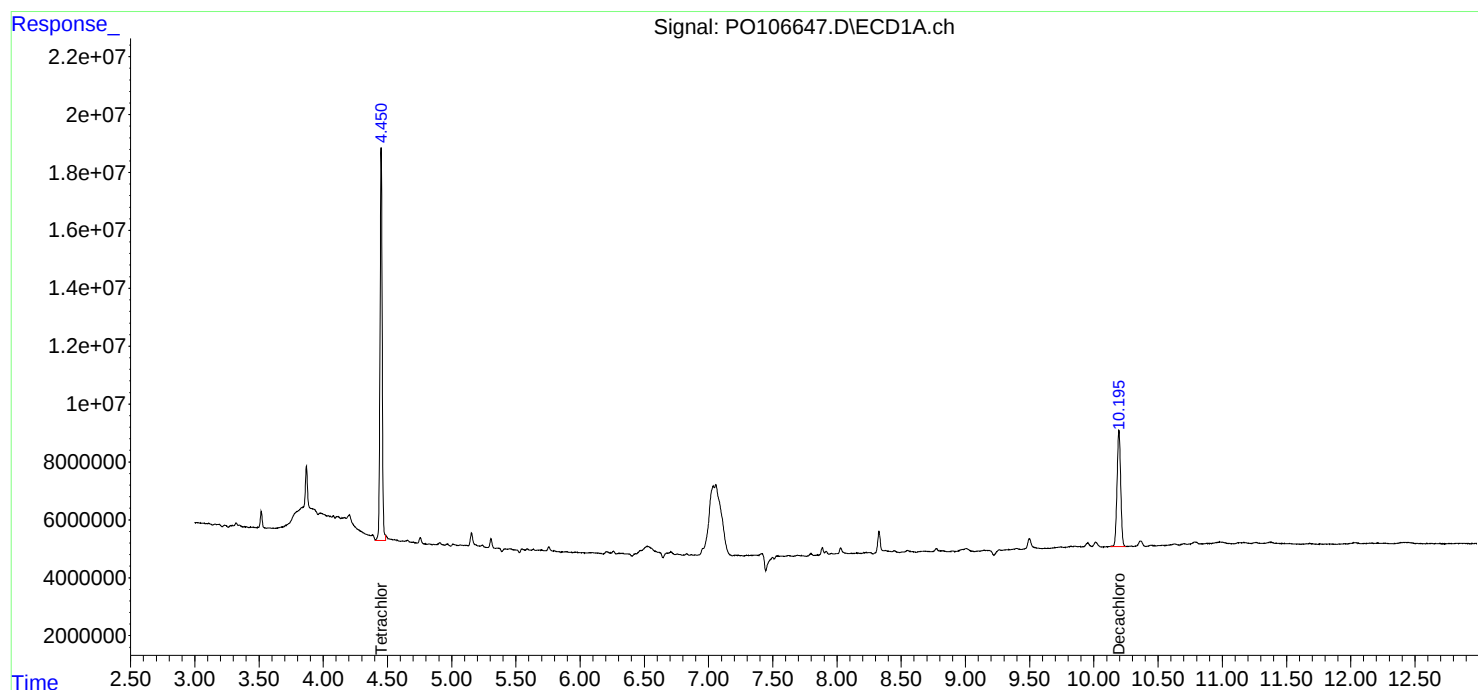

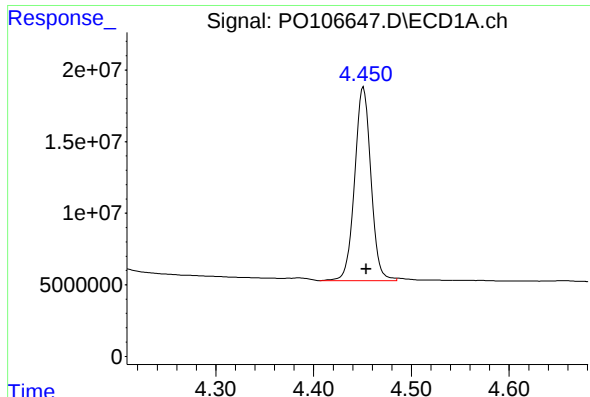


#1 Tetrachloro-m-xylene

R.T.: 4.450 min
Delta R.T.: -0.004 min
Response: 156844384
Conc: 20.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-614-COMP-07


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2024
Supervised By :Ankita Jodhani 09/19/2024

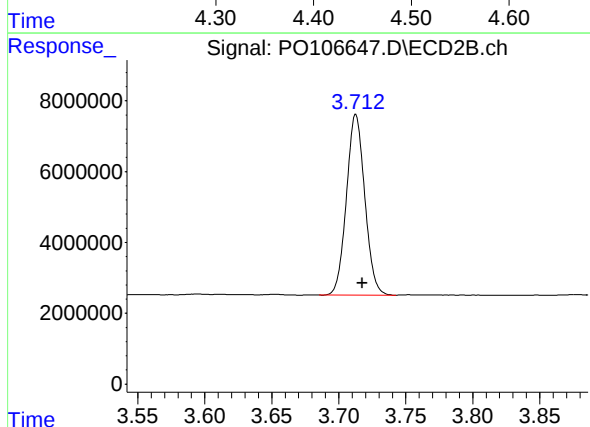


#1 Tetrachloro-m-xylene

R.T.: 3.713 min
Delta R.T.: -0.005 min
Response: 48454186
Conc: 18.14 ng/ml

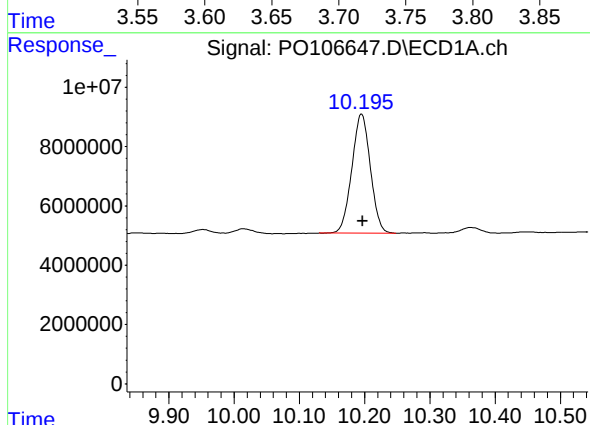

#2 Decachlorobiphenyl

R.T.: 10.195 min
Delta R.T.: -0.002 min
Response: 79116122
Conc: 16.01 ng/ml

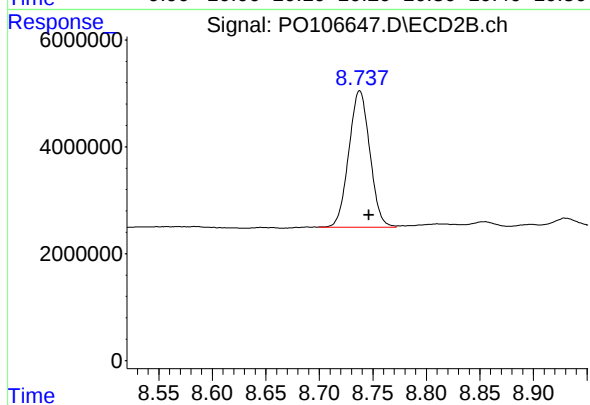

#2 Decachlorobiphenyl

R.T.: 8.737 min
Delta R.T.: -0.009 min
Response: 34832572
Conc: 17.41 ng/ml m