

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091824\
 Data File : P0106668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2024 02:35
 Operator : YP/AJ
 Sample : P4030-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-A-08-202409

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/19/2024
 Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 07:57:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.452	3.714	164.3E6	57449360	21.908m	21.507m
2) SA Decachlor...	10.198	8.738	100.3E6	40227290	20.286	20.111

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091824\
Data File : PO106668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2024 02:35
Operator : YP/AJ
Sample : P4030-02
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-A-08-202409


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2024
Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 07:57:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

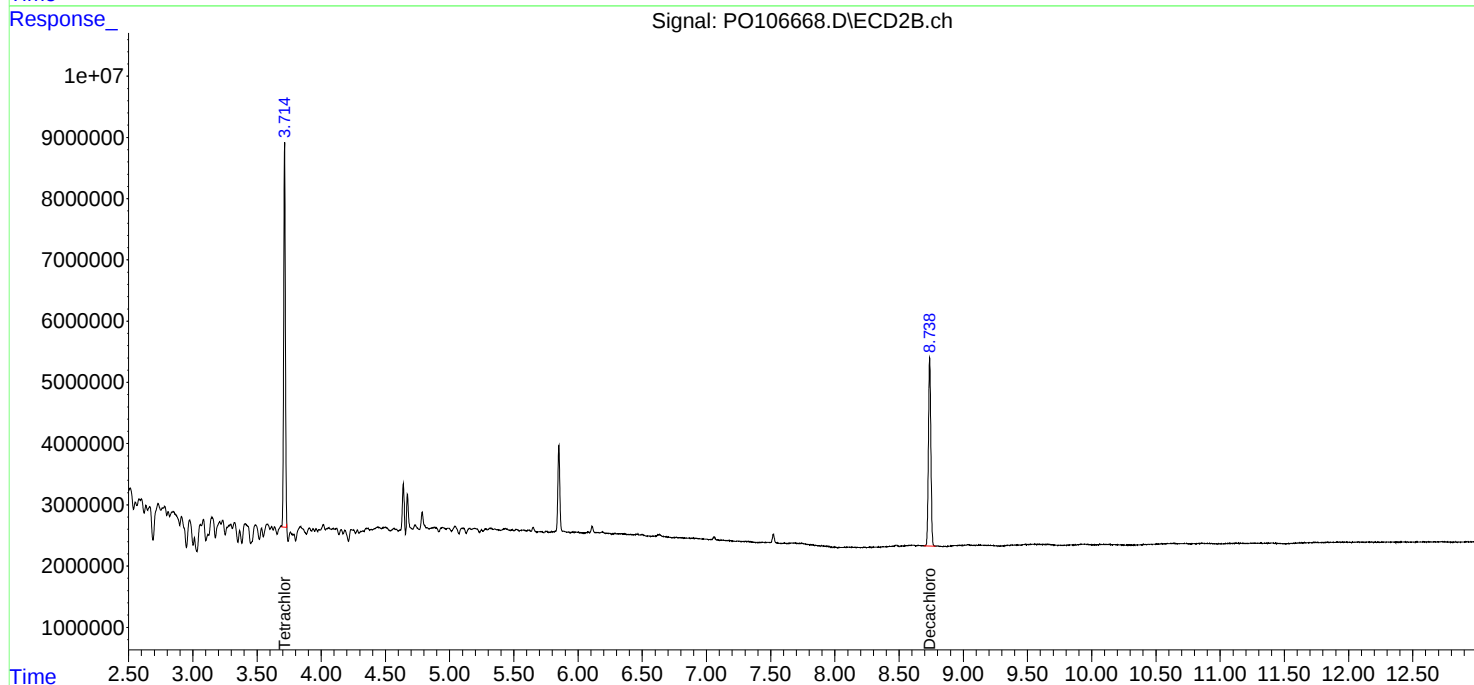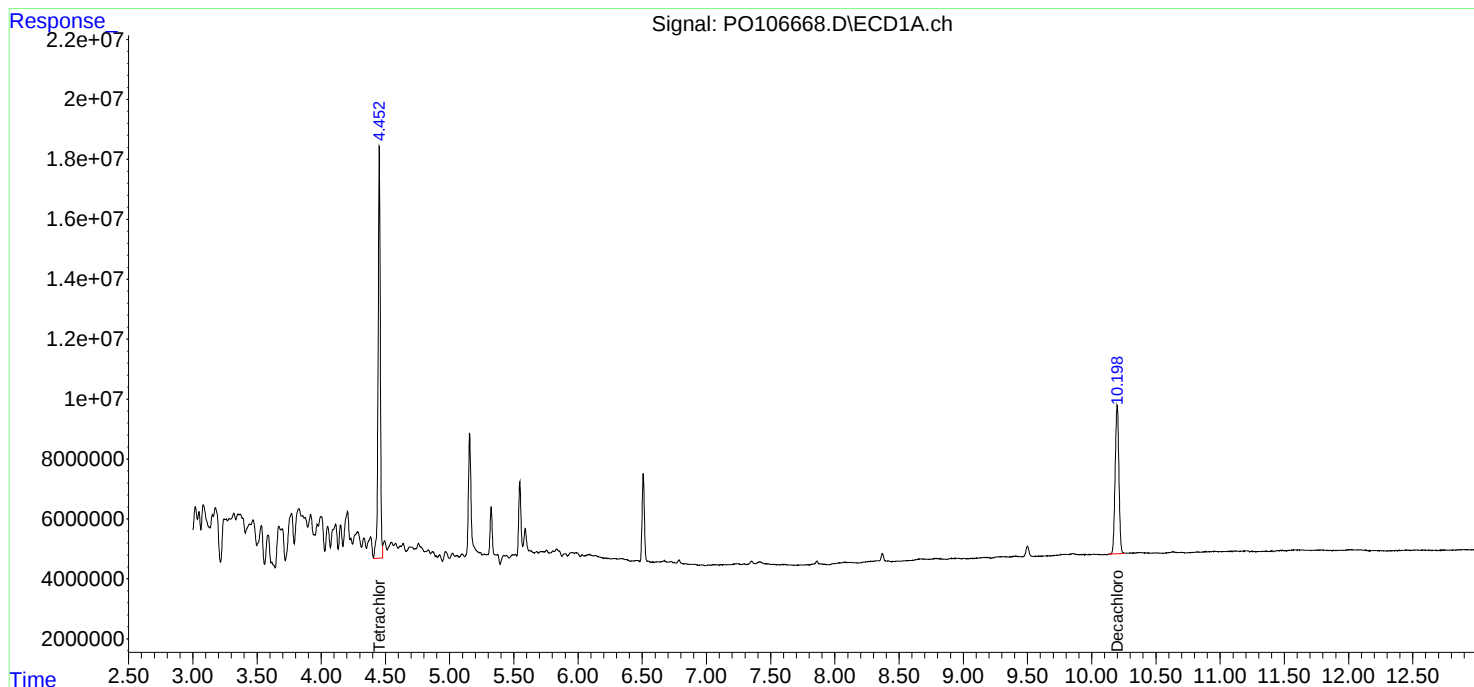

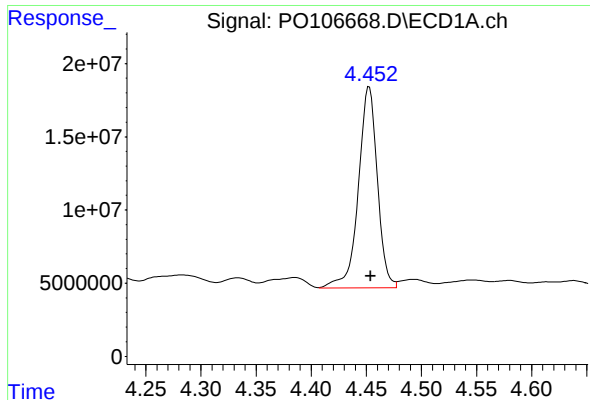


#1 Tetrachloro-m-xylene

R.T.: 4.452 min
Delta R.T.: -0.002 min
Response: 164340625
Conc: 21.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-A-08-202409


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2024
Supervised By :Ankita Jodhani 09/19/2024

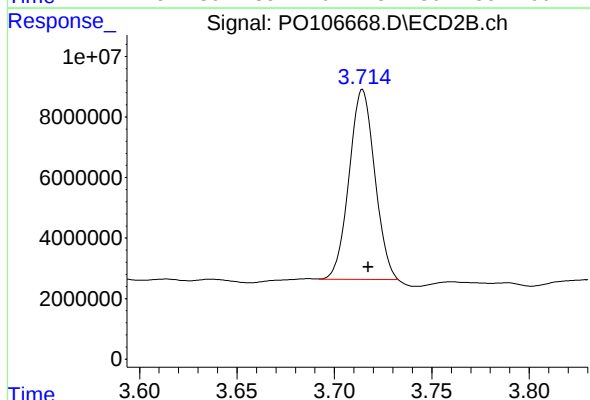


#1 Tetrachloro-m-xylene

R.T.: 3.714 min
Delta R.T.: -0.003 min
Response: 57449360
Conc: 21.51 ng/ml

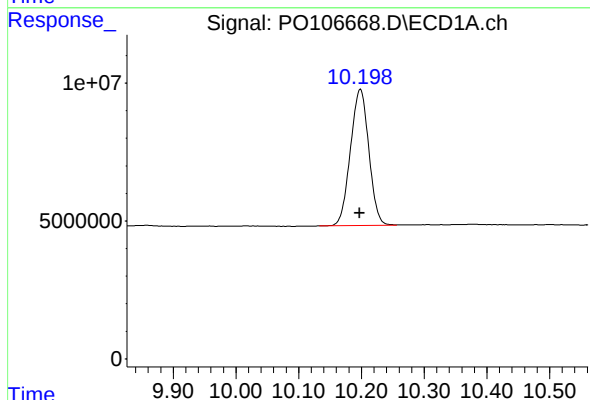

#2 Decachlorobiphenyl

R.T.: 10.198 min
Delta R.T.: 0.001 min
Response: 100271154
Conc: 20.29 ng/ml

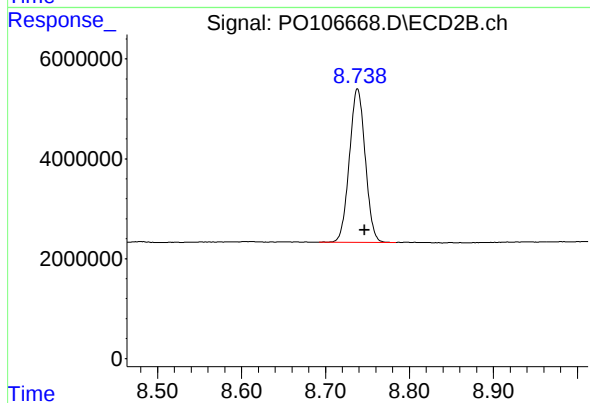

#2 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: -0.008 min
Response: 40227290
Conc: 20.11 ng/ml